




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013297.D
Acq On : 24 Dec 2022 13:34
Operator : CG/JU
Sample : N6016-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYC1

Manual IntegrationsAPPROVED

Quant Time: Dec 25 00:20:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/25/2022
Supervised By :Yogesh Patel 12/25/2022

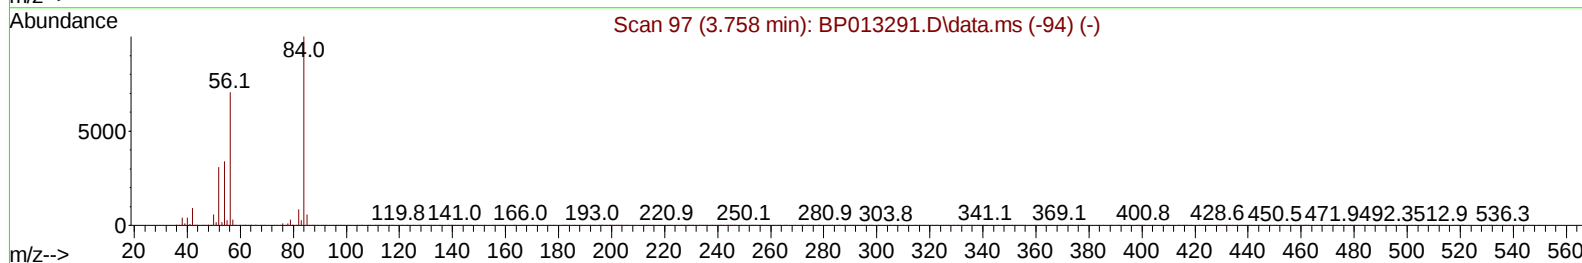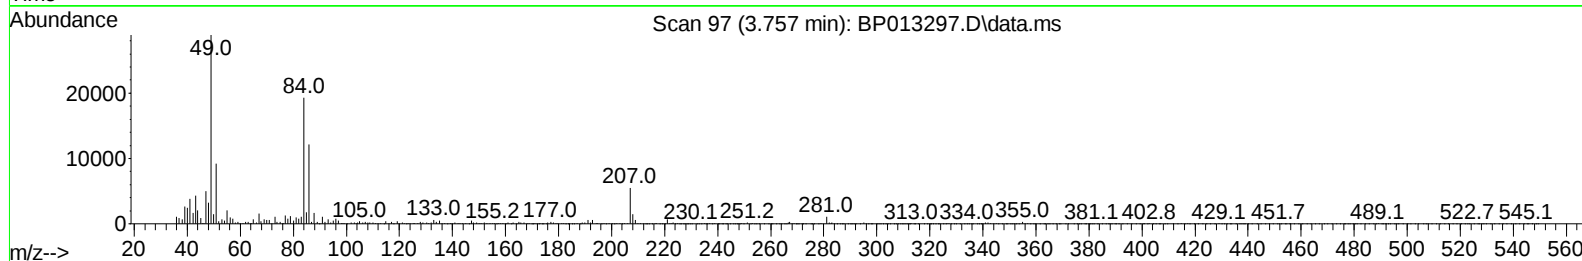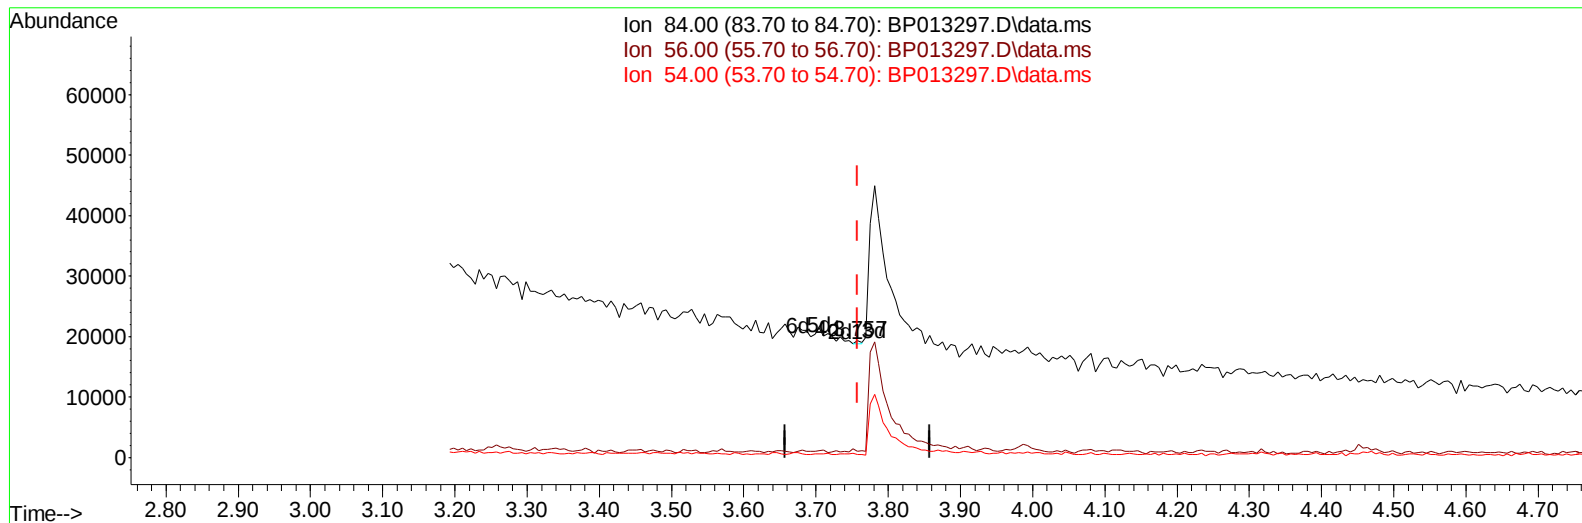

TIC: BP013297.D\data.ms

(4) Pyridine-d5 (S)

3.757min (-0.000) 0.01 ng/u1

response	254	
Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.30	5.33#
54.00	30.50	2.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013297.D
Acq On : 24 Dec 2022 13:34
Operator : CG/JU
Sample : N6016-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYC1

Manual IntegrationsAPPROVED

Quant Time: Dec 25 00:20:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/25/2022
Supervised By :Yogesh Patel 12/25/2022

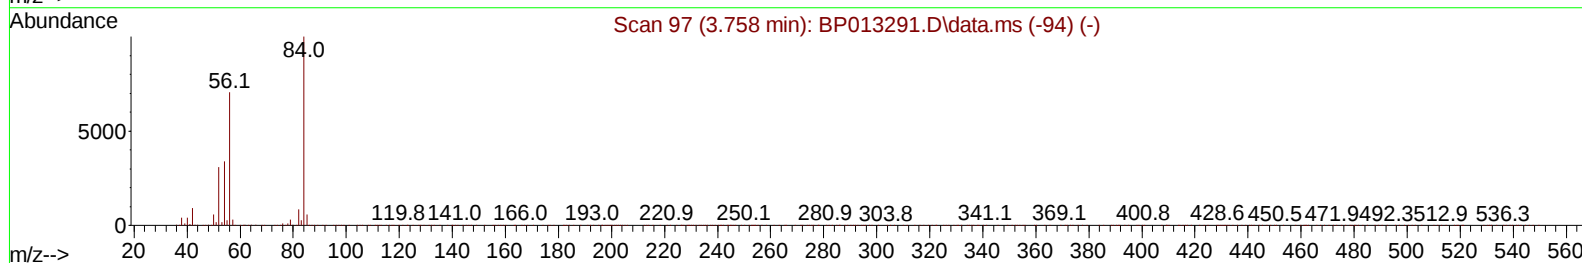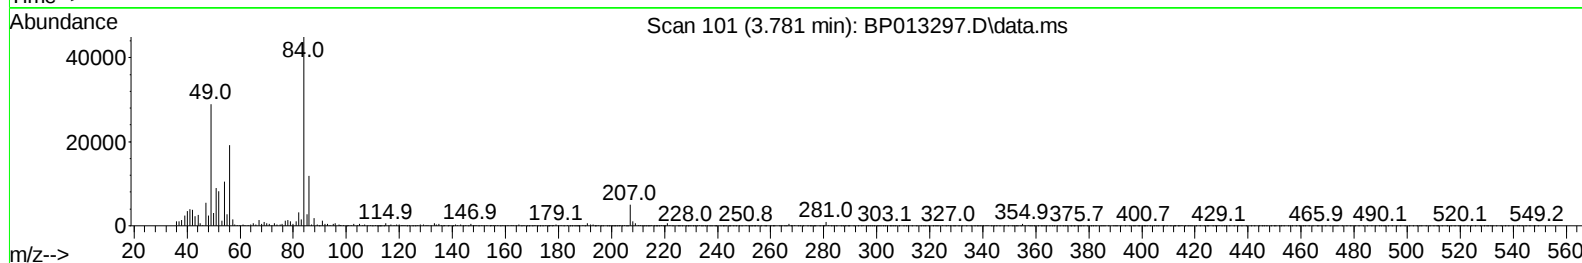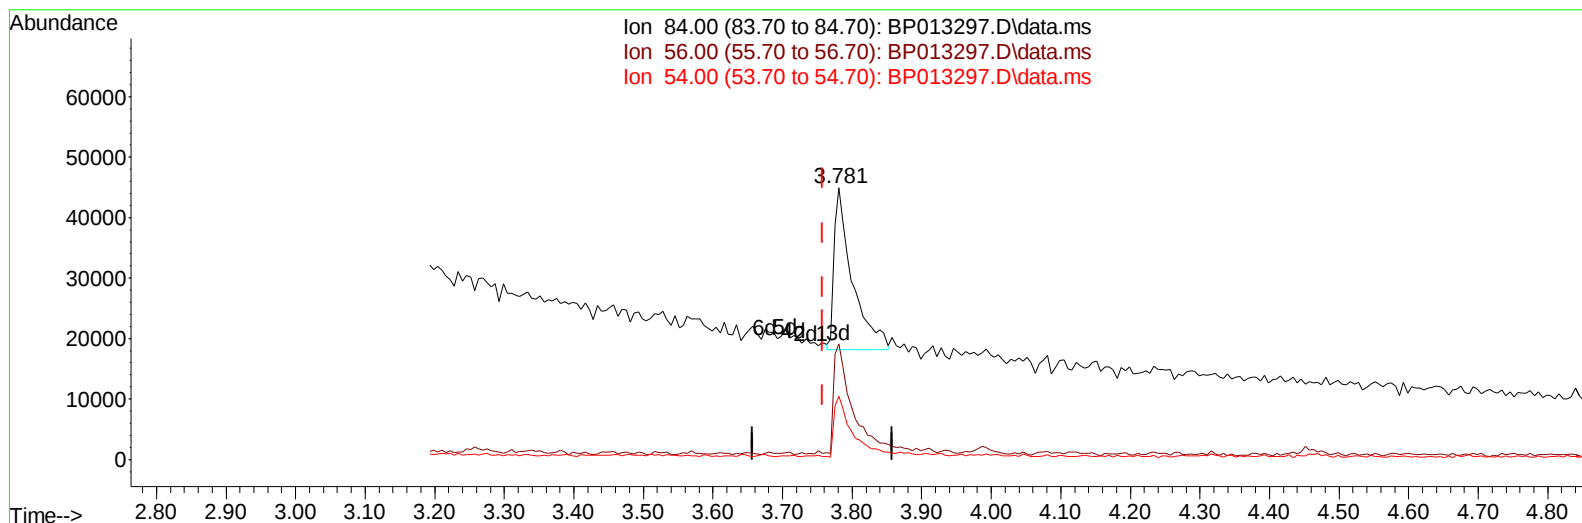

TIC: BP013297.D\data.ms

(4) Pyridine-d5 (S)

3.781min (+ 0.023) 1.05 ng/ul m

response 48830

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.30	42.63#
54.00	30.50	23.34#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013297.D
 Acq On : 24 Dec 2022 13:34
 Operator : CG/JU
 Sample : N6016-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYC1

Manual IntegrationsAPPROVED

Quant Time: Dec 25 00:20:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/25/2022
 Supervised By :Yogesh Patel 12/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.939	152	703216	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	2941584	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	1722555	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	3031290	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	2678104	20.000	ng/ul	0.00
88) Perylene-d12	23.915	264	3170561	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	46164	2.807	ng/uL	0.00
4) Pyridine-d5	3.781	84	48830m	1.045	ng/ul	0.02
7) Phenol-d5	7.104	99	988421	17.256	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	626842	18.142	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	812439	18.018	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113	771606	16.441	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	403760	18.682	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	450011	18.495	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	836429	17.698	ng/ul	0.00
31) 4-Chloroaniline-d4	10.892	131	965832	14.476	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	2469332	18.653	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	2702060	18.575	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	212555	8.926	ng/ul	0.00
60) Fluorene-d10	15.580	176	1981591	17.693	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	180204	9.238	ng/ul	0.00
73) Anthracene-d10	17.445	188	2557435	18.701	ng/ul	0.00
81) Pyrene-d10	19.680	212	2924009	19.021	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.756	264	3093340	19.574	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013297.D
Acq On : 24 Dec 2022 13:34
Operator : CG/JU
Sample : N6016-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYC1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/25/2022
Supervised By :Yogesh Patel 12/25/2022

Quant Time: Dec 25 00:20:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

