

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
 Data File : BP013331.D
 Acq On : 25 Dec 2022 09:50
 Operator : CG/JU
 Sample : PB149864BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK864

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	6	10	19	rVB	5699652	5738394	100.00%	18.153%
2	3.593	65	69	76	rVB	172883	207045	3.61%	0.655%
3	3.687	82	85	89	rVB6	13745	15615	0.27%	0.049%
4	4.081	148	152	159	rVB	38976	48492	0.85%	0.153%
5	4.223	173	176	181	rBV4	10731	16889	0.29%	0.053%
6	4.275	183	185	188	rVB3	10646	12425	0.22%	0.039%
7	5.023	307	312	321	rVB	136684	188942	3.29%	0.598%
8	7.934	800	807	815	rBV	1908915	2964961	51.67%	9.379%
9	10.752	1278	1286	1304	rBV	2390994	4018450	70.03%	12.712%
10	14.463	1912	1917	1920	rBV7	4366	7392	0.13%	0.023%
11	14.581	1929	1937	1949	rBV	3126912	4567921	79.60%	14.450%
12	16.516	2261	2266	2268	rBV7	7556	10966	0.19%	0.035%
13	16.845	2320	2322	2328	rVB7	8570	14251	0.25%	0.045%
14	17.339	2400	2406	2417	rBV	2812909	4065807	70.85%	12.862%
15	17.992	2515	2517	2519	rBV3	7498	8292	0.14%	0.026%
16	18.339	2574	2576	2581	rVB4	25917	31891	0.56%	0.101%
17	21.433	3097	3102	3108	rBV	3325441	4492390	78.29%	14.211%
18	23.910	3517	3523	3534	rVB2	2479535	5201019	90.64%	16.453%




Sum of corrected areas: 31611142

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013331.D
Acq On : 25 Dec 2022 09:50
Operator : CG/JU
Sample : PB149864BL
Misc : GCMS CONFIRMATION
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK864

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

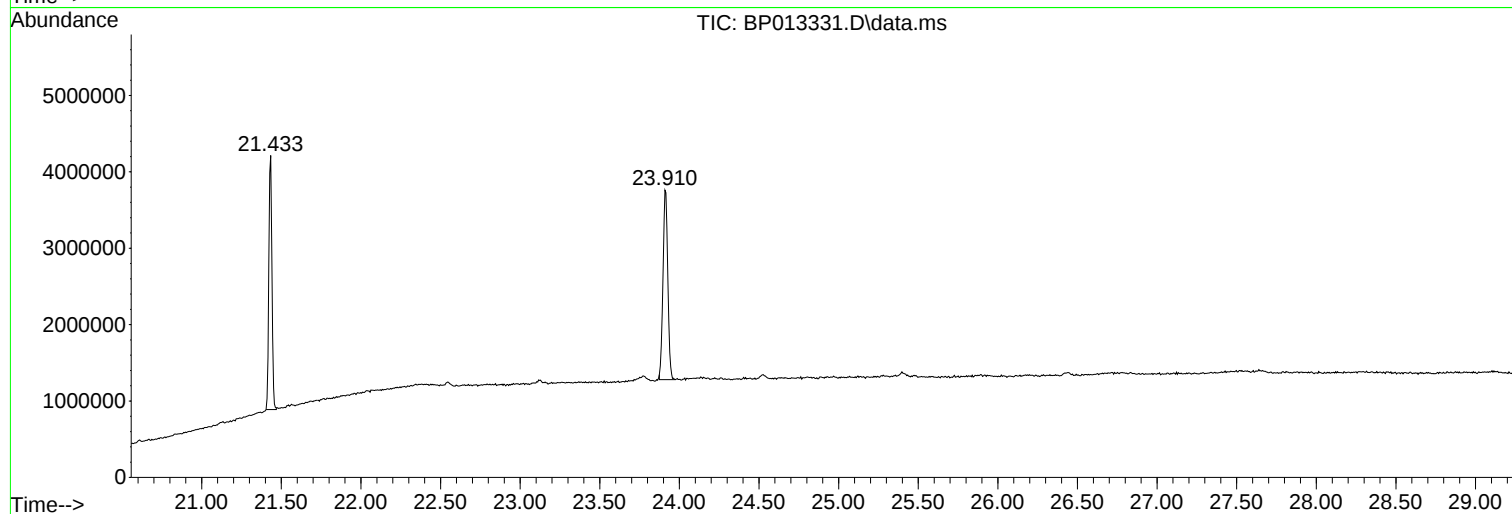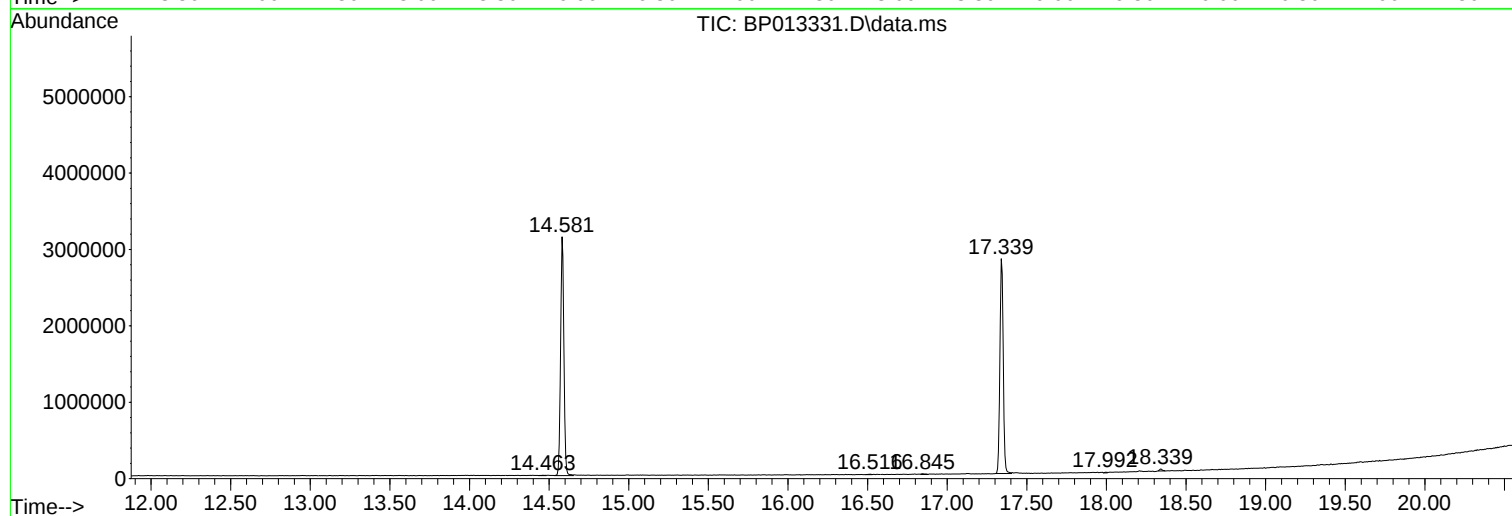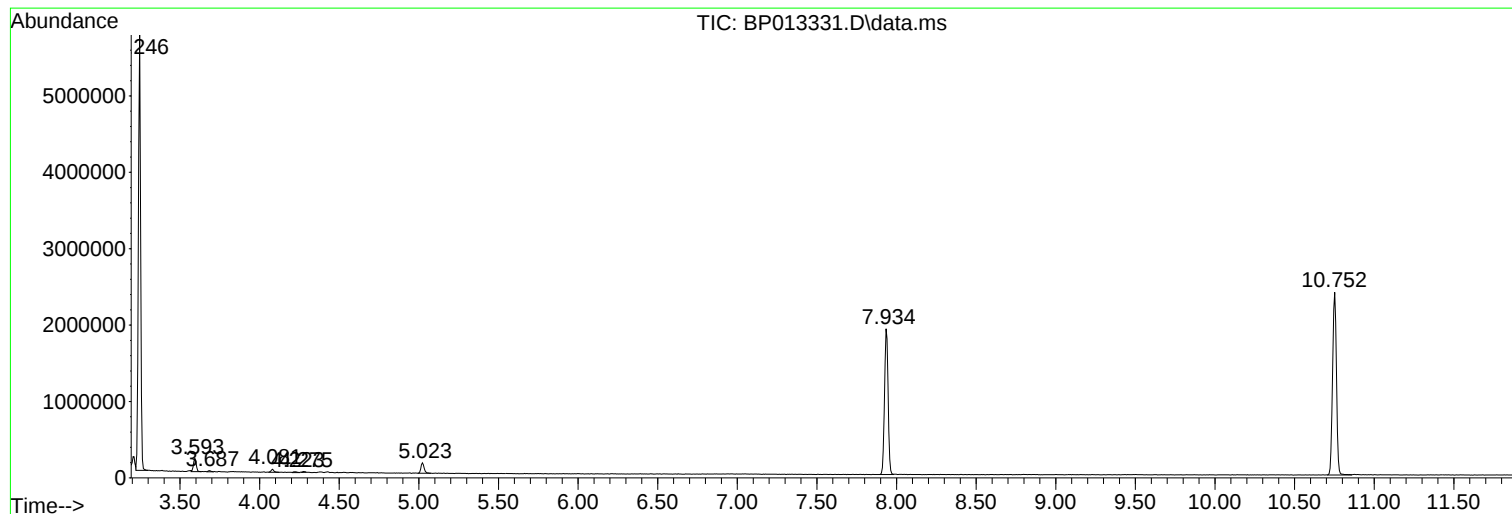

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013331.D
Acq On : 25 Dec 2022 09:50
Operator : CG/JU
Sample : PB149864BL
Misc : GCMS CONFIRMATION
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK864










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.246	38.71 ng/ul	5738390	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	95
2	Heptane			100	C7H16	000142-82-5	94
3	Heptane			100	C7H16	000142-82-5	91
4	Heptane			100	C7H16	000142-82-5	83
5	Oxalic acid, isobutyl pentyl ester			216	C11H20O4	1000309-37-0	64

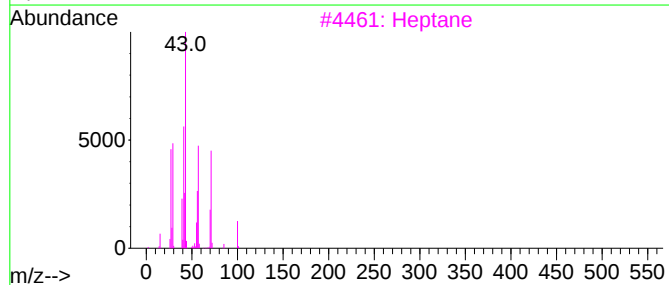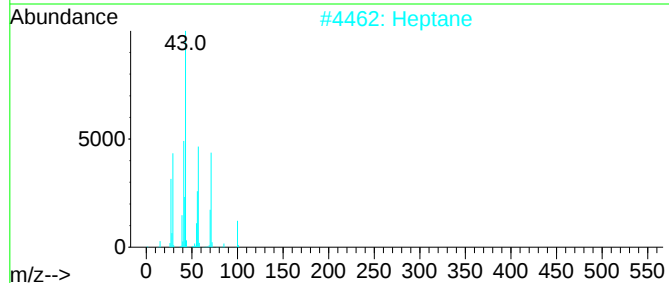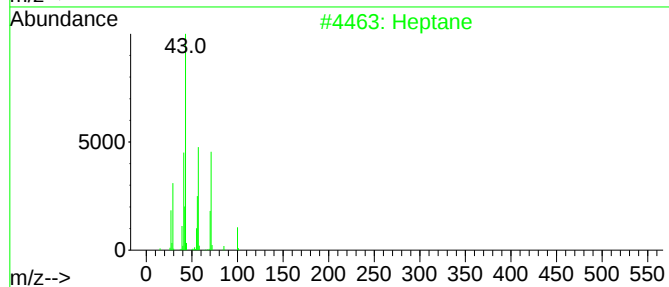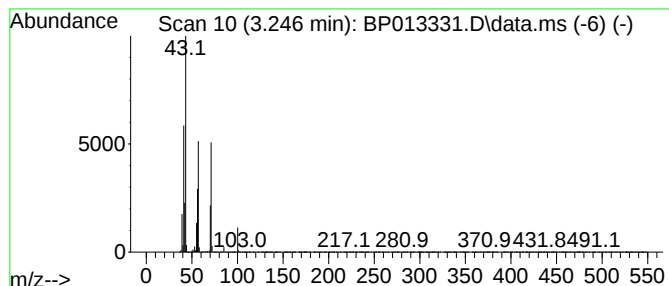

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122422\
Data File : BP013331.D
Acq On : 25 Dec 2022 09:50
Operator : CG/JU
Sample : PB149864BL
Misc : GCMS CONFIRMATION
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK864

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.246	38.7	ng/u1	5738390	1	7.934	2964960	20.0