
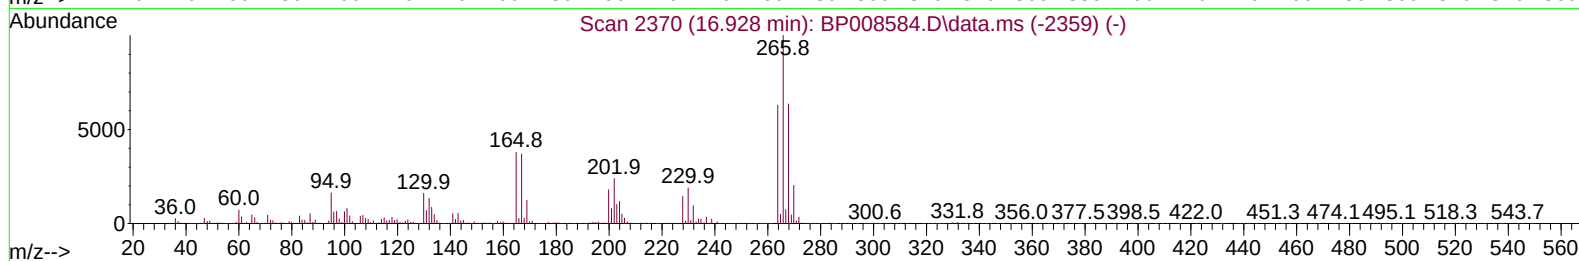
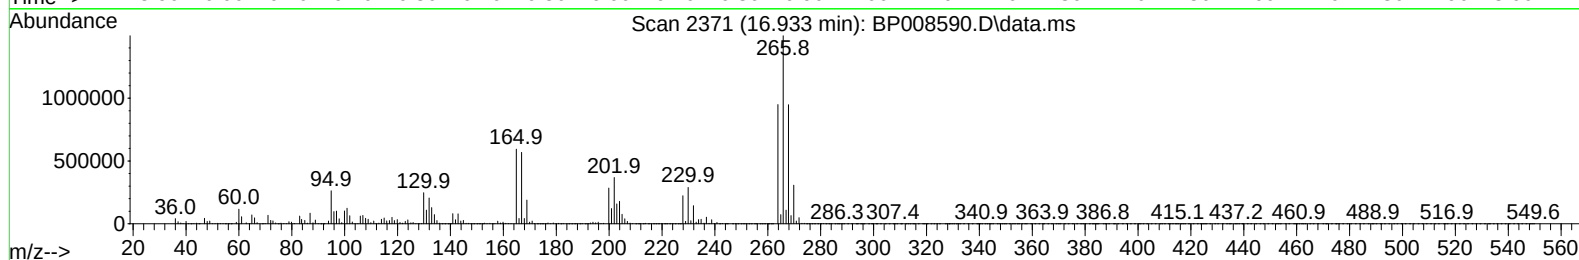


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122921\
 Data File : BP008590.D
 Acq On : 29 Dec 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 12:13:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 29 09:31:54 2021
 Response via : Initial Calibration

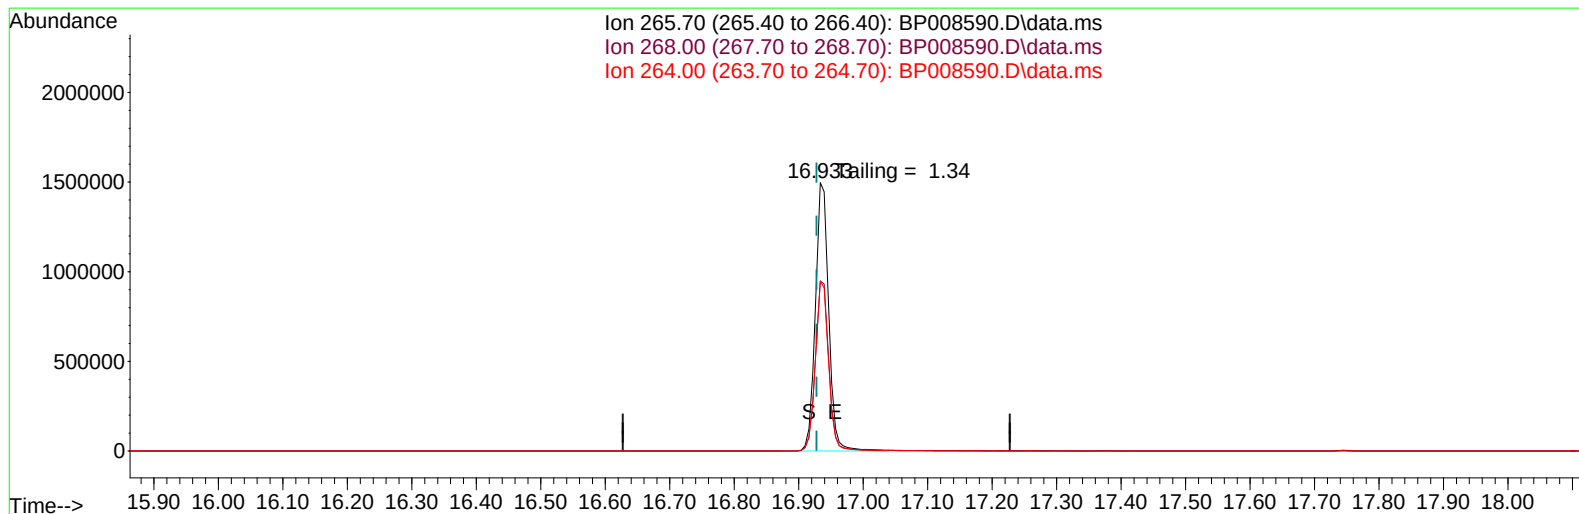

TIC: BP008590.D\data.ms

(70) Pentachlorophenol (C)




16.933min (+ 0.006) 502369.00 ng

response 2175727

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.35
264.00	62.90	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122921\
 Data File : BP008590.D
 Acq On : 29 Dec 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 12:13:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 29 09:31:54 2021
 Response via : Initial Calibration

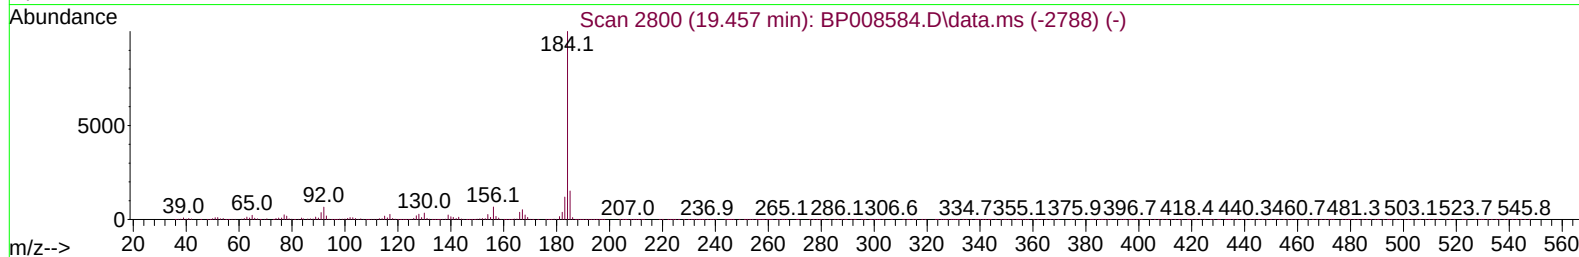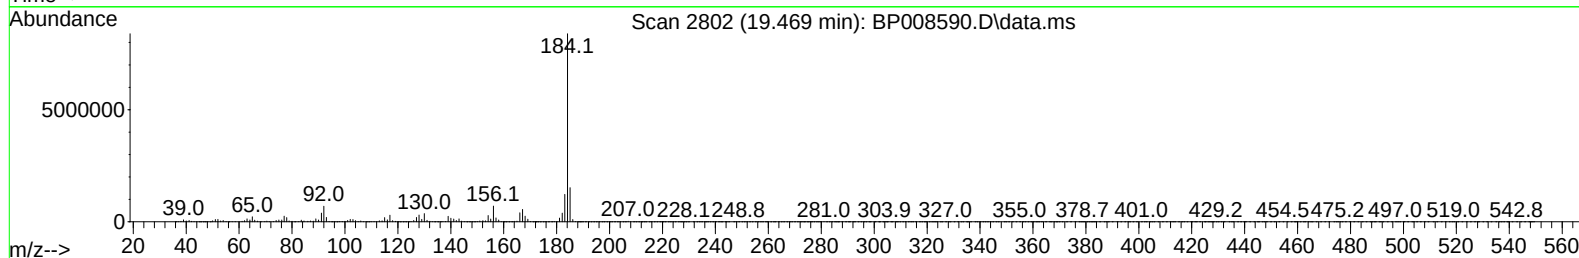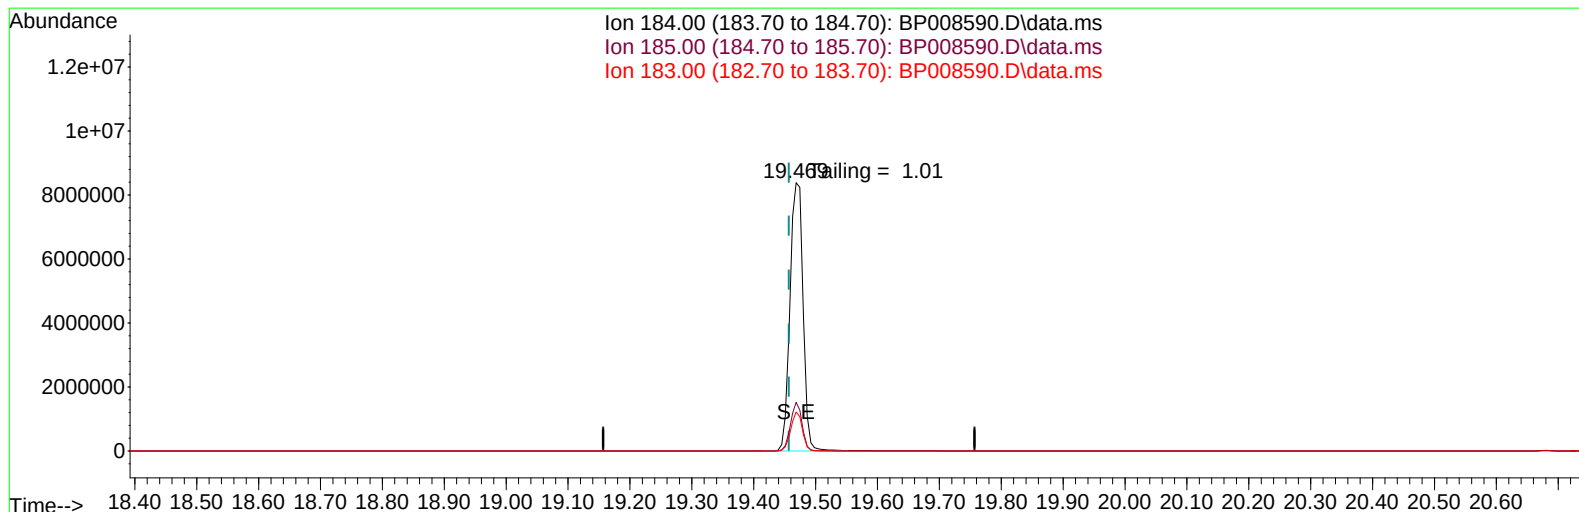

TIC: BP008590.D\data.ms

(77) Benzidine**19.469min (+ 0.012) 56520.64 ng****response 12384494**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	18.14
183.00	11.90	14.59#
0.00	0.00	0.00