

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122921\
Data File : BP008592.D
Acq On : 29 Dec 2021 10:14
Operator : CG/JU
Sample : PB141666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141666BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	415	423	436	rBV	9840181	14910245	33.82%	8.170%
2	7.063	684	693	708	rBV	9413881	15508428	35.18%	8.498%
3	7.899	827	835	843	rBV	2290222	3625230	8.22%	1.986%
4	9.052	1023	1031	1042	rBV	5956730	10108032	22.93%	5.539%
5	10.699	1302	1311	1320	rBV	3090206	5294155	12.01%	2.901%
6	13.157	1721	1729	1743	rBV	19104953	29502962	66.92%	16.166%
7	14.528	1953	1962	1970	rBV	5414027	8194176	18.59%	4.490%
8	16.016	2208	2215	2239	rBV	15325025	21990411	49.88%	12.049%
9	17.275	2422	2429	2441	rBV	7180970	10317849	23.40%	5.653%
10	19.833	2858	2864	2870	rBV2	32893877	44084948	100.00%	24.156%
11	21.357	3117	3123	3134	rBV	8115998	10125337	22.97%	5.548%
12	23.780	3528	3535	3551	rVB2	4413915	8842734	20.06%	4.845%




Sum of corrected areas: 182504507

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122921\
Data File : BP008592.D
Acq On : 29 Dec 2021 10:14
Operator : CG/JU
Sample : PB141666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

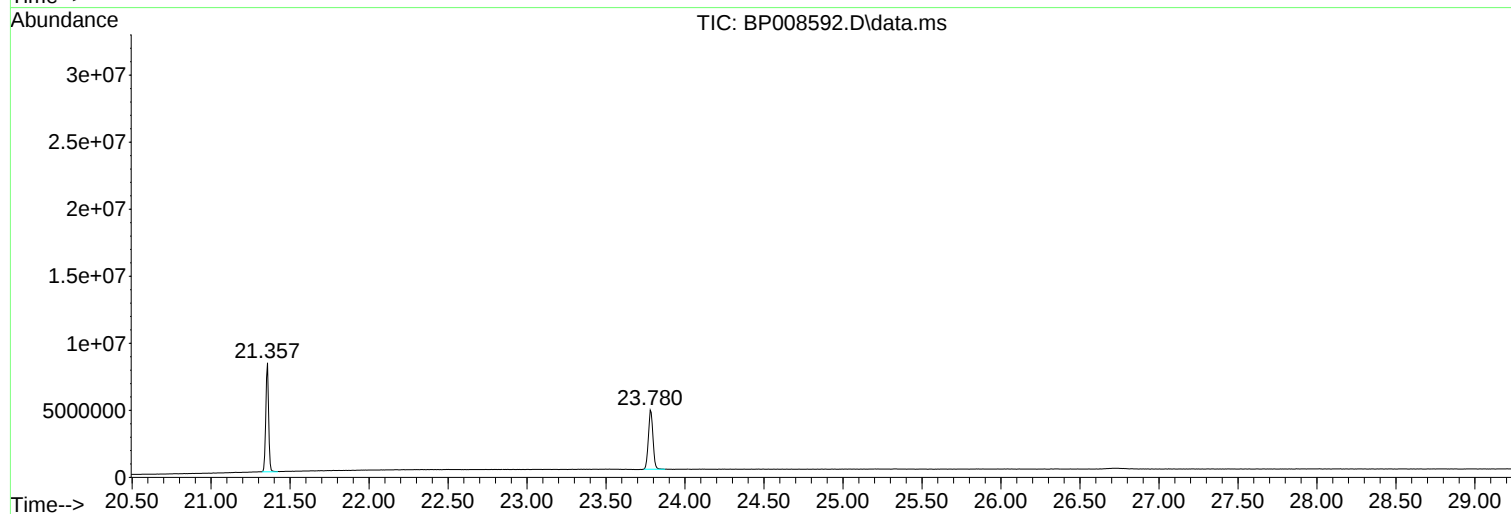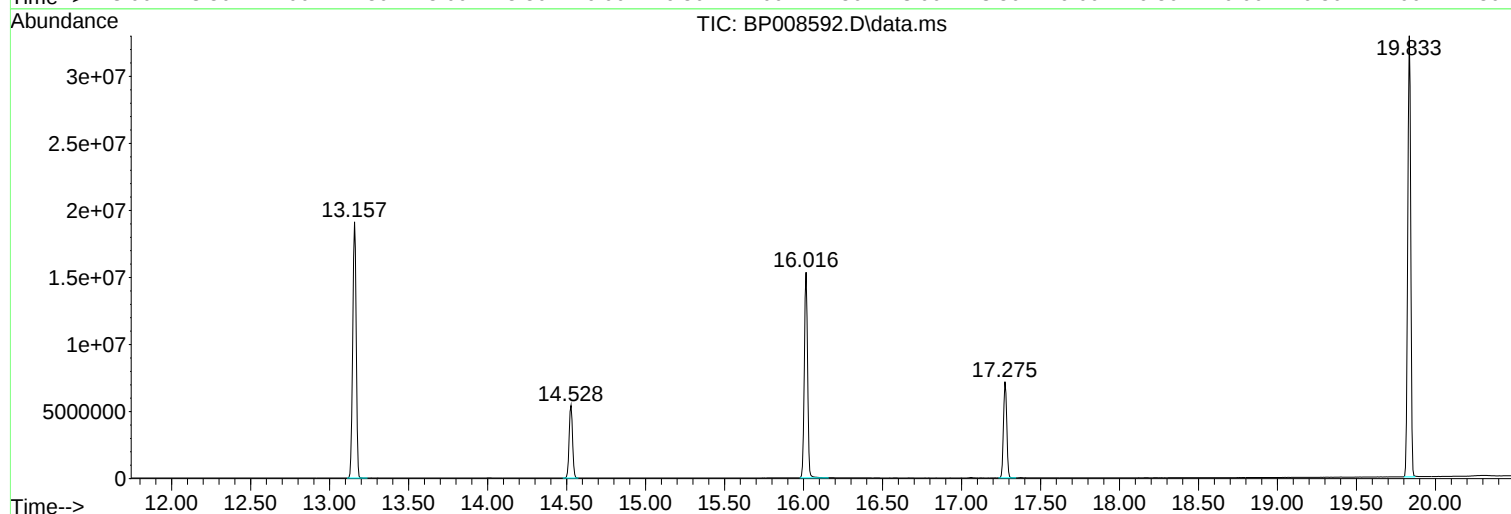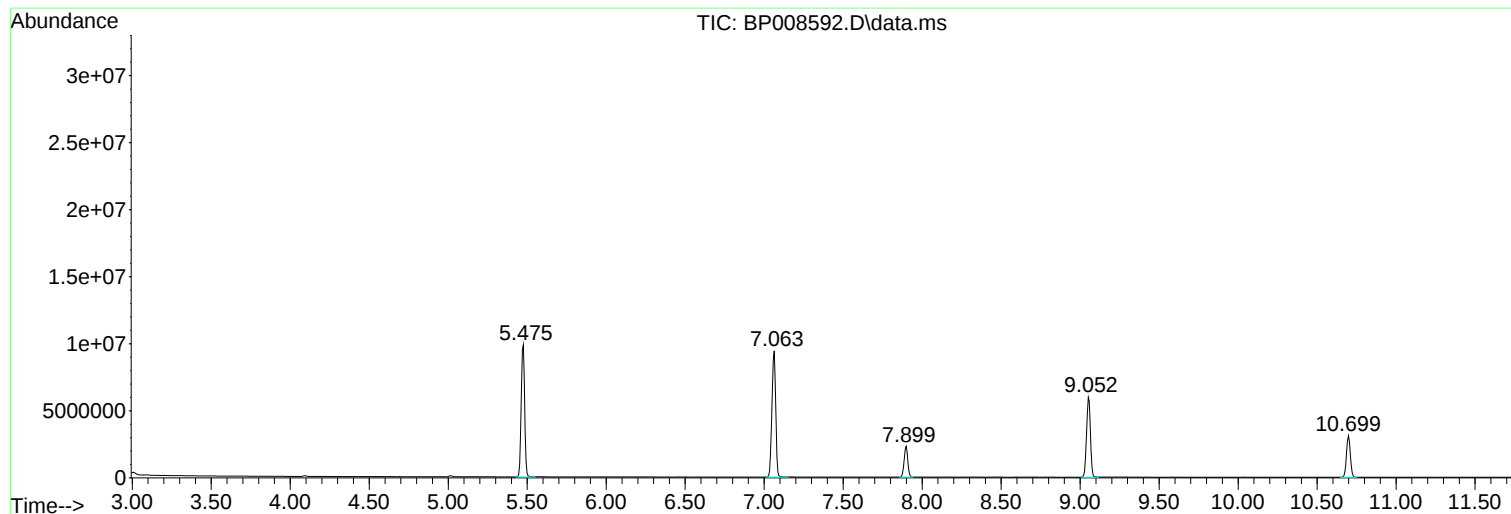

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122921\
Data File : BP008592.D
Acq On : 29 Dec 2021 10:14
Operator : CG/JU
Sample : PB141666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122921\
Data File : BP008592.D
Acq On : 29 Dec 2021 10:14
Operator : CG/JU
Sample : PB141666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------