
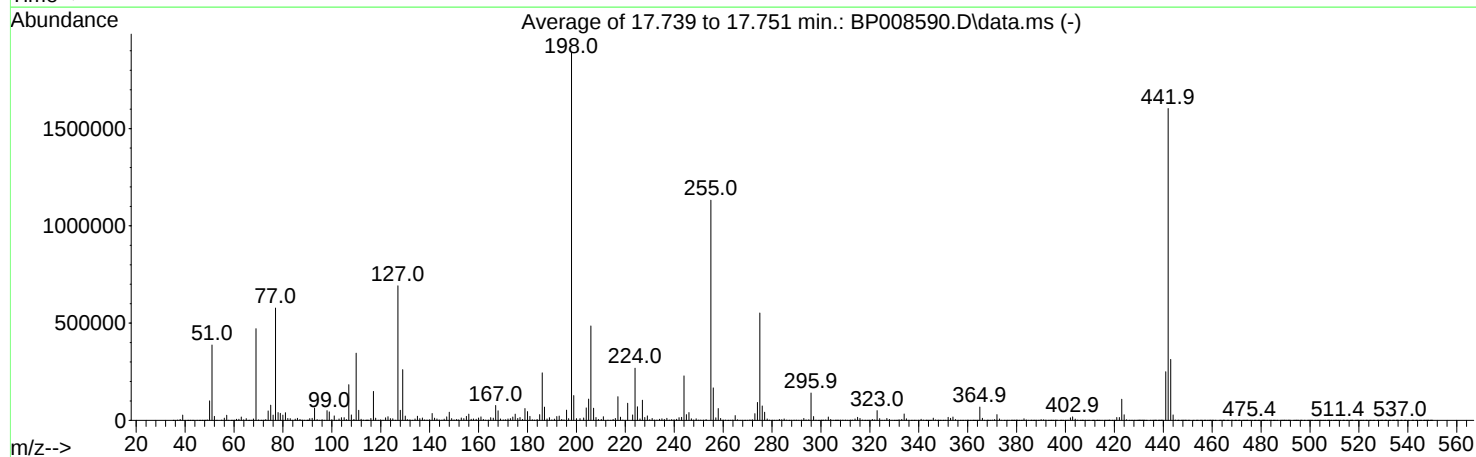


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122921\
 Data File : BP008590.D
 Acq On : 29 Dec 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 08:44:33 2021

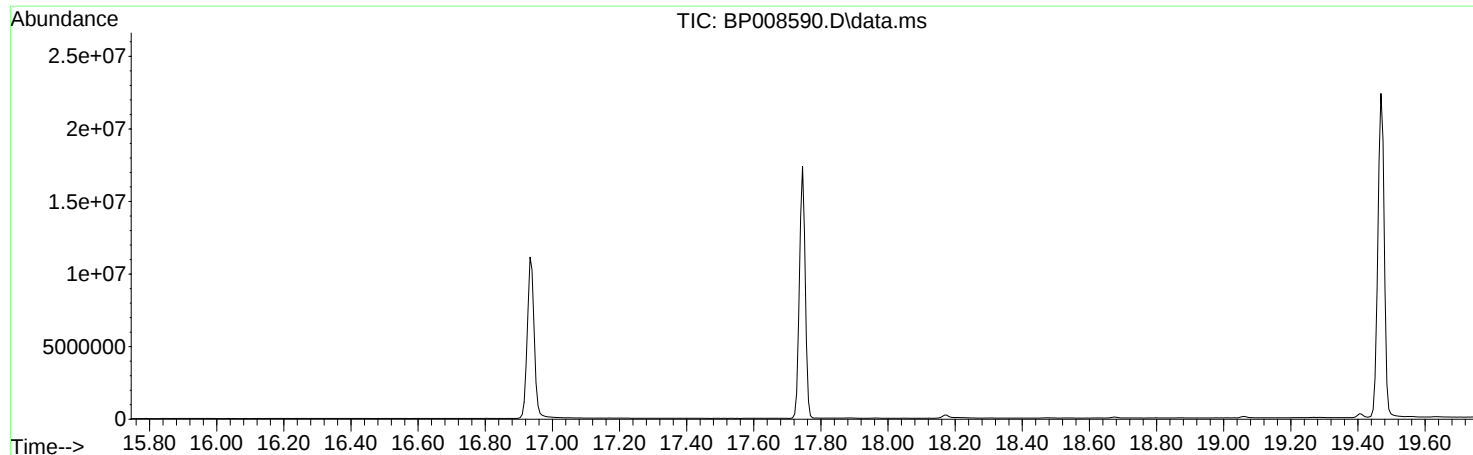

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.5	387782	PASS
68	69	0.00	2	1.6	7703	PASS
69	198	0.00	100	24.9	471802	PASS
70	69	0.00	2	0.5	2173	PASS
127	198	10	80	36.6	692167	PASS
197	198	0.00	2	0.5	8776	PASS
198	198	100	100	100.0	1891316	PASS
199	198	5	9	6.8	127827	PASS
275	198	10	60	29.2	552323	PASS
365	198	1	100	3.6	68703	PASS
441	198	0.01	100	13.2	250197	PASS
442	442	100	100	100.0	1603404	PASS
443	442	15	24	19.5	313344	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/29/2021	BNA_P	<u>BP008590.D</u>
Compound Name	Response	Retention Time
DDT	6510775	20.68
DDD	33254	20.24
DDE	2346	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35600	6546375	0.54

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122921\
 Data File : BP008590.D
 Acq On : 29 Dec 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 29 12:13:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 29 09:31:54 2021
 Response via : Initial Calibration

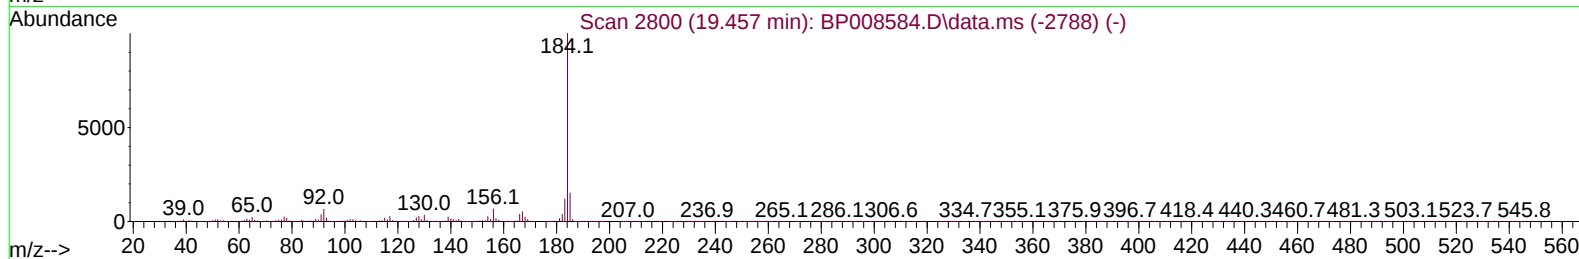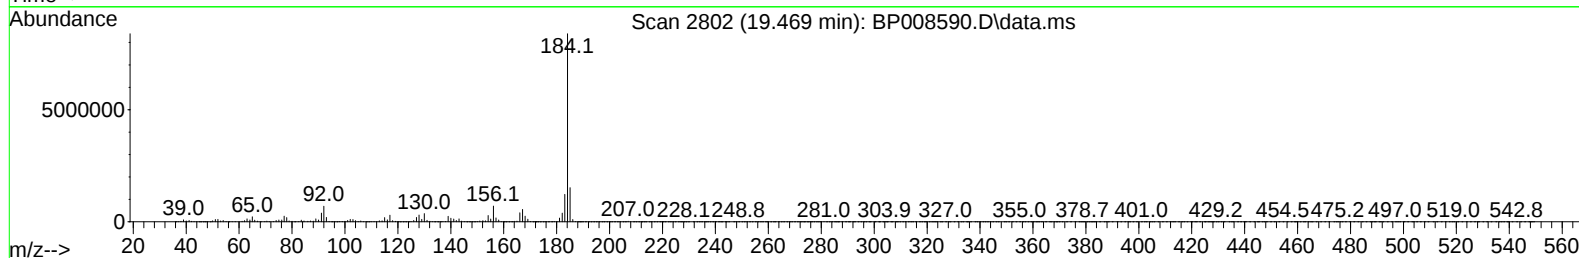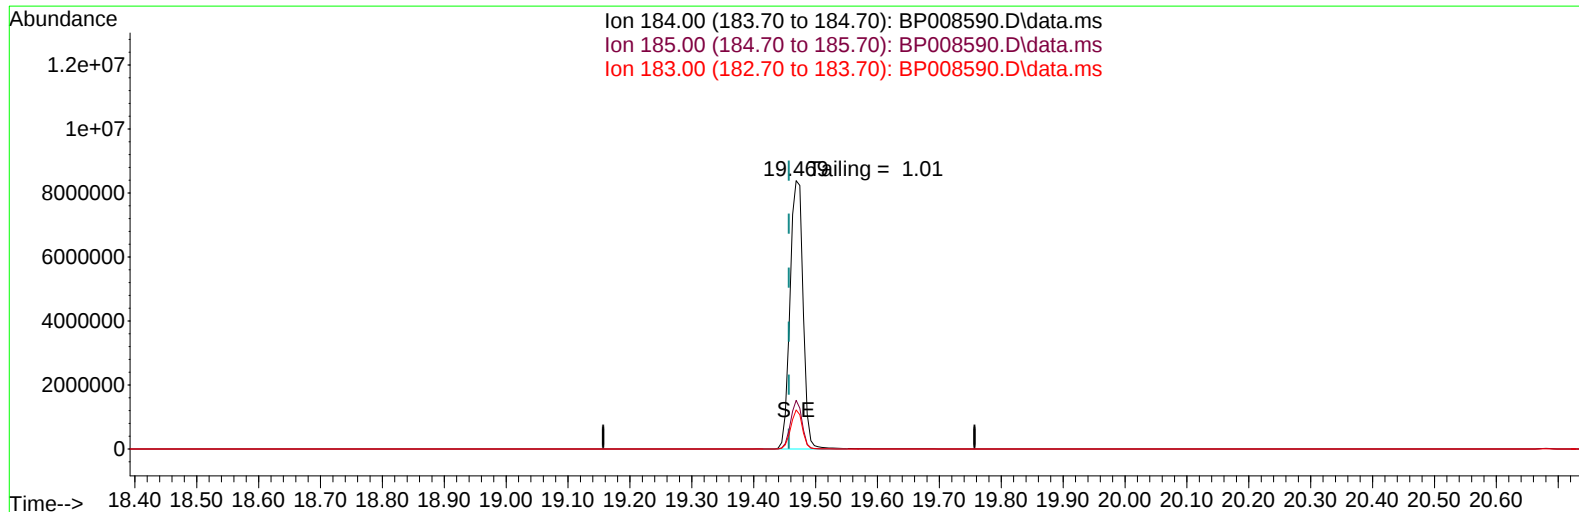

TIC: BP008590.D\data.ms

(77) Benzidine

19.469min (+ 0.012) 56520.64 ng

response 12384494

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	18.14
183.00	11.90	14.59#
0.00	0.00	0.00