
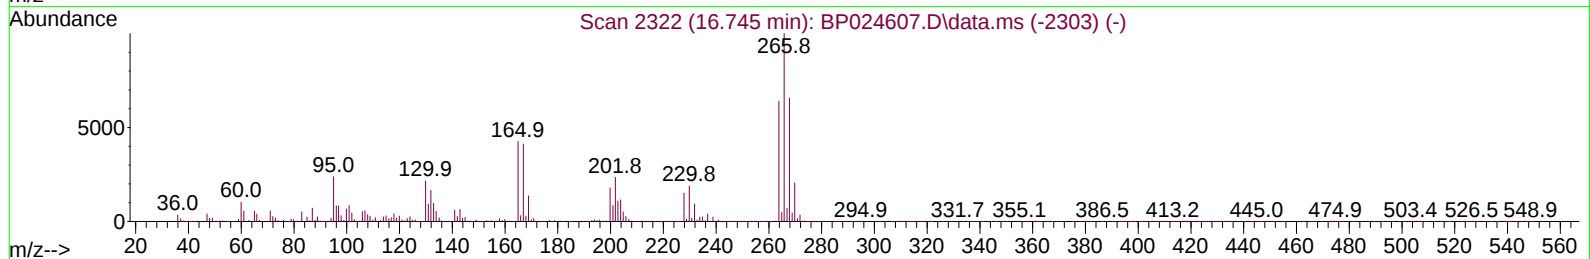
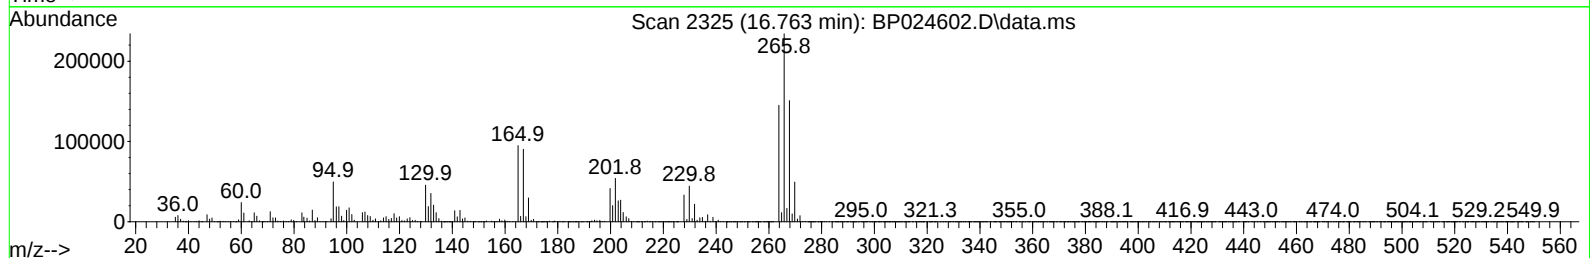


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051225\
Data File : BP024602.D
Acq On : 12 May 2025 14:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 04:08:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 03:56:11 2025
Response via : Initial Calibration

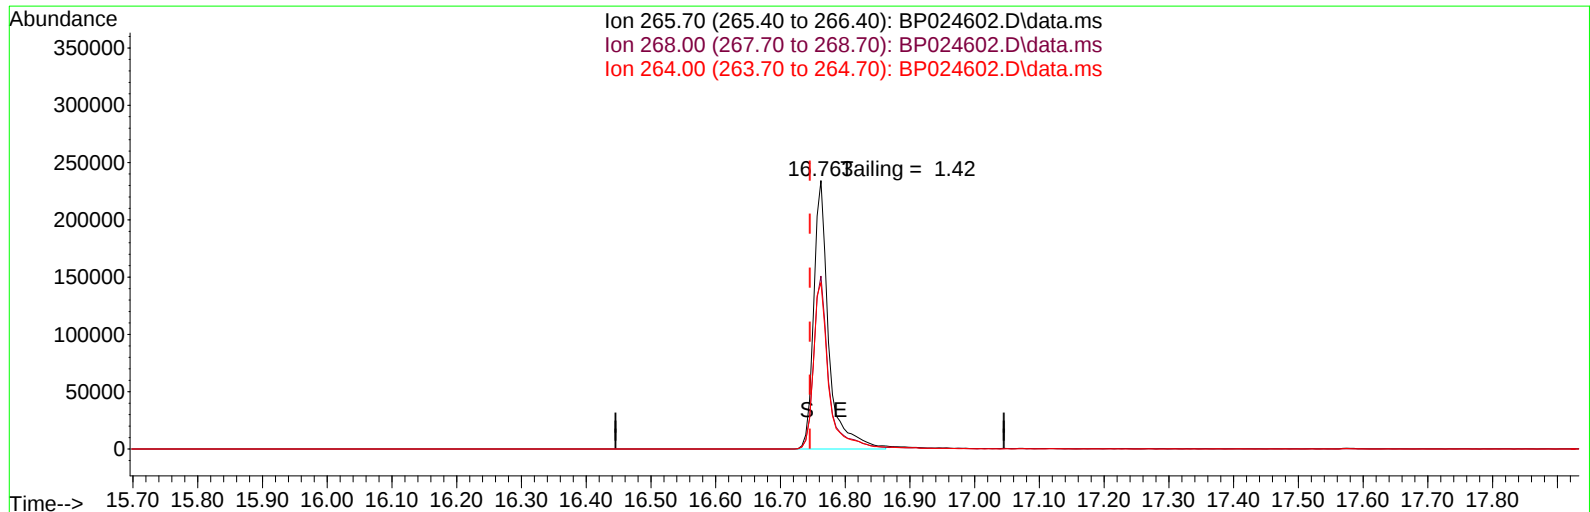

TIC: BP024602.D\data.ms

(70) Pentachlorophenol (C)




16.763min (+ 0.017) 325696.67 ng

response 385147

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	64.40
264.00	64.00	61.99
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051225\  
Data File : BP024602.D  
Acq On    : 12 May 2025  14:38  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 13 04:08:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 03:56:11 2025
Response via : Initial Calibration

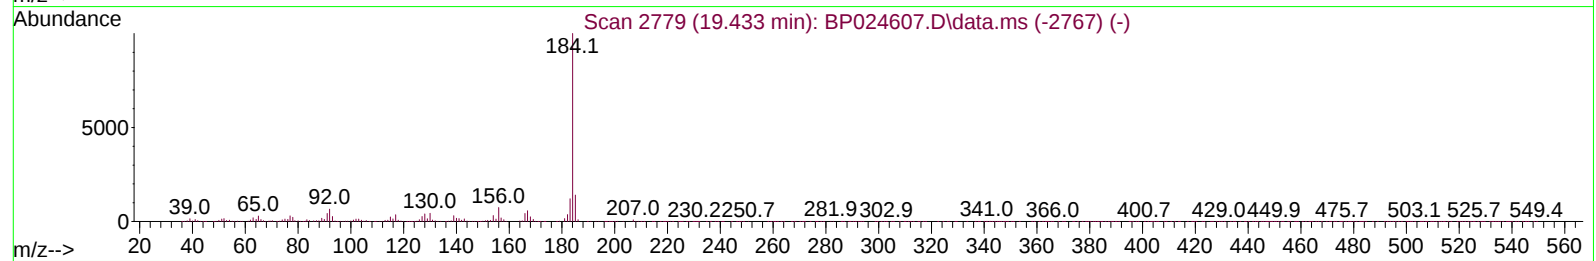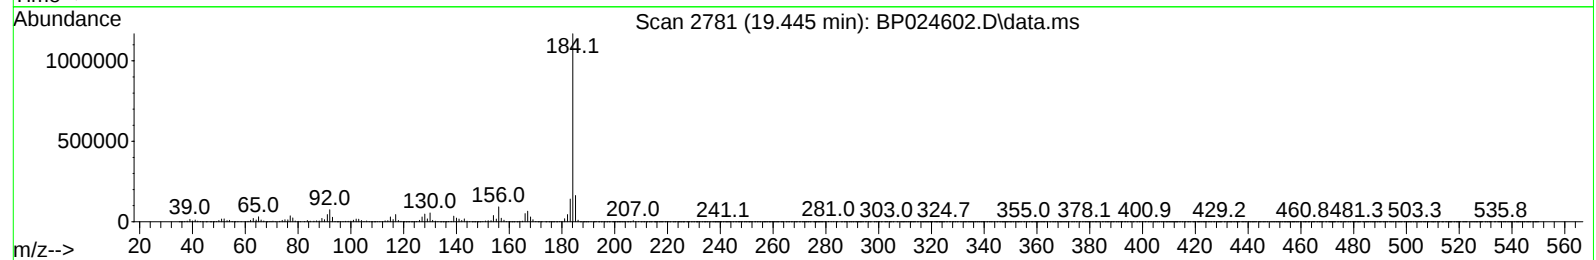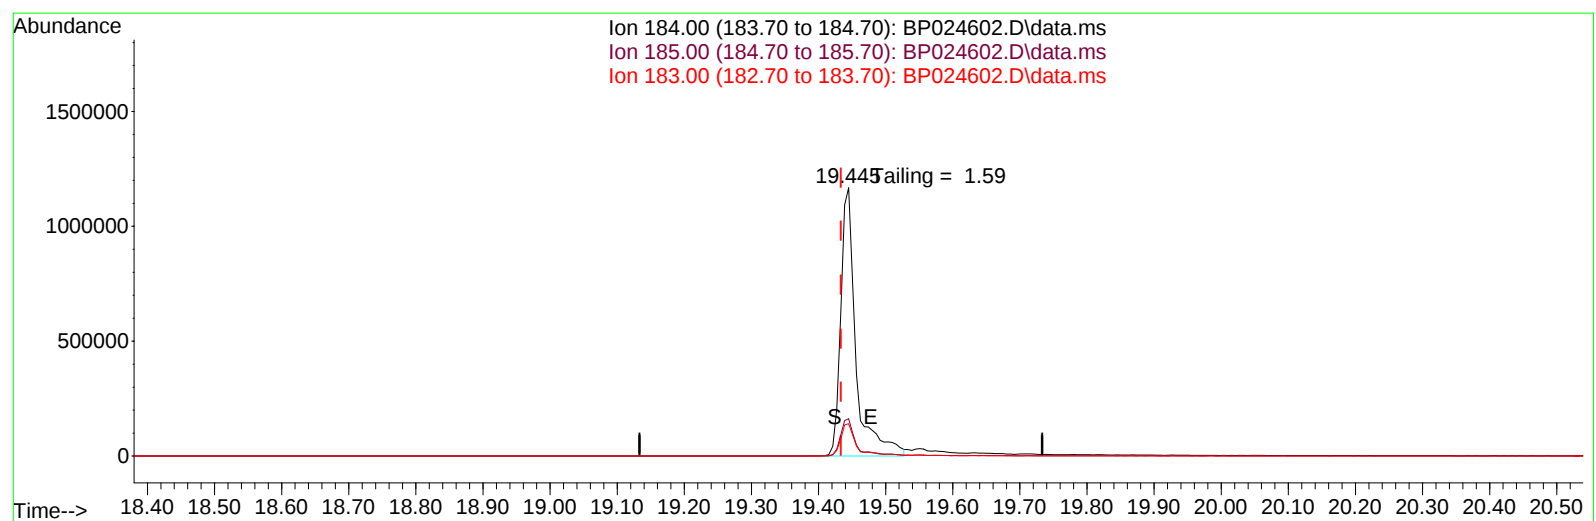

TIC: BP024602.D\data.ms

(77) Benzidine

19.445min (+ 0.011) 68140.40 ng

response **1870396**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.94
183.00	12.10	12.09
0.00	0.00	0.00