
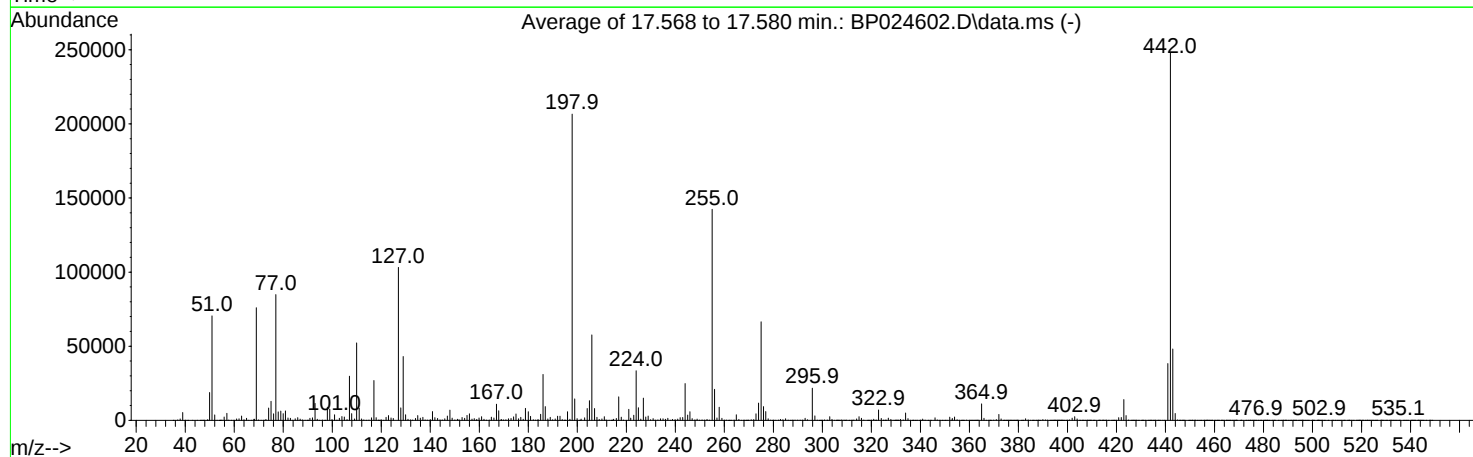


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP051225\  
Data File : BP024602.D  
Acq On : 12 May 2025 14:38  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051225.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue May 13 03:56:11 2025

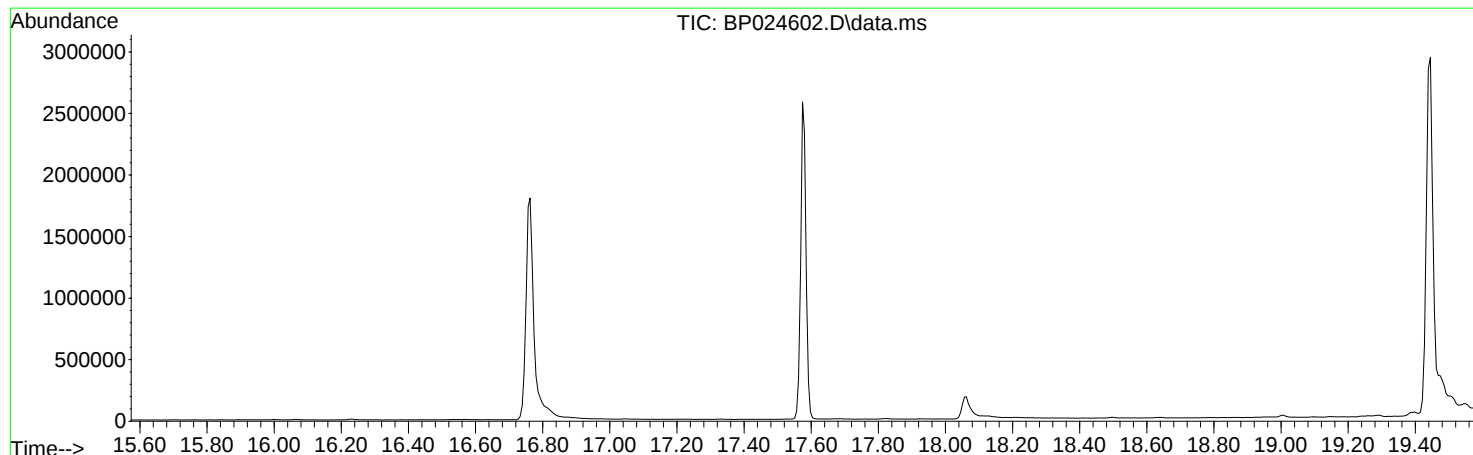

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 51     | 198     | 10     | 80     | 34.1  | 70444  | PASS      |
| 68     | 69      | 0.00   | 2      | 1.1   | 802    | PASS      |
| 69     | 198     | 0.00   | 100    | 36.8  | 75982  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.5   | 378    | PASS      |
| 127    | 198     | 10     | 80     | 49.9  | 103142 | PASS      |
| 197    | 198     | 0.00   | 2      | 0.4   | 763    | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 206549 | PASS      |
| 199    | 198     | 5      | 9      | 7.0   | 14431  | PASS      |
| 275    | 198     | 10     | 60     | 32.2  | 66539  | PASS      |
| 365    | 198     | 1      | 100    | 5.4   | 11123  | PASS      |
| 441    | 198     | 0.01   | 100    | 18.5  | 38277  | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 248137 | PASS      |
| 443    | 442     | 15     | 24     | 19.4  | 48105  | PASS      |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/12/2025     | BNA_P            | <u>BP024602.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 760601           | 20.733             |
| DDD           | 10363            | 20.327             |
| DDE           | 748              | 19.745             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 11111         | 771712           | 1.44               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP051225\  
Data File : BP024602.D  
Acq On : 12 May 2025 14:38  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: May 13 04:08:09 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP051225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 13 03:56:11 2025  
Response via : Initial Calibration

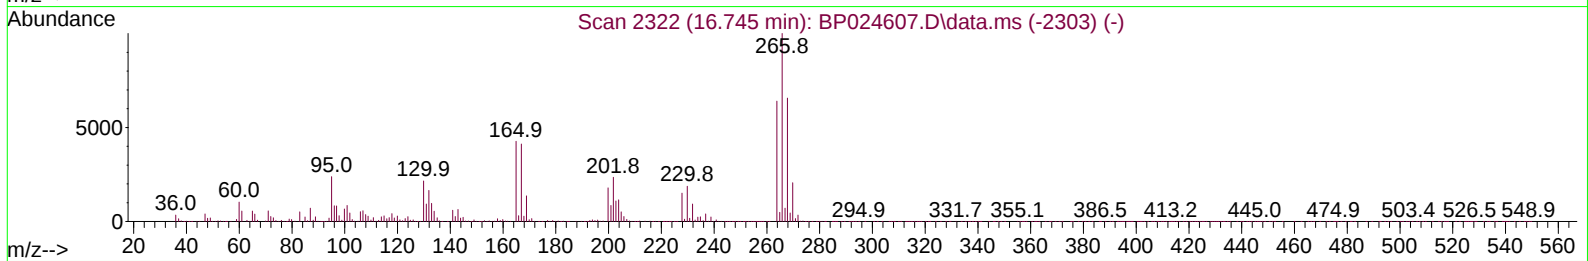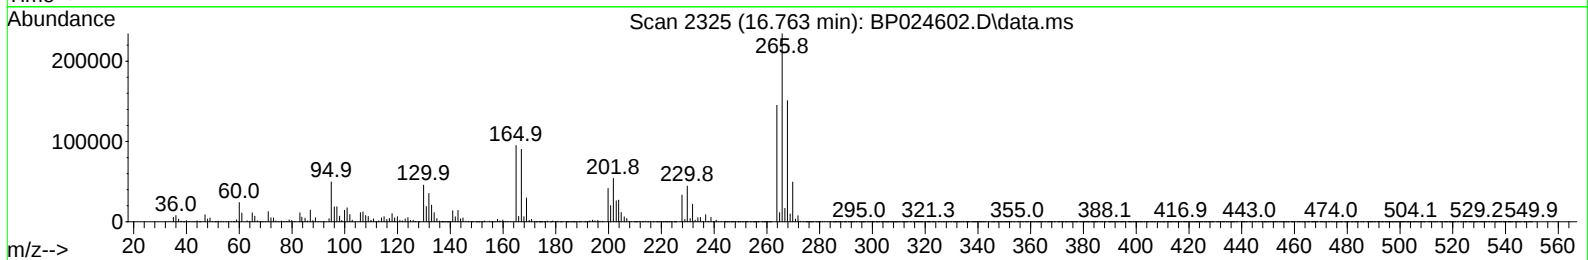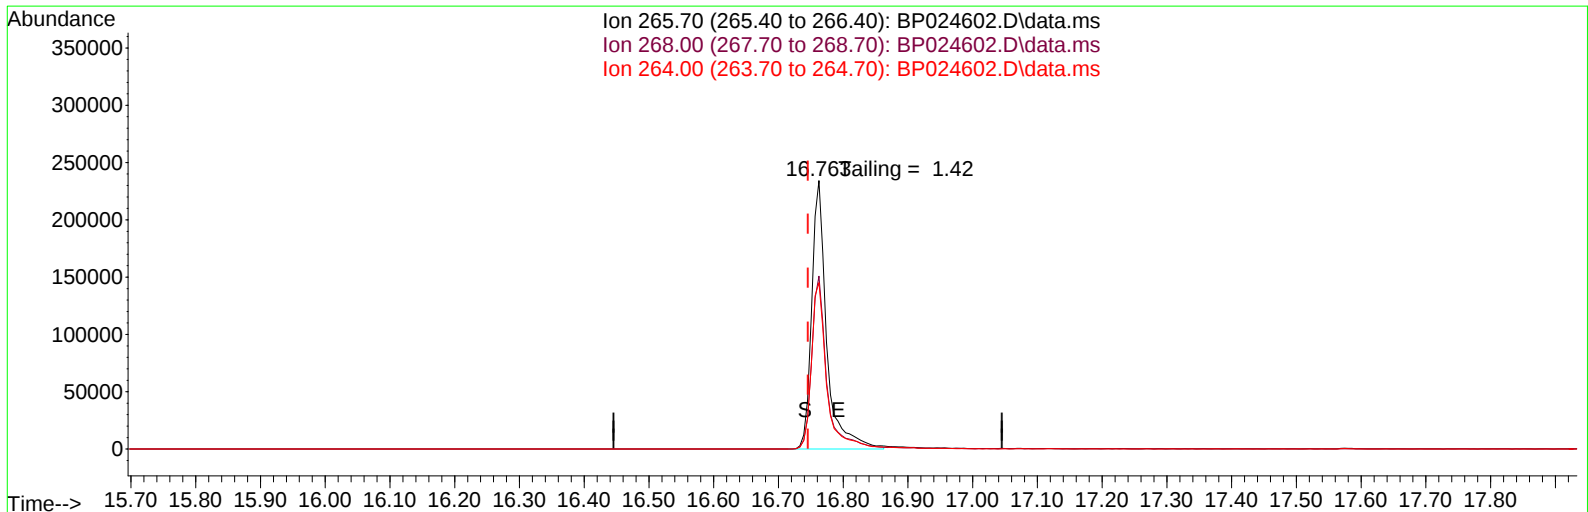

TIC: BP024602.D\data.ms

**(70) Pentachlorophenol (C)**

**16.763min (+ 0.017) 325696.67 ng**

**response 385147**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.60  | 64.40  |
| 264.00 | 64.00  | 61.99  |
| 0.00   | 0.00   | 0.00   |

