
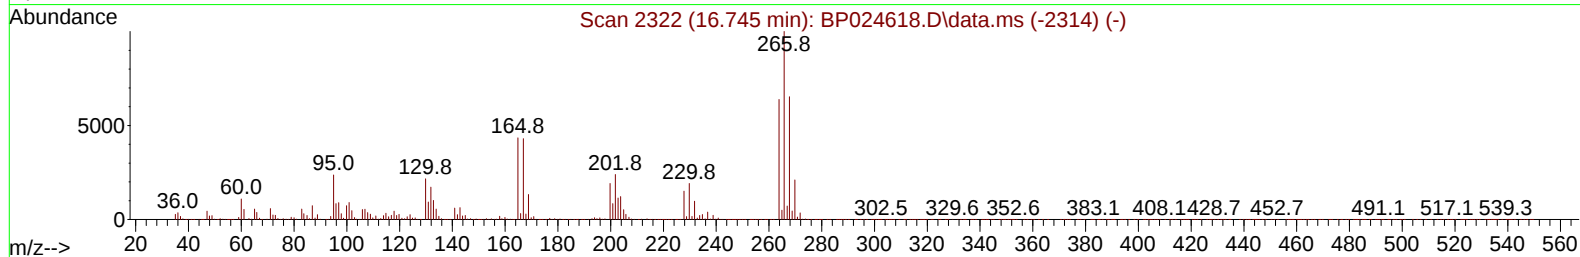
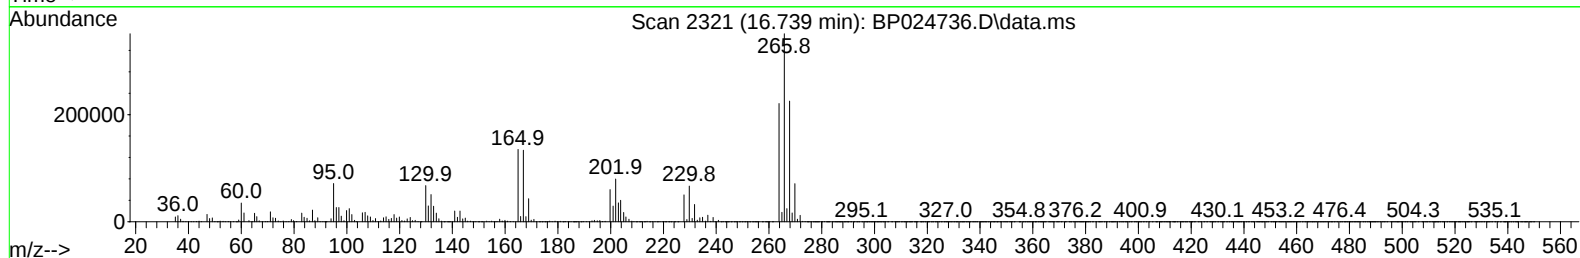


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052125\
Data File : BP024736.D
Acq On : 21 May 2025 12:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 13:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

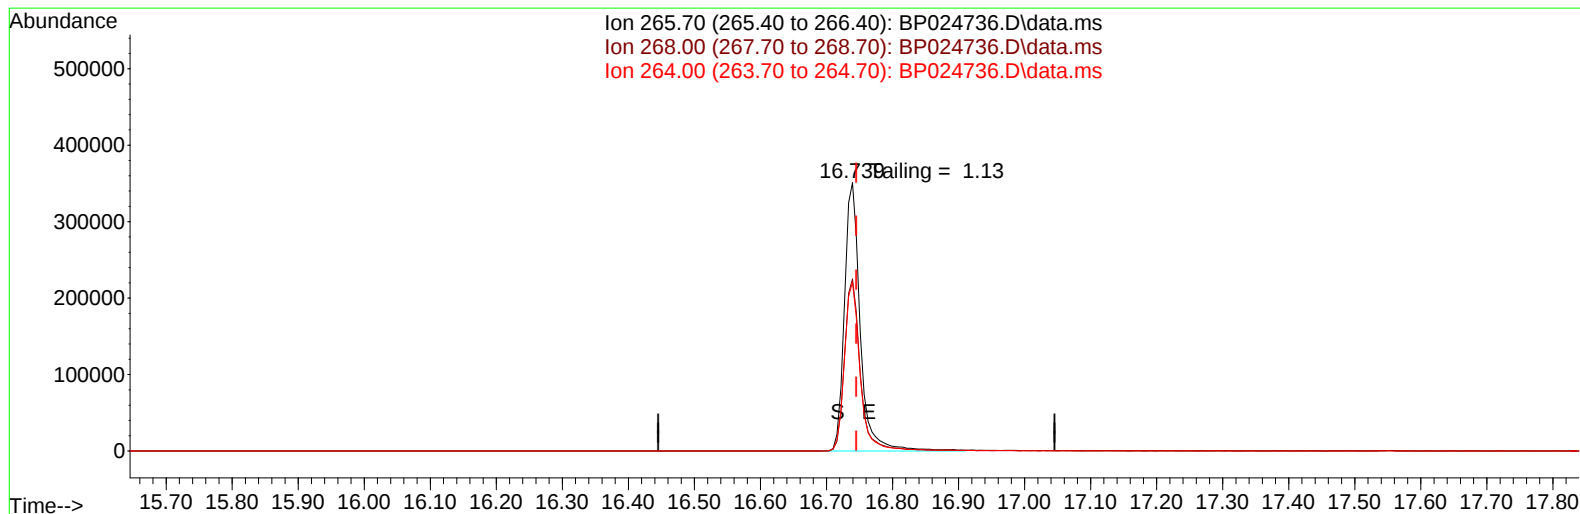

TIC: BP024736.D\data.ms

(70) Pentachlorophenol (C)




16.739min (-0.006) 2229164.54 ng

response 580825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.16
264.00	63.90	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052125\
Data File : BP024736.D
Acq On : 21 May 2025 12:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 21 13:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

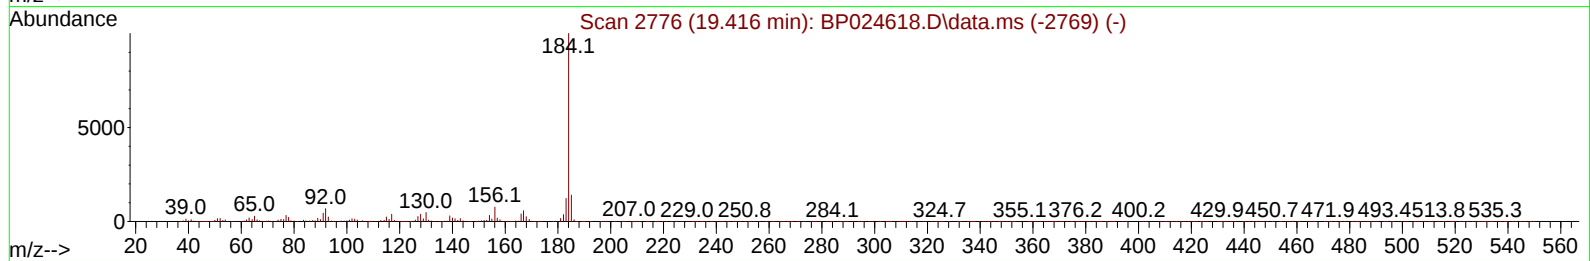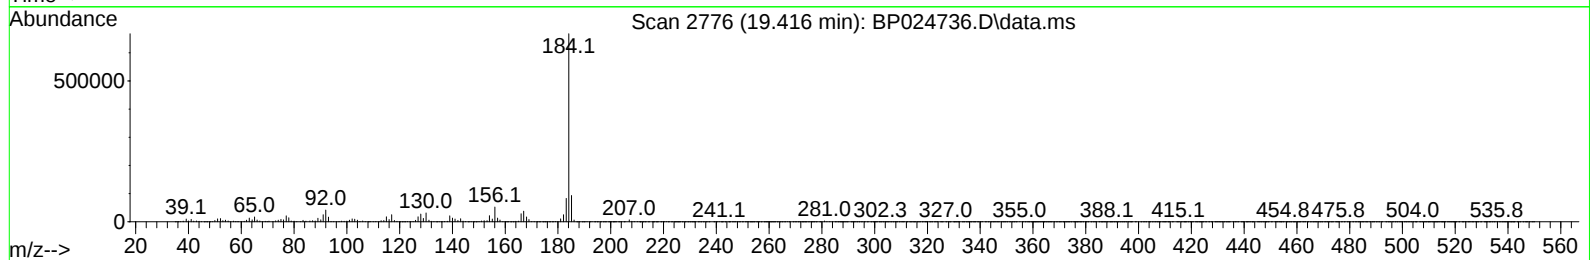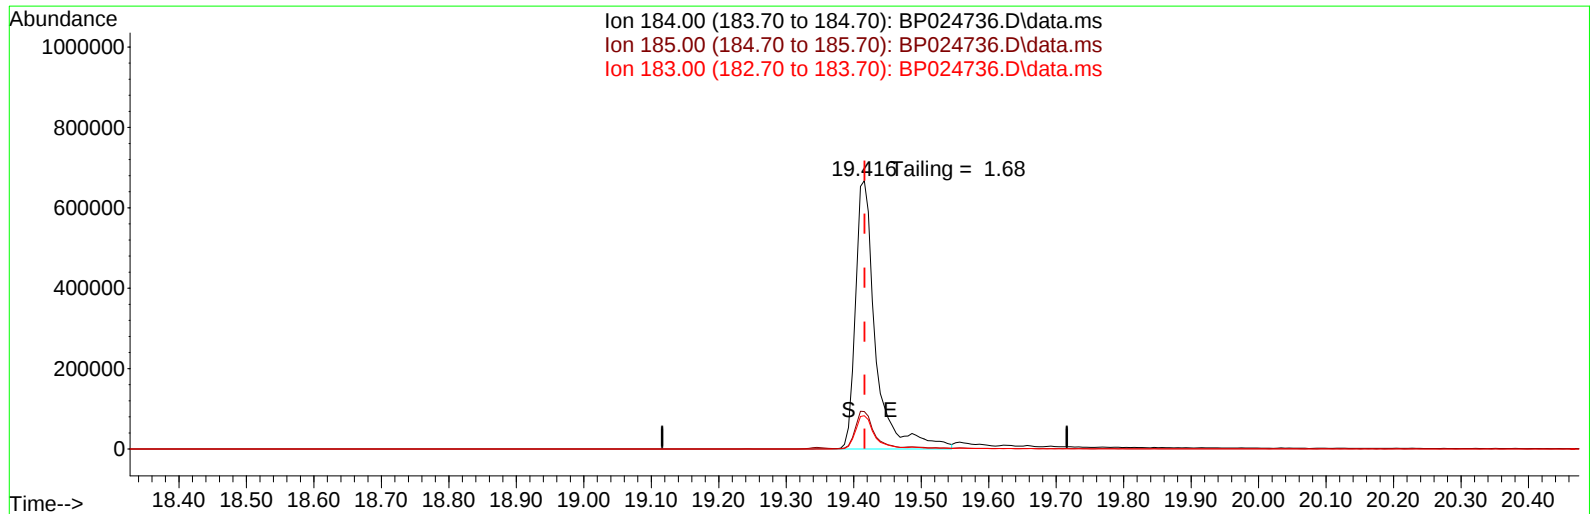

TIC: BP024736.D\data.ms

(77) Benzidine

19.416min (-0.000) 1103021.58 ng

response 1291799

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.97
183.00	12.30	12.45
0.00	0.00	0.00