
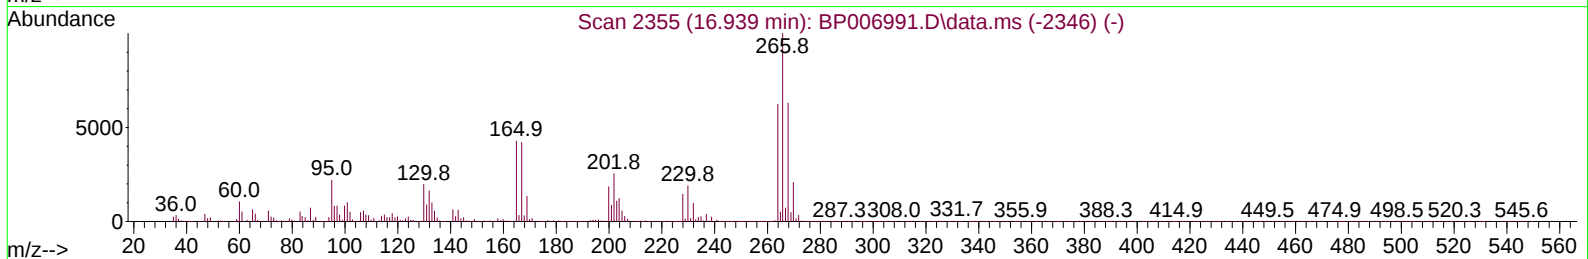
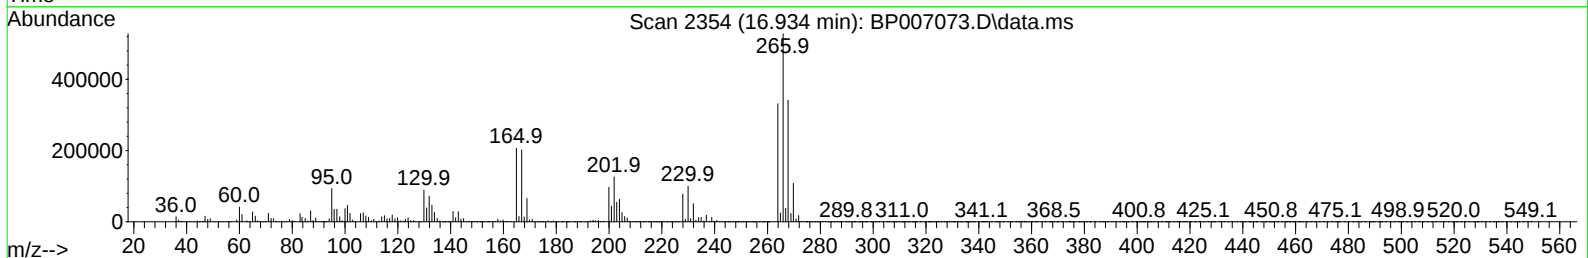


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092121\
 Data File : BP007073.D
 Acq On : 21 Sep 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 10:50:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 10:50:16 2021
 Response via : Initial Calibration

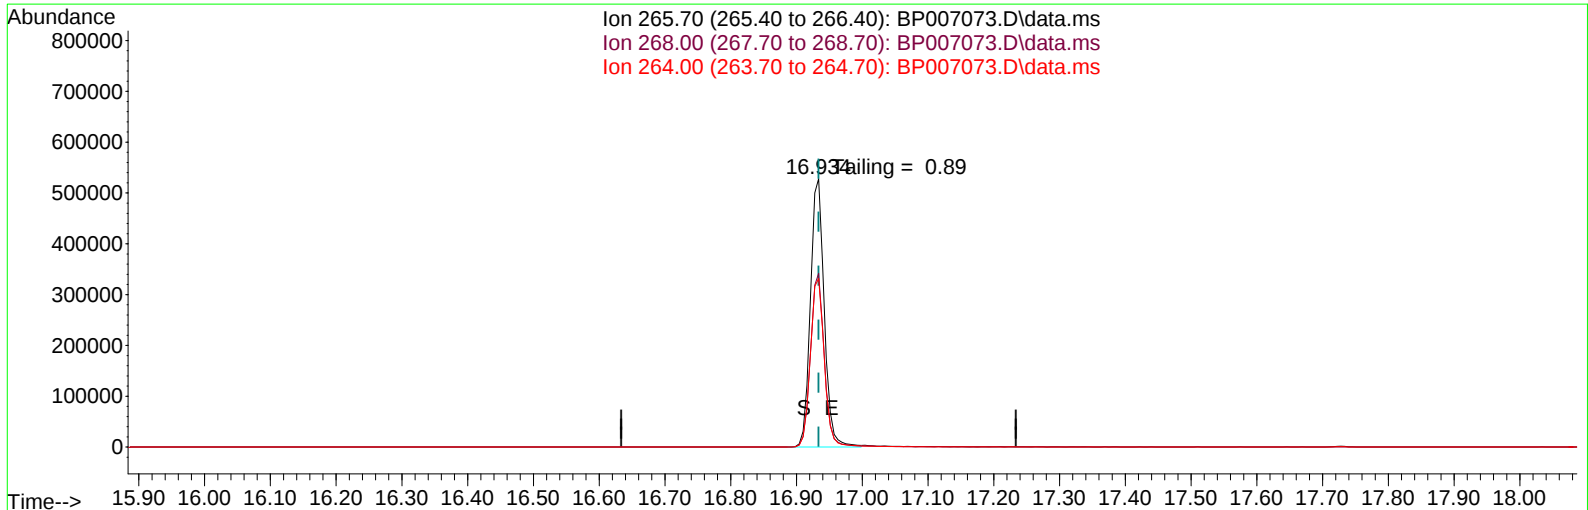

TIC: BP007073.D\data.ms




(70) Pentachlorophenol (C)

16.934min (+ 0.000) 198479.55 ng

response 779134

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.68
264.00	62.90	62.81
0.00	0.00	0.00

Quant Time: Sep 21 10:50:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 17 10:50:16 2021
Response via : Initial Calibration

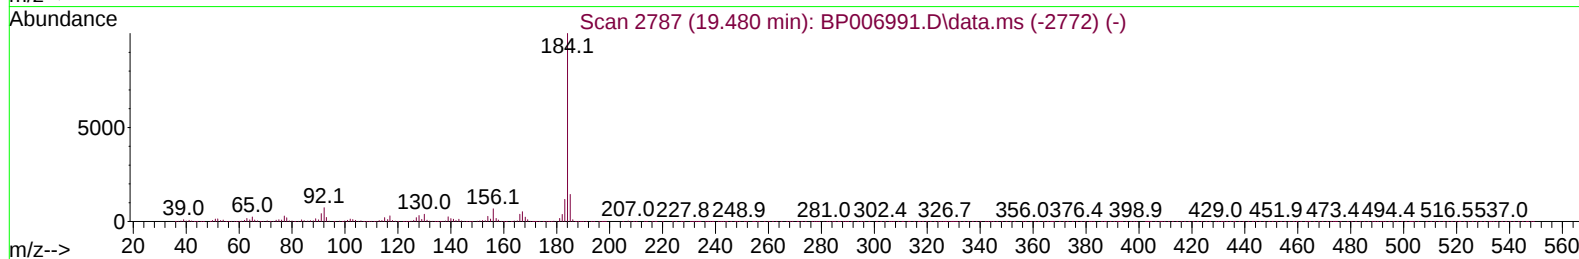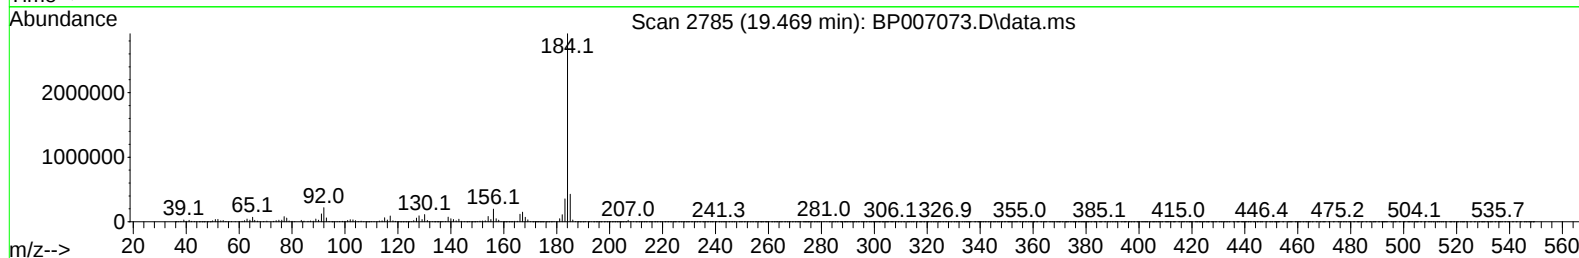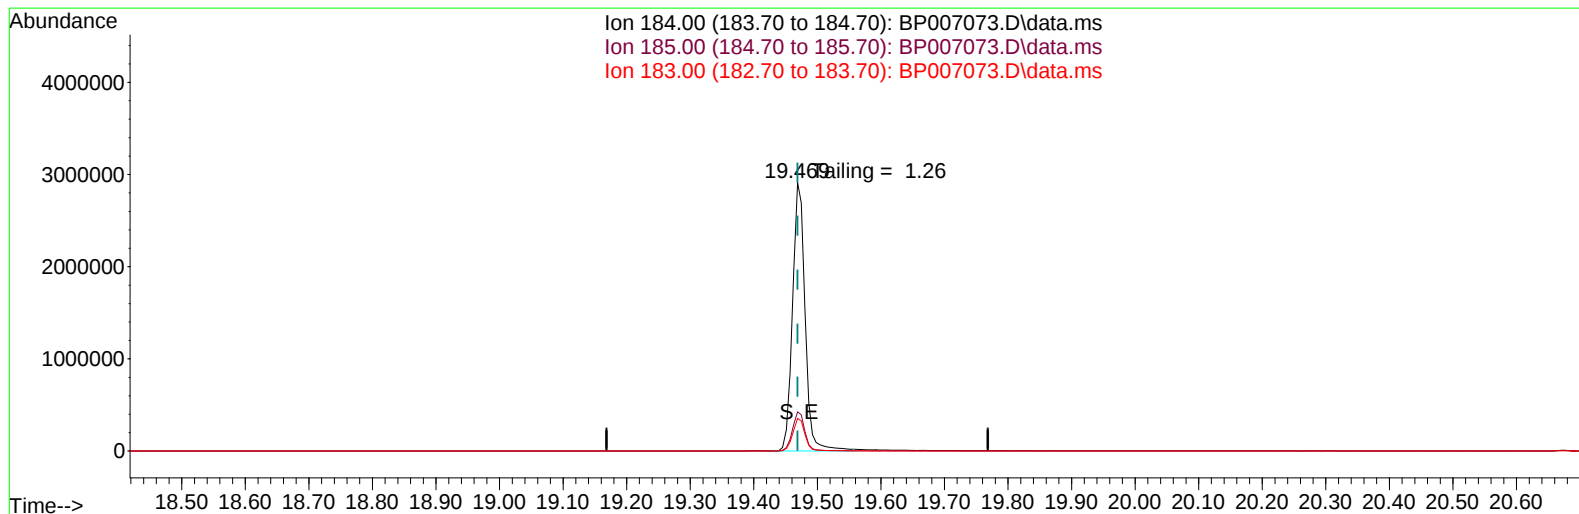

TIC: BP007073.D\data.ms

(77) Benzidine

19.469min (+ 0.000) -20.00 ng

response **4091161**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.60
183.00	11.90	12.14
0.00	0.00	0.00