
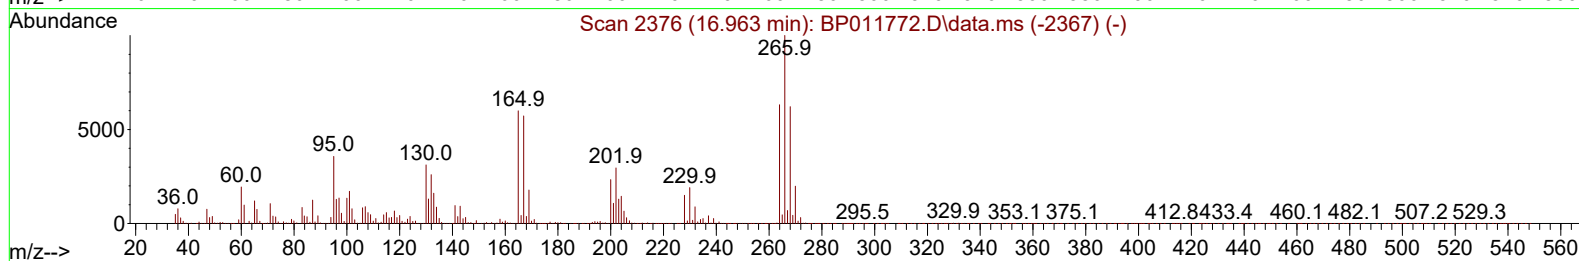
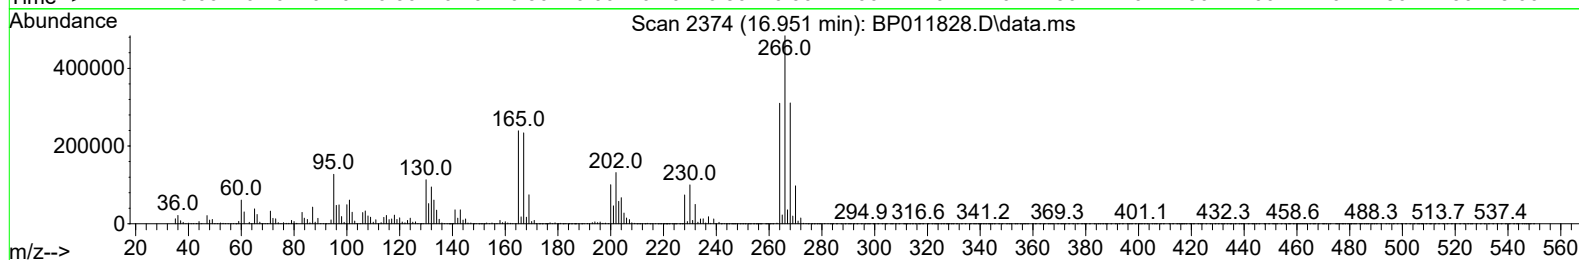


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092822\
 Data File : BP011828.D
 Acq On : 28 Sep 2022 13:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 05:34:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:03:33 2022
 Response via : Initial Calibration

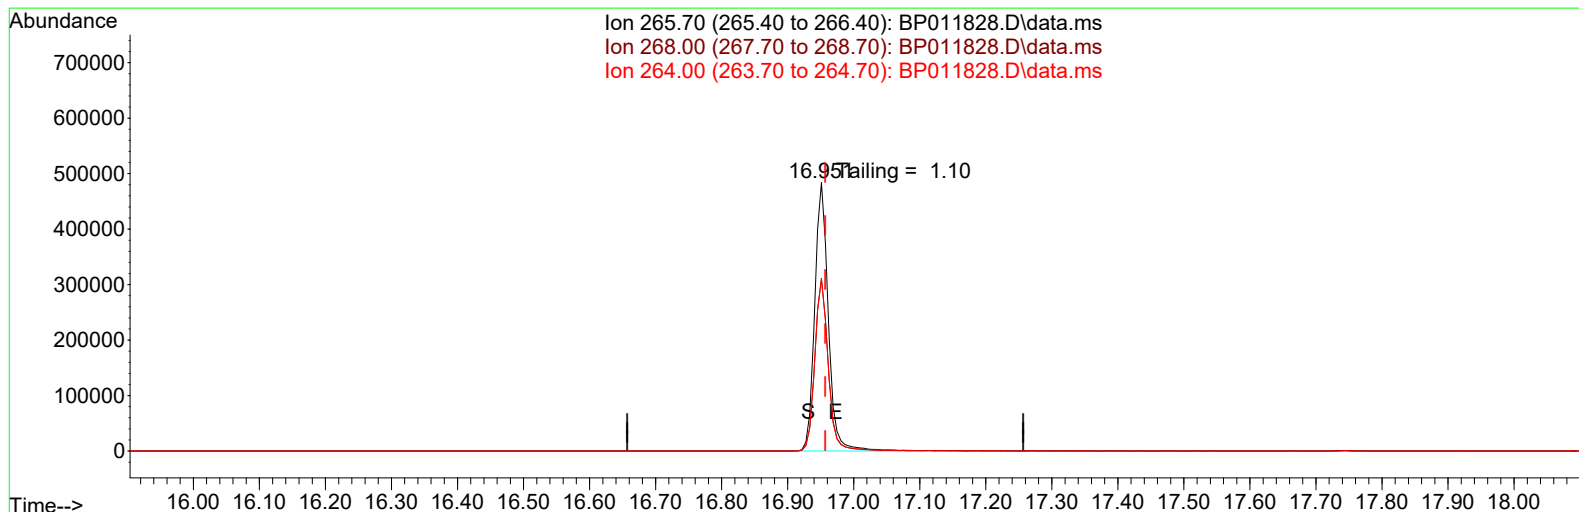

TIC: BP011828.D\data.ms

(70) Pentachlorophenol (C)




16.951min (-0.006) 261790.70 ng

response 691025

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	64.25
264.00	63.20	64.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092822\
 Data File : BP011828.D
 Acq On : 28 Sep 2022 13:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 05:34:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:03:33 2022
 Response via : Initial Calibration

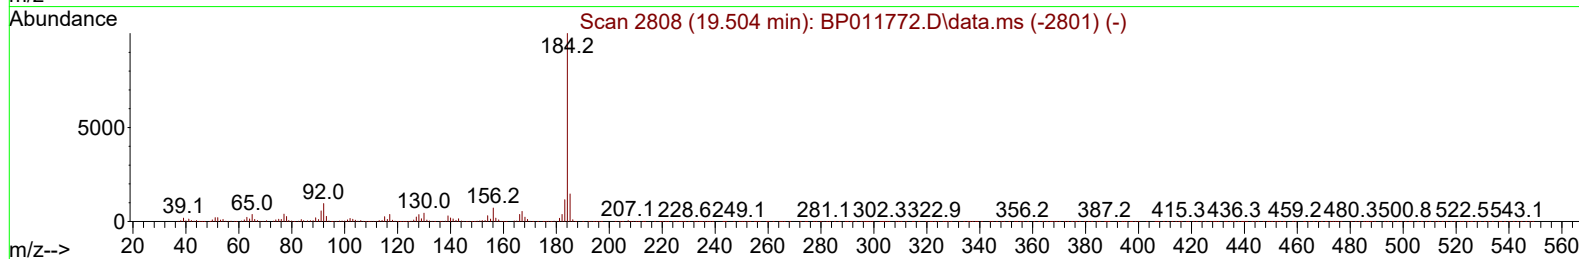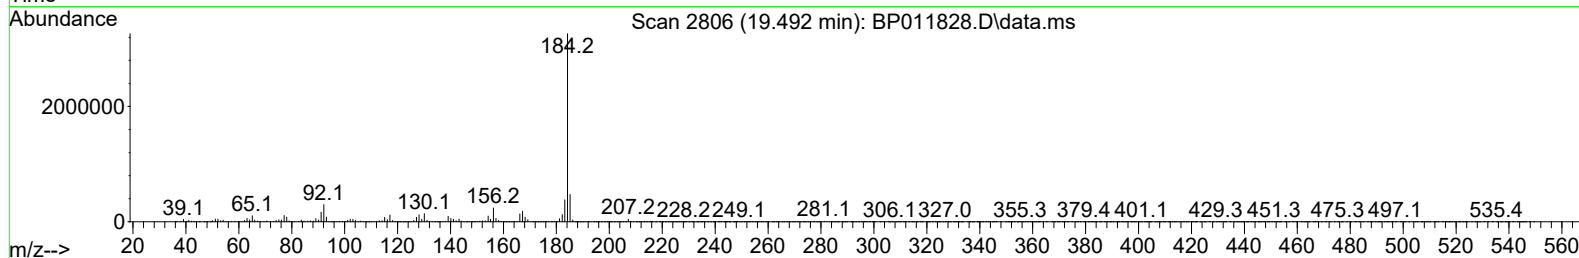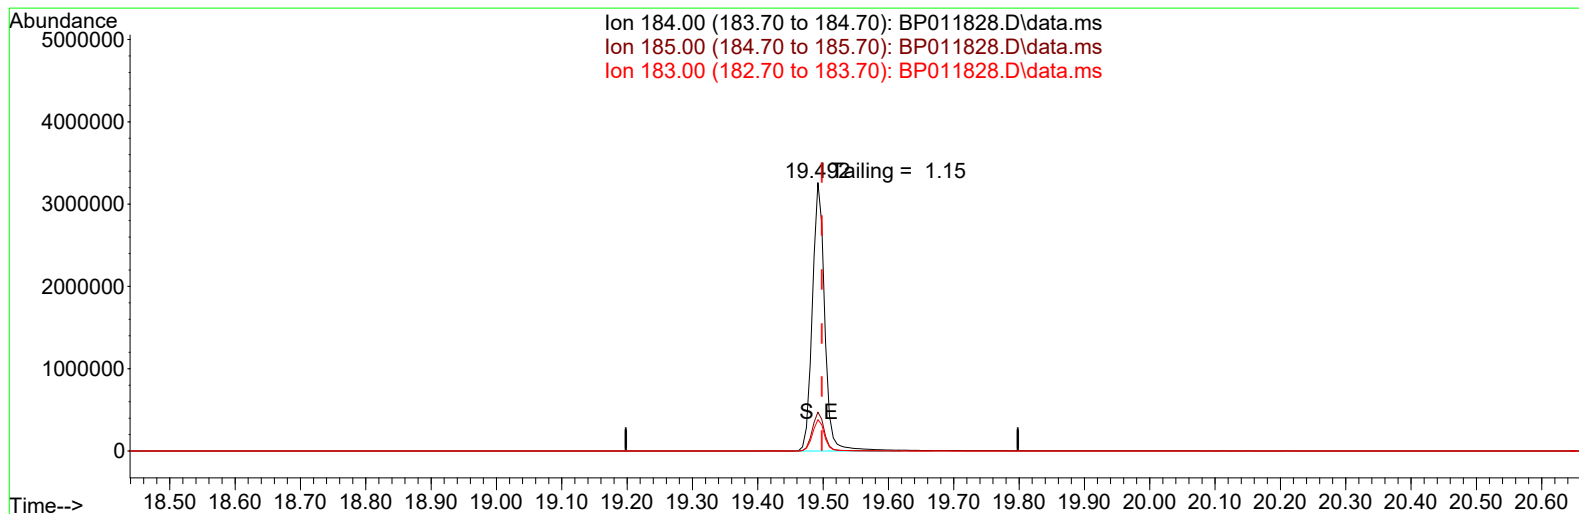

TIC: BP011828.D\data.ms

(77) Benzidine**19.492min (-0.006) 4195346.73 ng****response 4315443**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.50
183.00	11.60	11.68
0.00	0.00	0.00