

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019210.D
 Acq On : 02 Jan 2024 16:21
 Operator : MA/JU
 Sample : 05918-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF19

Quant Time: Jan 02 16:54:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	160276	20.000	ng/u1	0.00
20) Naphthalene-d8	10.593	136	531496	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.439	164	292938	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	648650	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	749200	20.000	ng/u1	0.00
88) Perylene-d12	23.663	264	972457	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	11857	2.527	ng/uL	0.00
4) Pyridine-d5	3.669	84	23694	2.012	ng/u1	0.02
7) Phenol-d5	6.981	99	194914	13.561	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	116780	14.044	ng/u1	0.00
11) 2-Chlorophenol-d4	7.328	132	161483	13.936	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	121648	10.871	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	73184	15.929	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	77959	15.700	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	146669	14.628	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	93176	7.555	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	402197	15.544	ng/u1	-0.01
49) Acenaphthylene-d8	14.134	160	467221	16.642	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	53797	12.313	ng/u1	0.00
60) Fluorene-d10	15.434	176	361430	16.169	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.563	200	45585	10.720	ng/u1	-0.01
73) Anthracene-d10	17.298	188	559383	16.513	ng/u1	0.00
81) Pyrene-d10	19.545	212	784819	17.189	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.515	264	938373	16.788	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.628	105	26058	1.555	ng/u1	95
71) Pentachlorophenol	16.851	266	159320	27.542	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019210.D
Acq On : 02 Jan 2024 16:21
Operator : MA/JU
Sample : 05918-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF19

Quant Time: Jan 02 16:54:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration




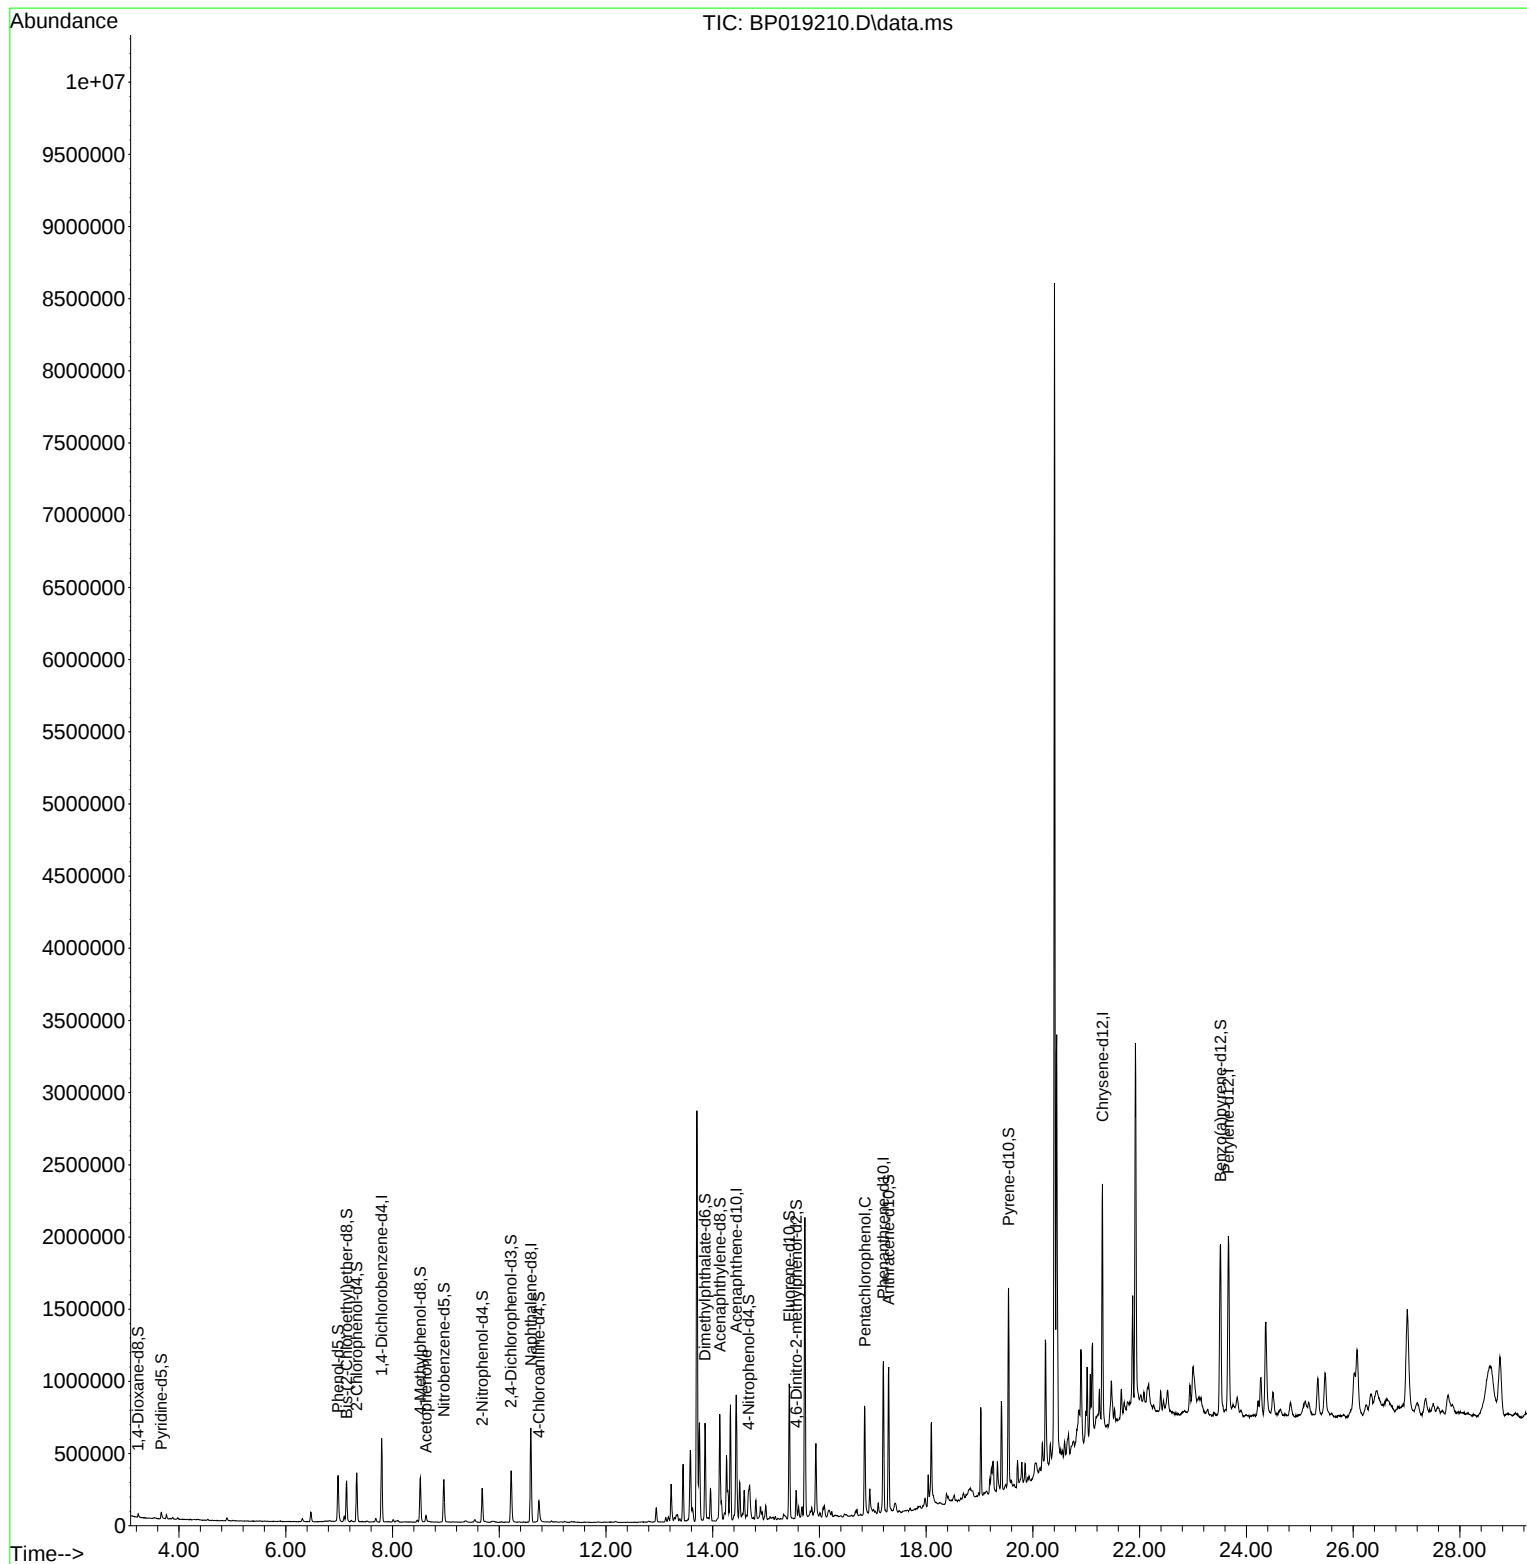


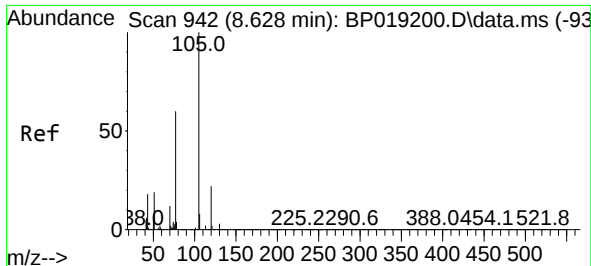

#16
Acetophenone
Concen: 1.555 ng/ul
RT: 8.628 min Scan# 942
Delta R.T. -0.006 min
Lab File: BP019210.D
Acq: 02 Jan 2024 16:21

Instrument :
BNA_P
ClientSampleId :
GCF19

Tgt Ion:	105	Resp:	26058
Ion	Ratio	Lower	Upper
105	100		
77	70.0	59.8	89.6
51	25.9	19.3	28.9

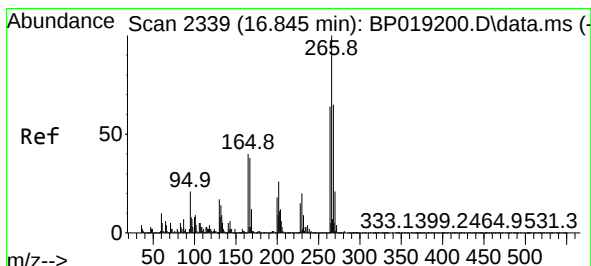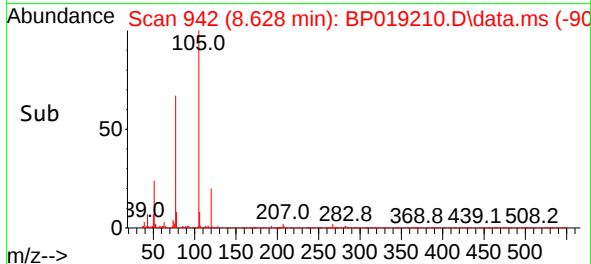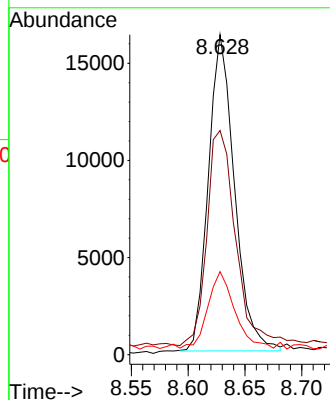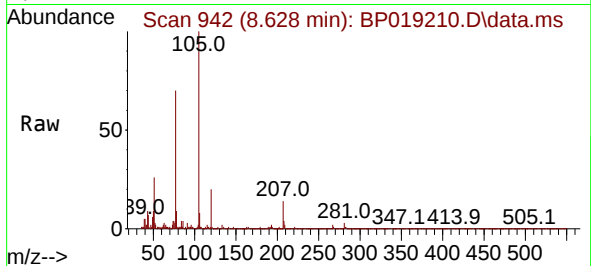

#71
Pentachlorophenol
Concen: 27.542 ng/ul
RT: 16.851 min Scan# 2340
Delta R.T. -0.000 min
Lab File: BP019210.D
Acq: 02 Jan 2024 16:21

Tgt Ion:	266	Resp:	159320
Ion	Ratio	Lower	Upper
266	100		
264	63.0	50.0	75.0
268	64.1	52.8	79.2

