

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019222.D
 Acq On : 02 Jan 2024 23:09
 Operator : MA/JU
 Sample : 05919-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF52

Quant Time: Jan 03 00:05:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	199362	20.000	ng/u1	0.00
20) Naphthalene-d8	10.593	136	767680	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.440	164	494798	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	1164169	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	1190294	20.000	ng/u1	-0.01
88) Perylene-d12	23.669	264	1393711	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	29012	4.970	ng/uL	0.00
4) Pyridine-d5	3.658	84	447358	30.533	ng/u1	0.00
7) Phenol-d5	6.981	99	765668	42.827	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	380446	36.783	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	555842	38.565	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	620548	44.583	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	284811	42.918	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	344960	48.098	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.222	165	678906	46.878	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	424460	23.828	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	2046036	46.815	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	2373096	50.042	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	374755	50.779	ng/u1	0.01
60) Fluorene-d10	15.440	176	1848981	48.971	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	312822	40.989	ng/u1	0.00
73) Anthracene-d10	17.298	188	2768062	45.530	ng/u1	0.00
81) Pyrene-d10	19.545	212	3714422	51.204	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.521	264	3846943	48.021	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	16.851	266	31481	3.032	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019222.D
Acq On : 02 Jan 2024 23:09
Operator : MA/JU
Sample : 05919-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF52

Quant Time: Jan 03 00:05:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

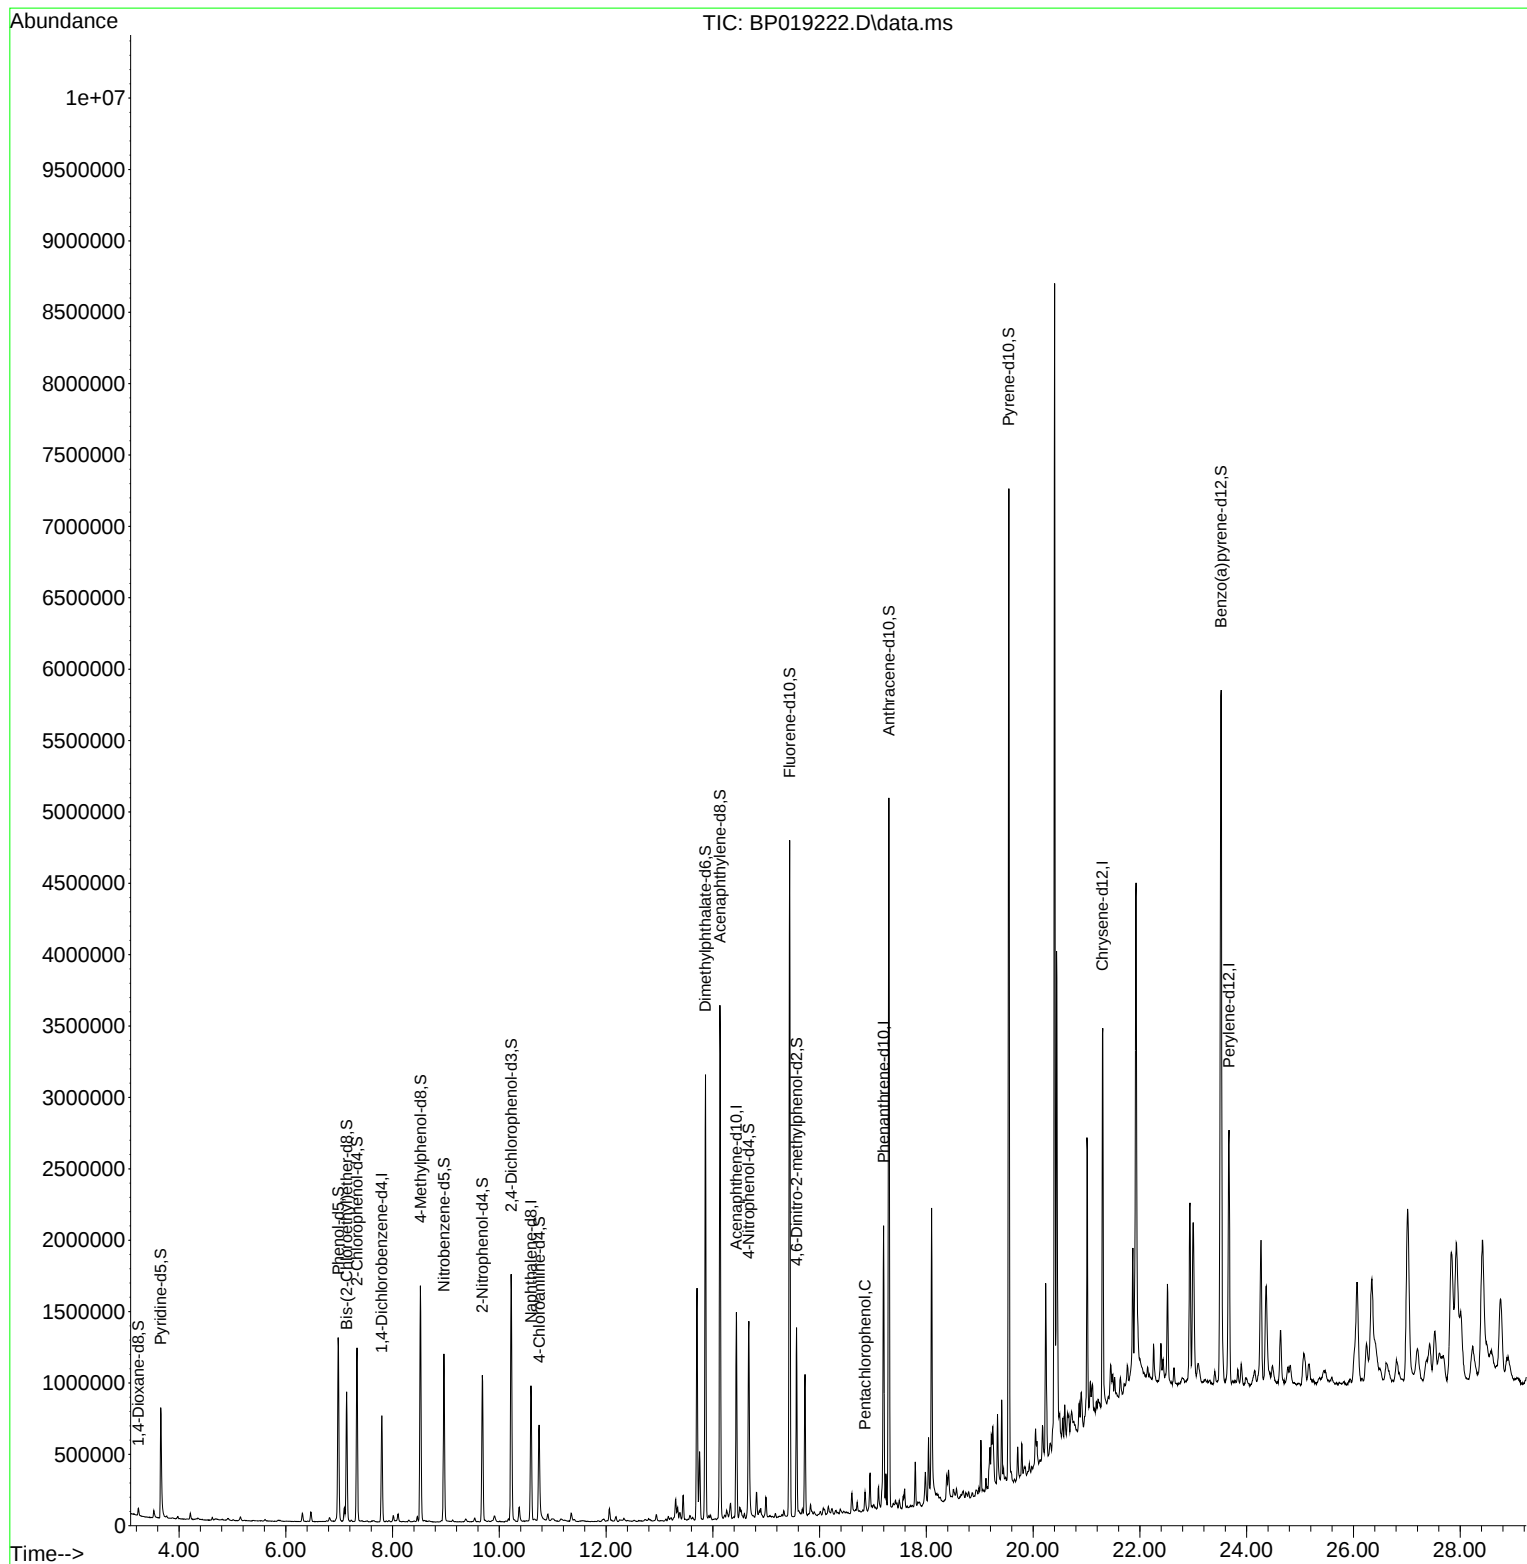

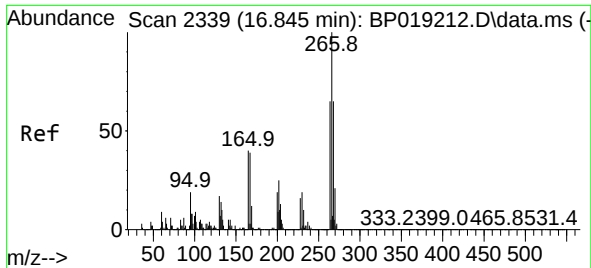

#71
 Pentachlorophenol
 Concen: 3.032 ng/ul
 RT: 16.851 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP019222.D
 Acq: 02 Jan 2024 23:09

Instrument :
 BNA_P
 ClientSampleId :
 GCF52

Tgt Ion:266 Resp: 31481
 Ion Ratio Lower Upper
 266 100
 264 60.2 50.0 75.0
 268 67.8 52.8 79.2

