

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019225.D
 Acq On : 03 Jan 2024 00:51
 Operator : MA/JU
 Sample : 05919-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF49

Quant Time: Jan 03 01:25:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	168168	20.000	ng/u1	0.00
20) Naphthalene-d8	10.598	136	634578	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	399559	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	955182	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	970431	20.000	ng/u1	0.00
88) Perylene-d12	23.668	264	1140584	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	31193	6.335	ng/uL	0.00
4) Pyridine-d5	3.663	84	371306	30.044	ng/u1	0.01
7) Phenol-d5	6.987	99	548431	36.366	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	308657	35.378	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	434587	35.745	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	410298	34.945	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	207090	37.752	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	241291	40.700	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	447050	37.343	ng/u1	0.00
31) 4-Chloroaniline-d4	10.745	131	153324	10.412	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	1254472	35.545	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	1477888	38.593	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	236054	39.609	ng/u1	0.02
60) Fluorene-d10	15.439	176	1147247	37.628	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	184513	29.466	ng/u1	0.00
73) Anthracene-d10	17.298	188	1748993	35.062	ng/u1	0.00
81) Pyrene-d10	19.545	212	2340921	39.581	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.521	264	2371080	36.166	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	16.851	266	55944	6.568	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019225.D
Acq On : 03 Jan 2024 00:51
Operator : MA/JU
Sample : 05919-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF49

Quant Time: Jan 03 01:25:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

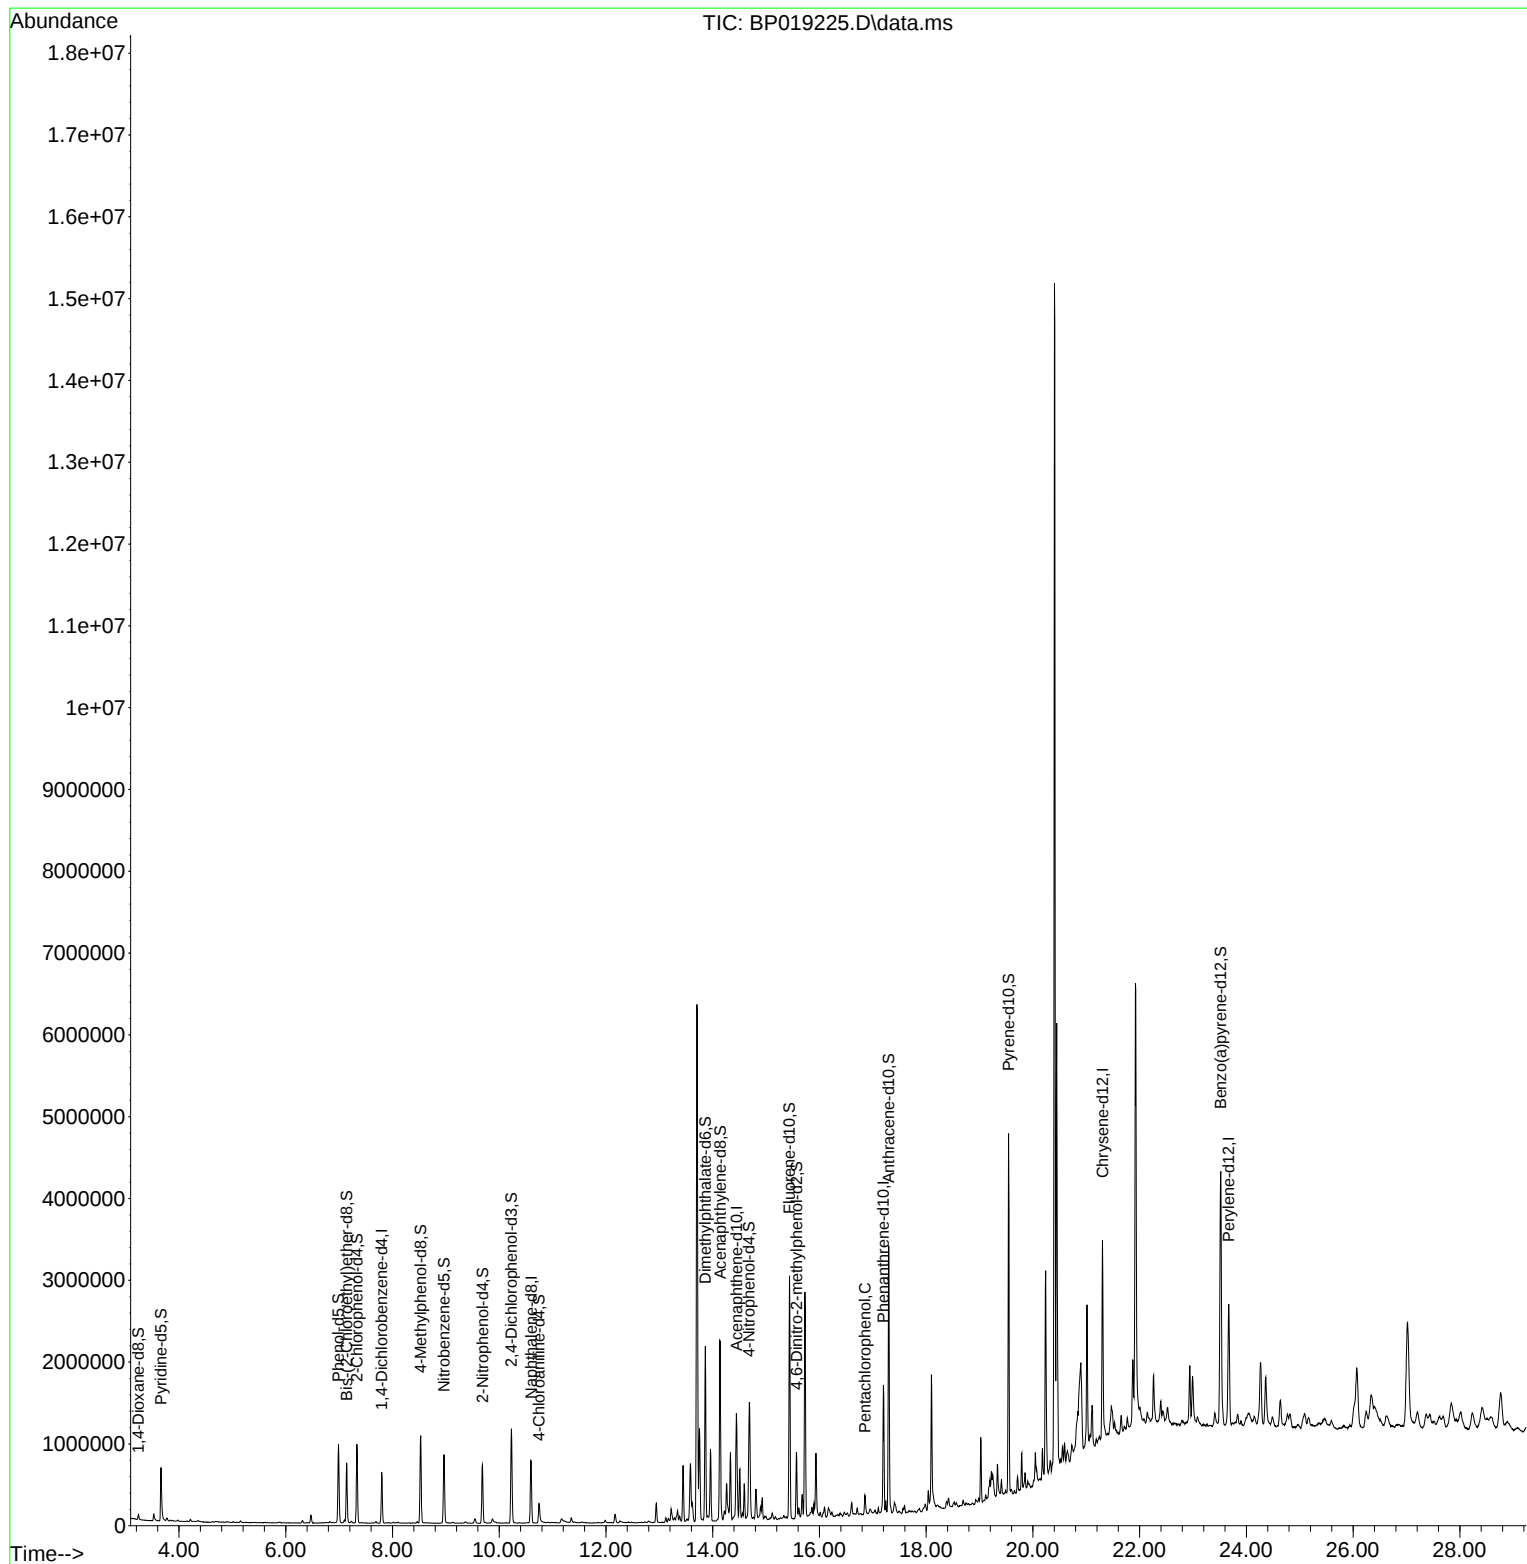

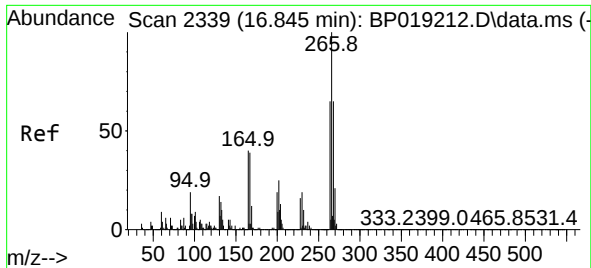

#71
 Pentachlorophenol
 Concen: 6.568 ng/ul
 RT: 16.851 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP019225.D
 Acq: 03 Jan 2024 00:51

Instrument :
 BNA_P
 ClientSampleId :
 GCF49

Tgt Ion:266 Resp: 55944
 Ion Ratio Lower Upper
 266 100
 264 65.1 50.0 75.0
 268 71.6 52.8 79.2

