

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019226.D
 Acq On : 03 Jan 2024 01:25
 Operator : MA/JU
 Sample : 05919-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF37

Quant Time: Jan 03 01:53:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	178815	20.000	ng/u1	0.00
20) Naphthalene-d8	10.593	136	691294	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.446	164	432840	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	1018440	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1035779	20.000	ng/u1	0.00
88) Perylene-d12	23.669	264	1251528	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	20695	3.953	ng/uL	0.00
4) Pyridine-d5	3.664	84	218735	16.645	ng/u1	0.01
7) Phenol-d5	6.987	99	374410	23.348	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	208618	22.488	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	298745	23.109	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	261324	20.932	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	139027	23.265	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	163121	25.257	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	307331	23.566	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	186936	11.653	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	874108	22.863	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	1031155	24.857	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	151429	23.456	ng/u1	0.02
60) Fluorene-d10	15.440	176	806082	24.405	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	120367	18.028	ng/u1	0.00
73) Anthracene-d10	17.298	188	1239297	23.301	ng/u1	0.00
81) Pyrene-d10	19.545	212	1601749	25.374	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	1674606	23.279	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	16.851	266	33241	3.660	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019226.D
Acq On : 03 Jan 2024 01:25
Operator : MA/JU
Sample : 05919-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF37

Quant Time: Jan 03 01:53:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

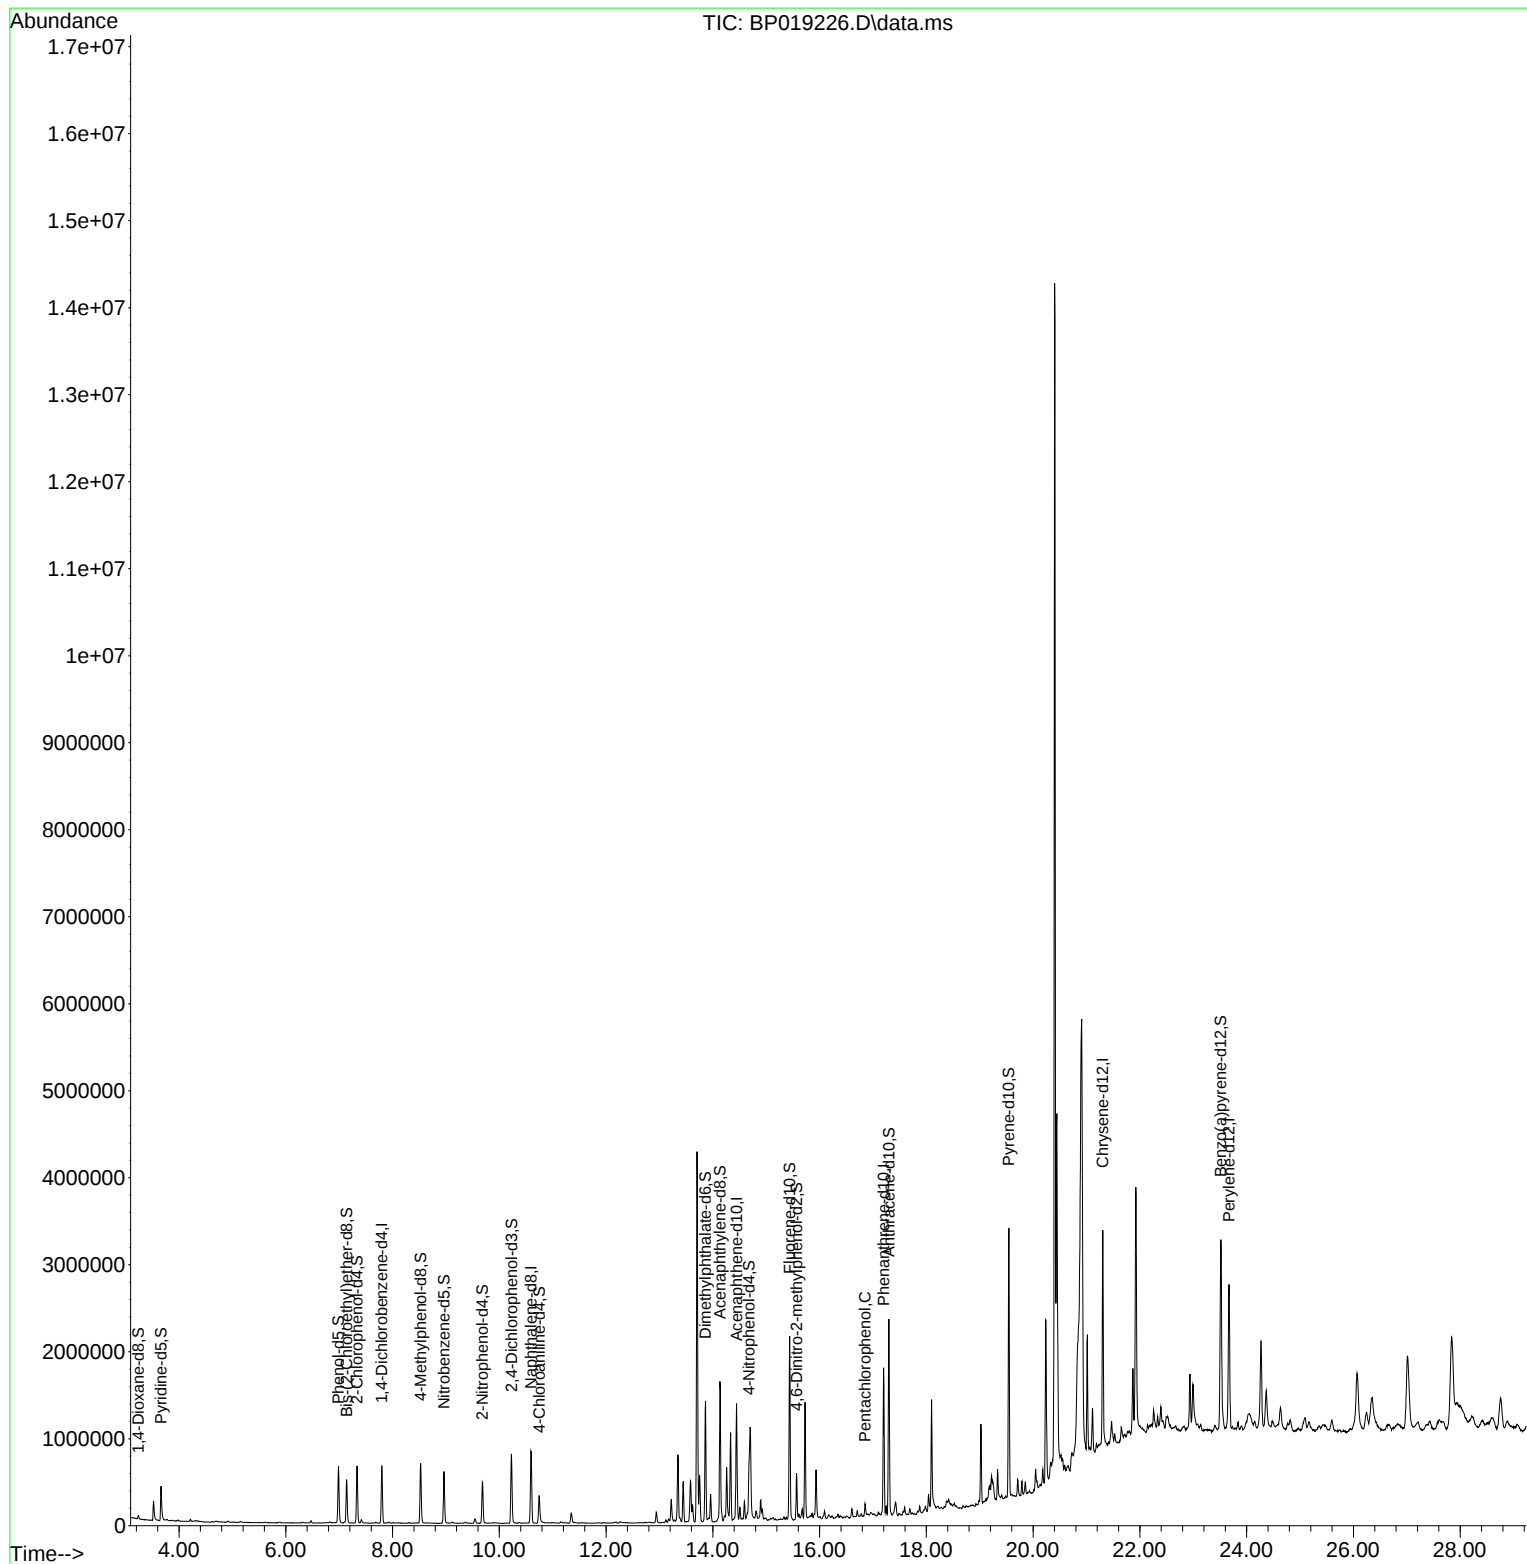

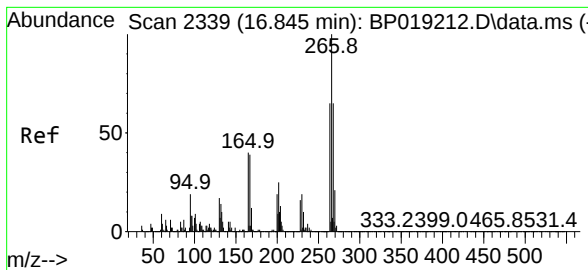

#71
 Pentachlorophenol
 Concen: 3.660 ng/ul
 RT: 16.851 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP019226.D
 Acq: 03 Jan 2024 01:25

Instrument :
 BNA_P
 ClientSampleId :
 GCF37

Tgt Ion:266 Resp: 33241
 Ion Ratio Lower Upper
 266 100
 264 65.3 50.0 75.0
 268 65.3 52.8 79.2

