

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019227.D
 Acq On : 03 Jan 2024 01:59
 Operator : MA/JU
 Sample : 05919-21
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF53

Quant Time: Jan 03 04:35:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	155951	20.000	ng/u1	0.00
20) Naphthalene-d8	10.593	136	586677	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.446	164	361204	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	860478	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	947288	20.000	ng/u1	0.00
88) Perylene-d12	23.669	264	1108297	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	27918	6.114	ng/uL	0.00
4) Pyridine-d5	3.652	84	373538	32.592	ng/u1	0.00
7) Phenol-d5	6.987	99	474039	33.895	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	271508	33.558	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	378296	33.553	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	370051	33.987	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	177180	34.936	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	207275	37.817	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	383952	34.691	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	429856	31.575	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	1085272	34.016	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	1295074	37.410	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	195529	36.293	ng/u1	0.02
60) Fluorene-d10	15.440	176	995095	36.103	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	142854	25.324	ng/u1	0.00
73) Anthracene-d10	17.298	188	1559818	34.711	ng/u1	0.00
81) Pyrene-d10	19.545	212	2078218	35.998	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	2266785	35.583	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.851	266	184914	24.097	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019227.D
Acq On : 03 Jan 2024 01:59
Operator : MA/JU
Sample : 05919-21
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF53

Quant Time: Jan 03 04:35:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

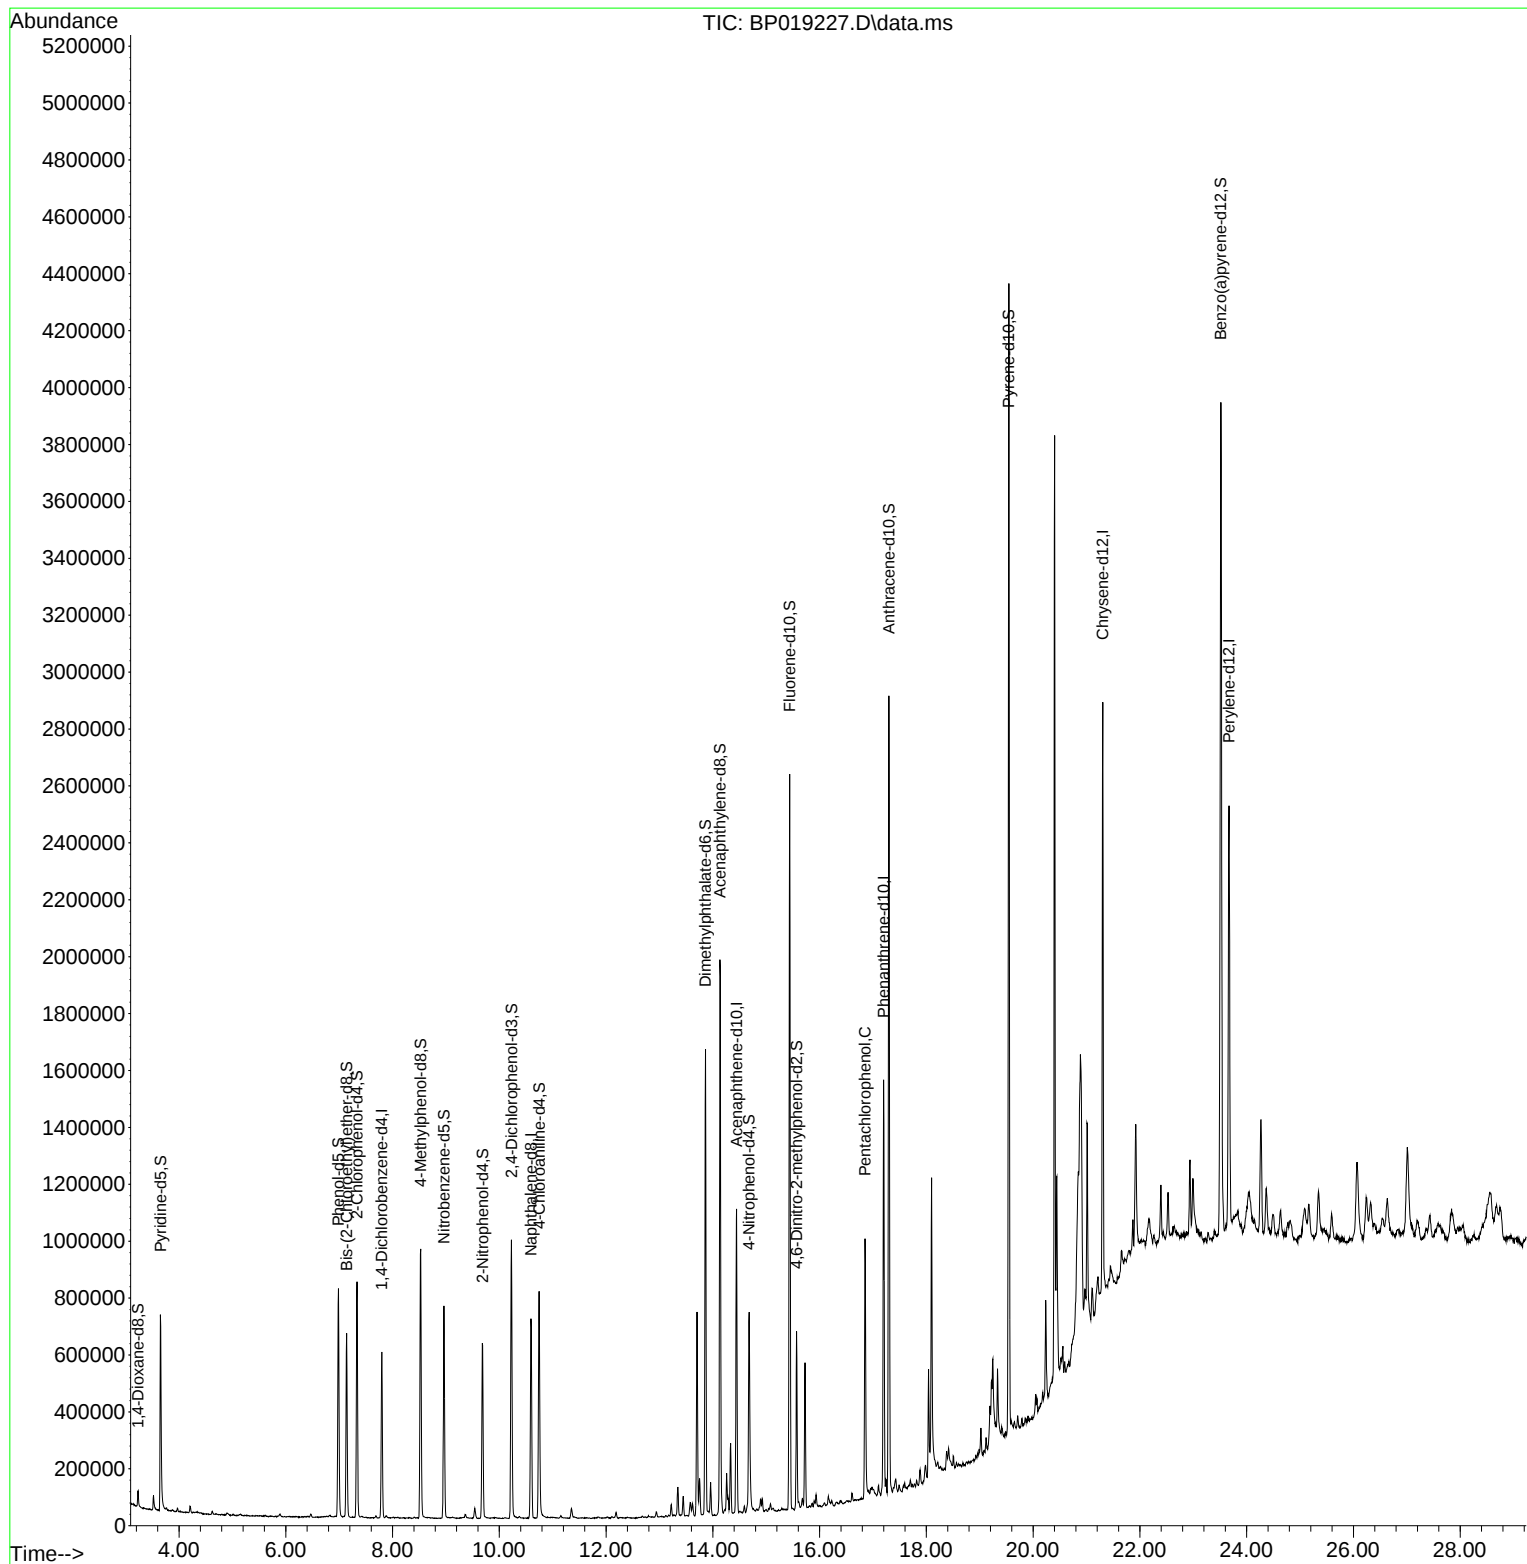

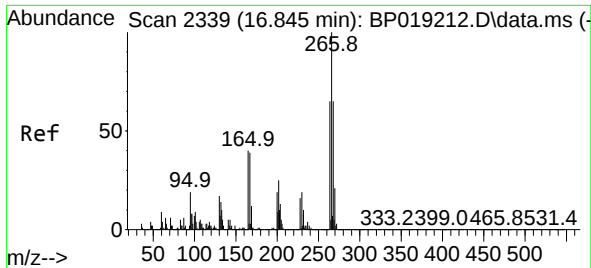

#71
 Pentachlorophenol
 Concen: 24.097 ng/ul
 RT: 16.851 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP019227.D
 Acq: 03 Jan 2024 01:59

Instrument :
 BNA_P
 ClientSampleId :
 GCF53

Tgt Ion:266 Resp: 184914
 Ion Ratio Lower Upper
 266 100
 264 63.5 50.0 75.0
 268 64.1 52.8 79.2

