

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019228.D
 Acq On : 03 Jan 2024 02:33
 Operator : MA/JU
 Sample : 05919-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF41

Quant Time: Jan 03 04:34:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	178183	20.000	ng/u1	0.00
20) Naphthalene-d8	10.598	136	688283	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	434736	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	998709	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	994557	20.000	ng/u1	0.00
88) Perylene-d12	23.668	264	1159957	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	24052	4.610	ng/uL	0.00
4) Pyridine-d5	3.658	84	304030	23.217	ng/u1	0.00
7) Phenol-d5	6.987	99	453360	28.372	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	250585	27.108	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	351233	27.266	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	346485	27.852	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	167376	28.131	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	194754	30.287	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	371968	28.647	ng/u1	0.00
31) 4-Chloroaniline-d4	10.745	131	325361	20.372	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	1071998	27.917	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	1258466	30.204	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	168199	25.940	ng/u1	0.02
60) Fluorene-d10	15.439	176	974556	29.377	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	122160	18.658	ng/u1	0.00
73) Anthracene-d10	17.298	188	1463976	28.069	ng/u1	0.00
81) Pyrene-d10	19.545	212	1896074	31.282	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.515	264	1929569	28.940	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	16.857	266	45003	5.053	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019228.D
Acq On : 03 Jan 2024 02:33
Operator : MA/JU
Sample : 05919-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF41

Quant Time: Jan 03 04:34:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

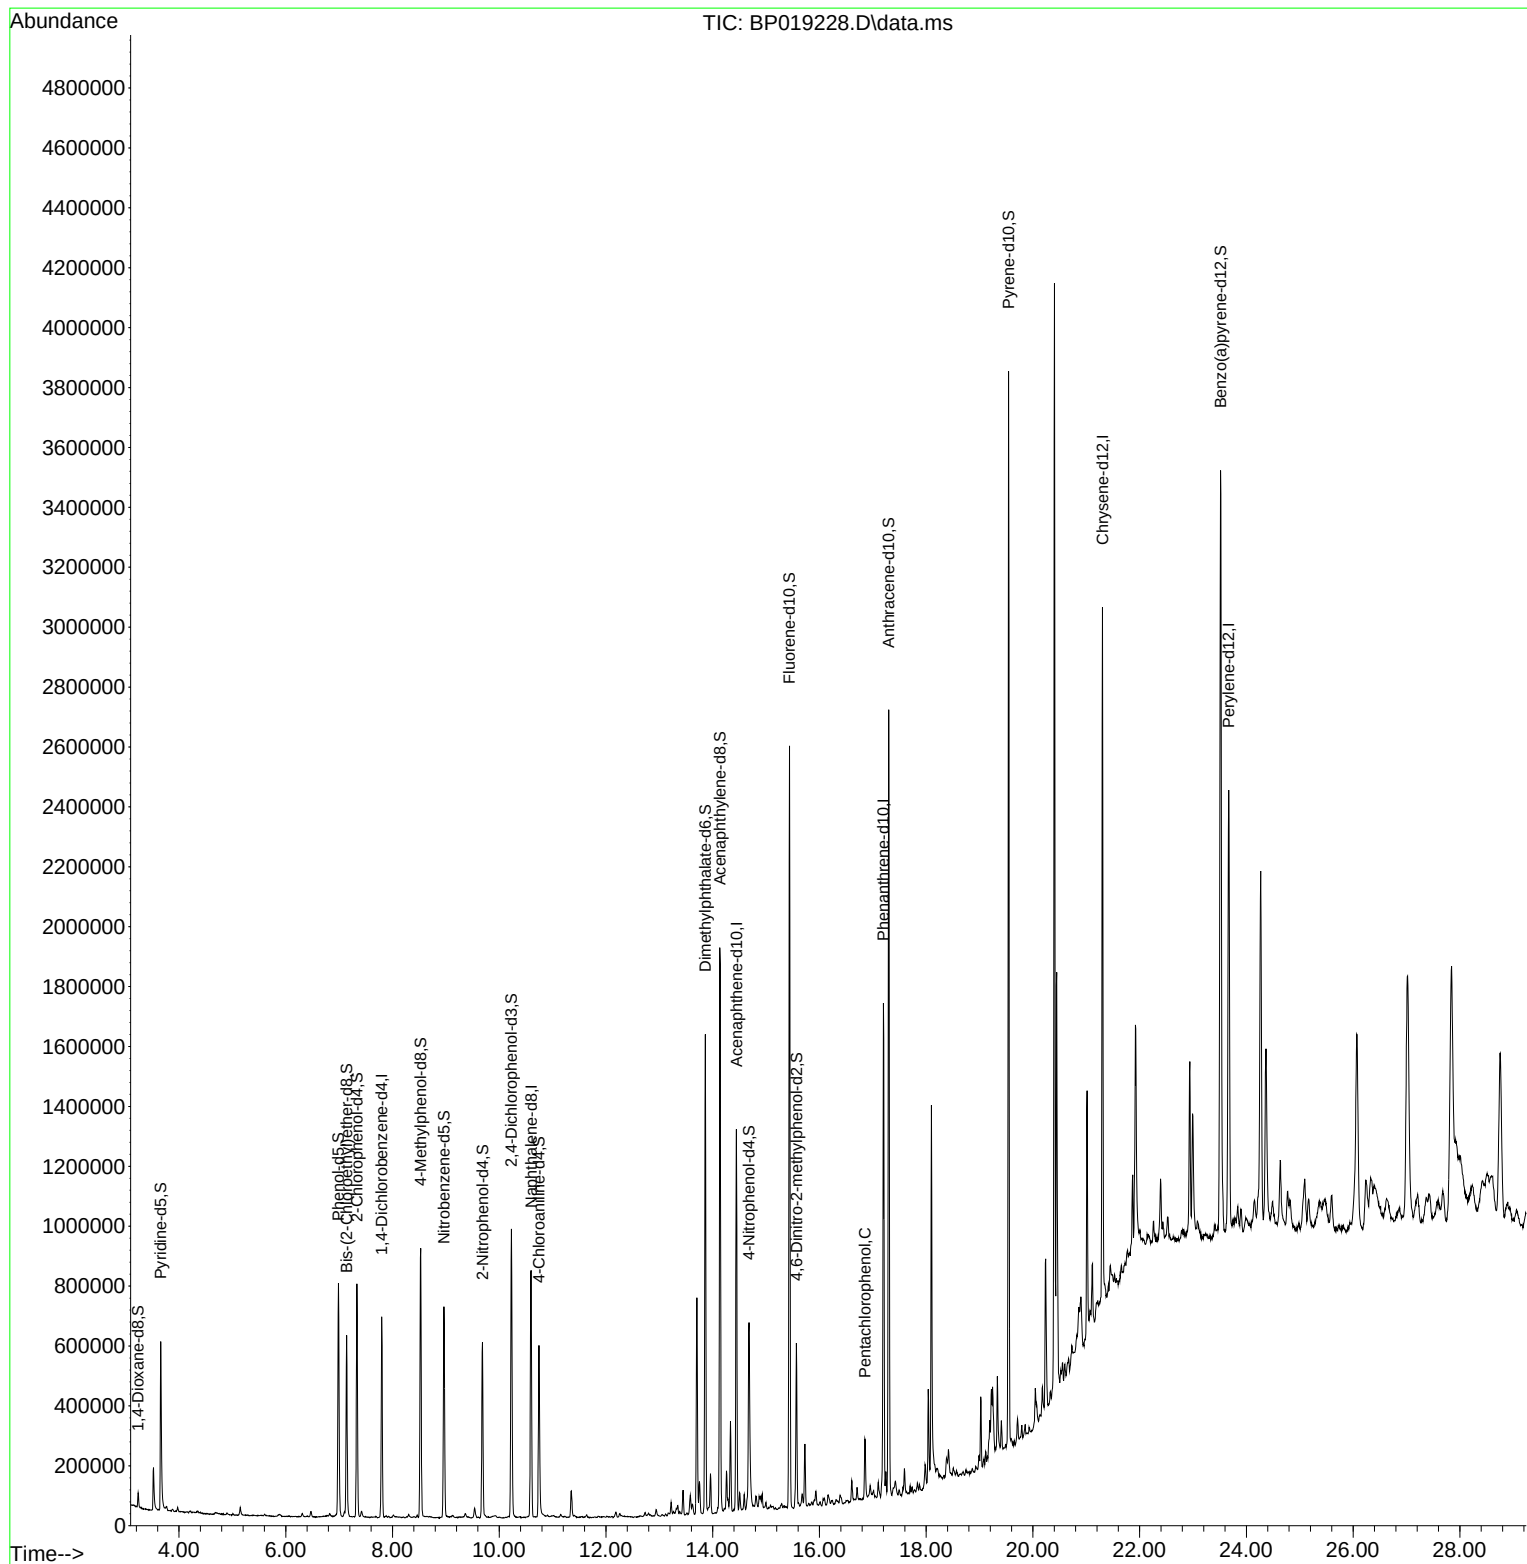

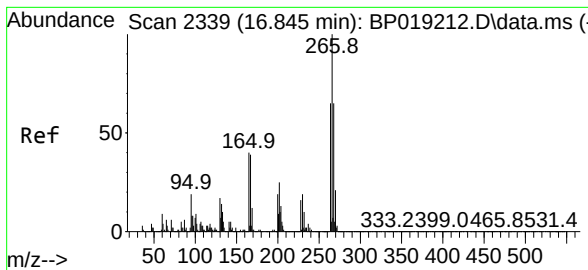

#71
 Pentachlorophenol
 Concen: 5.053 ng/ul
 RT: 16.857 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP019228.D
 Acq: 03 Jan 2024 02:33

Instrument :
 BNA_P
 ClientSampleId :
 GCF41

Tgt Ion:	266	Resp:	45003
Ion	Ratio	Lower	Upper
266	100		
264	64.7	50.0	75.0
268	68.2	52.8	79.2

