

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019240.D
 Acq On : 03 Jan 2024 09:53
 Operator : MA/JU
 Sample : 05952-10
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF93

Quant Time: Jan 03 11:21:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	208026	20.000	ng/u1	0.00
20) Naphthalene-d8	10.599	136	796774	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	502292	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	1135442	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1133114	20.000	ng/u1	0.00
88) Perylene-d12	23.674	264	1367082	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	18790	3.085	ng/uL	0.00
4) Pyridine-d5	3.658	84	156365	10.228	ng/u1	0.00
7) Phenol-d5	6.987	99	397231	21.293	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	221178	20.494	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	311209	20.693	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	264443	18.207	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	148305	21.532	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	171233	23.004	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	316884	21.082	ng/u1	0.00
31) 4-Chloroaniline-d4	10.752	131	108038	5.843	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	941620	21.224	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1091157	22.666	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	152291	20.328	ng/u1	0.02
60) Fluorene-d10	15.440	176	847578	22.113	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	119707	16.082	ng/u1	0.00
73) Anthracene-d10	17.298	188	1233941	20.810	ng/u1	0.00
81) Pyrene-d10	19.545	212	1668704	24.164	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	1662099	21.152	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.857	266	225710	22.290	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019240.D
Acq On : 03 Jan 2024 09:53
Operator : MA/JU
Sample : 05952-10
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF93

Quant Time: Jan 03 11:21:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

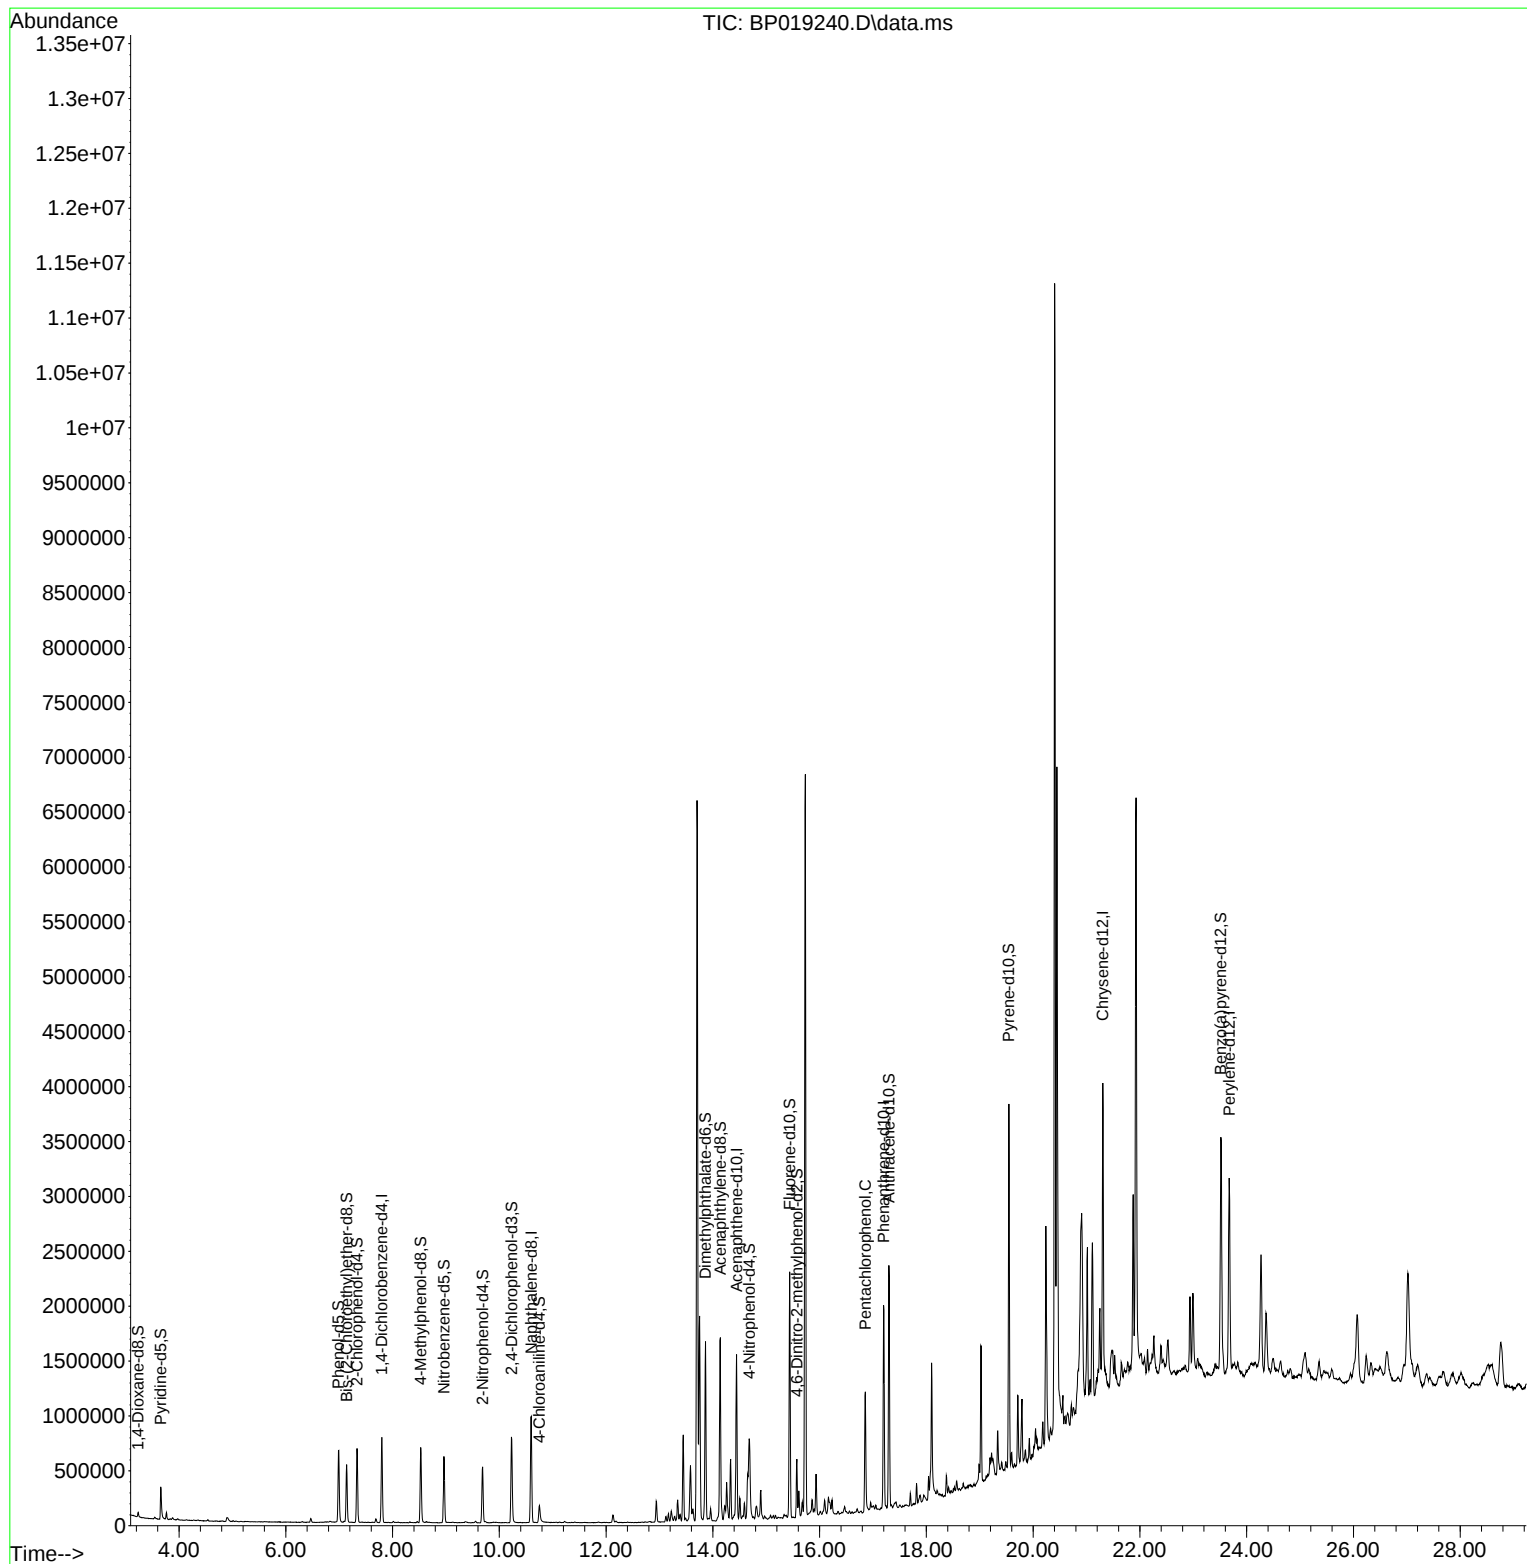

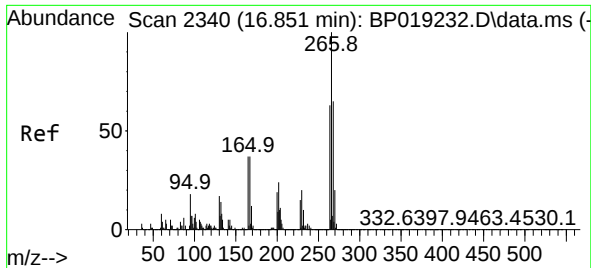

#71
 Pentachlorophenol
 Concen: 22.290 ng/ul
 RT: 16.857 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP019240.D
 Acq: 03 Jan 2024 09:53

Instrument :
 BNA_P
 ClientSampleId :
 GCF93

Tgt Ion:266 Resp: 225710
 Ion Ratio Lower Upper
 266 100
 264 64.6 50.0 75.0
 268 64.9 52.8 79.2

