

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019243.D
 Acq On : 03 Jan 2024 11:36
 Operator : MA/JU
 Sample : 05952-15
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF98

Quant Time: Jan 03 12:02:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.799	152	181082	20.000	ng/u1	0.00
20) Naphthalene-d8	10.599	136	680776	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	440235	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	1061243	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1069194	20.000	ng/u1	0.00
88) Perylene-d12	23.674	264	1278688	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	21230	4.004	ng/uL	0.00
4) Pyridine-d5	3.664	84	184089	13.833	ng/u1	0.01
7) Phenol-d5	6.993	99	367925	22.657	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.140	67	212817	22.653	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	296281	22.632	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	253361	20.040	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	140382	23.855	ng/u1	0.00
24) 2-Nitrophenol-d4	9.687	143	163794	25.753	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	303299	23.616	ng/u1	0.00
31) 4-Chloroaniline-d4	10.752	131	109611	6.939	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	875339	22.511	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1033792	24.502	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	150114	22.861	ng/u1	0.02
60) Fluorene-d10	15.439	176	817924	24.348	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	117308	16.861	ng/u1	0.00
73) Anthracene-d10	17.298	188	1303170	23.514	ng/u1	0.00
81) Pyrene-d10	19.545	212	1664203	25.540	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.521	264	1695012	23.062	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.857	266	300105	31.710	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019243.D
Acq On : 03 Jan 2024 11:36
Operator : MA/JU
Sample : 05952-15
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF98

Quant Time: Jan 03 12:02:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

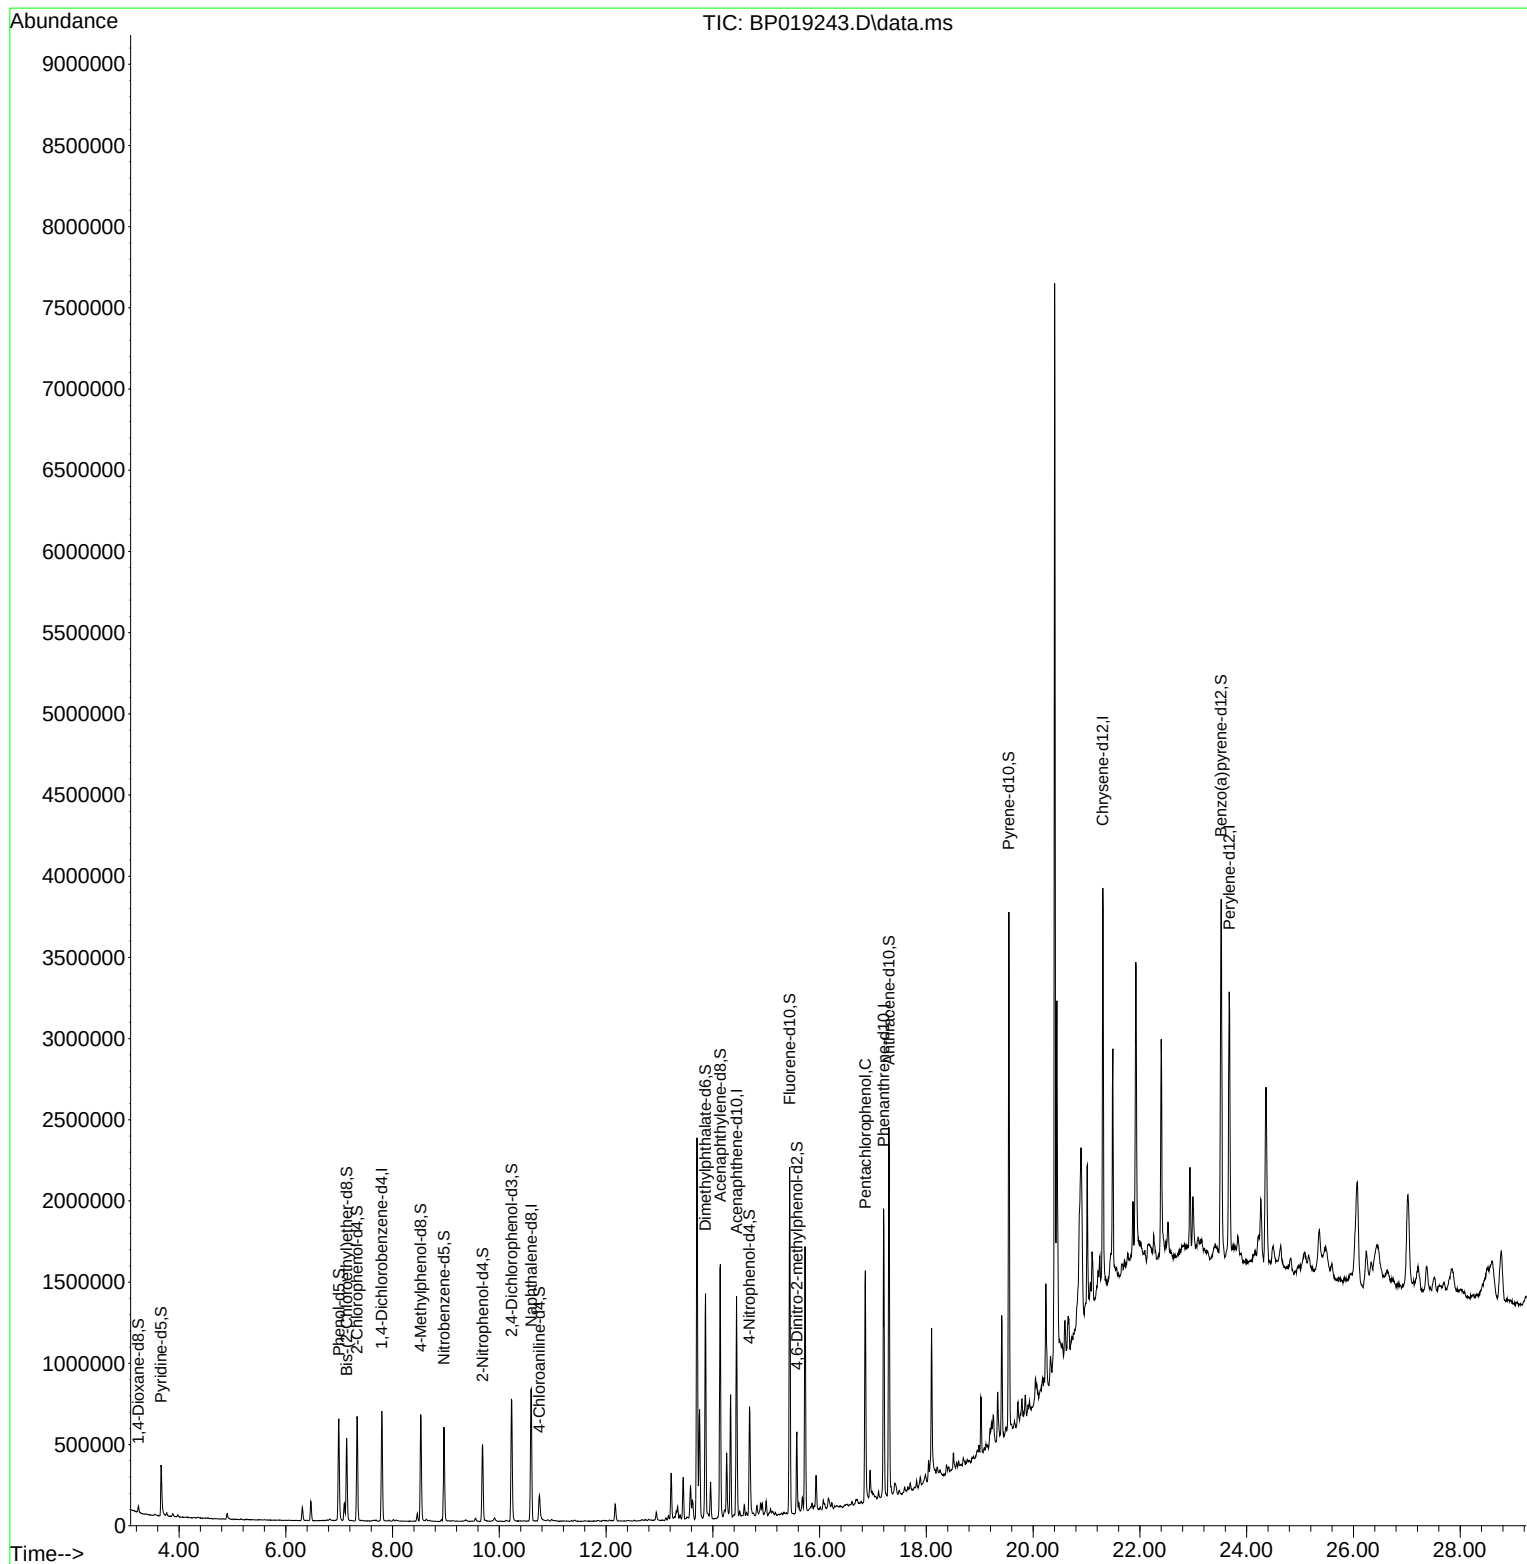

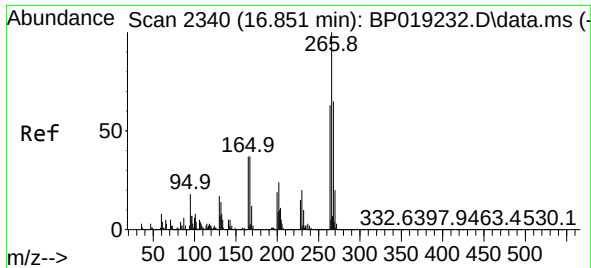

#71
Pentachlorophenol
Concen: 31.710 ng/ul
RT: 16.857 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP019243.D
Acq: 03 Jan 2024 11:36

Instrument :
BNA_P
ClientSampleId :
GCF98

Tgt Ion:266 Resp: 300105
Ion Ratio Lower Upper
266 100
264 63.1 50.0 75.0
268 64.6 52.8 79.2

