

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019201.D
 Acq On : 02 Jan 2024 10:59
 Operator : MA/JU
 Sample : PB158064BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	32	rVB	59812	74554	1.84%	0.204%
2	3.652	92	96	108	rBV	651154	931481	22.93%	2.543%
3	3.975	148	151	160	rVB2	14092	22667	0.56%	0.062%
4	5.222	361	363	368	rVB6	3075	4858	0.12%	0.013%
5	6.287	541	544	547	rVB4	3310	4254	0.10%	0.012%
6	6.975	654	661	671	rBV	671187	1049903	25.85%	2.867%
7	7.140	681	689	702	rBV	559464	871775	21.46%	2.380%
8	7.328	714	721	732	rBV	697383	1077752	26.54%	2.943%
9	7.799	793	801	813	rBV	579743	907106	22.33%	2.477%
10	8.516	916	923	940	rBV	771364	1249529	30.76%	3.412%
11	8.963	991	999	1012	rBV	586961	954457	23.50%	2.606%
12	9.681	1114	1121	1132	rBV	425967	715518	17.62%	1.954%
13	10.222	1205	1213	1228	rBV	699449	1220804	30.06%	3.333%
14	10.593	1268	1276	1288	rBV	716313	1172193	28.86%	3.201%
15	10.740	1292	1301	1315	rBV	676820	1196617	29.46%	3.267%
16	11.857	1486	1491	1493	rBV6	2566	4512	0.11%	0.012%
17	12.204	1545	1550	1561	rVB4	8246	18210	0.45%	0.050%
18	13.340	1739	1743	1751	rVB9	7401	13438	0.33%	0.037%
19	13.857	1825	1831	1842	rBV	1092104	1547078	38.09%	4.224%
20	14.134	1871	1878	1890	rBV	1358102	1941742	47.81%	5.302%
21	14.440	1923	1930	1941	rBV	958757	1431902	35.25%	3.910%
22	14.657	1961	1967	1990	rBV	317299	641183	15.79%	1.751%
23	15.434	2092	2099	2110	rBV	1690661	2499703	61.54%	6.825%
24	15.563	2114	2121	2132	rBV	365606	532005	13.10%	1.453%
25	15.681	2137	2141	2147	rVB6	9289	14796	0.36%	0.040%
26	16.239	2229	2236	2243	rBV7	14182	28313	0.70%	0.077%
27	16.675	2306	2310	2315	rBV6	3293	6749	0.17%	0.018%
28	16.981	2359	2362	2367	rBV5	3842	5915	0.15%	0.016%
29	17.198	2392	2399	2405	rBV	1150647	1663308	40.95%	4.542%
30	17.298	2409	2416	2431	rBV	1851383	2690213	66.24%	7.345%
31	17.733	2488	2490	2494	rBV5	3044	4269	0.11%	0.012%
32	17.869	2511	2513	2515	rBV3	4381	4402	0.11%	0.012%
33	18.092	2548	2551	2552	rBV3	5132	5078	0.13%	0.014%
34	19.116	2722	2725	2730	rBV3	23488	30227	0.74%	0.083%
35	19.186	2734	2737	2741	rVV	20578	26065	0.64%	0.071%
36	19.539	2791	2797	2806	rBV	2661636	3390138	83.47%	9.257%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019201.D
Acq On : 02 Jan 2024 10:59
Operator : MA/JU
Sample : PB158064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	21.298	3091	3096	3103	rBV	1672154	2157550	53.12%	5.891%
38	23.504	3465	3471	3484	rVB2	2165468	4061617	100.00%	11.090%
39	23.657	3491	3497	3511	rVB	1199260	2452222	60.38%	6.696%




Sum of corrected areas: 36624103

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP019201.D
Data File : BP019201.D
Acq On : 02 Jan 2024 10:59
Operator : MA/JU
Sample : PB158064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

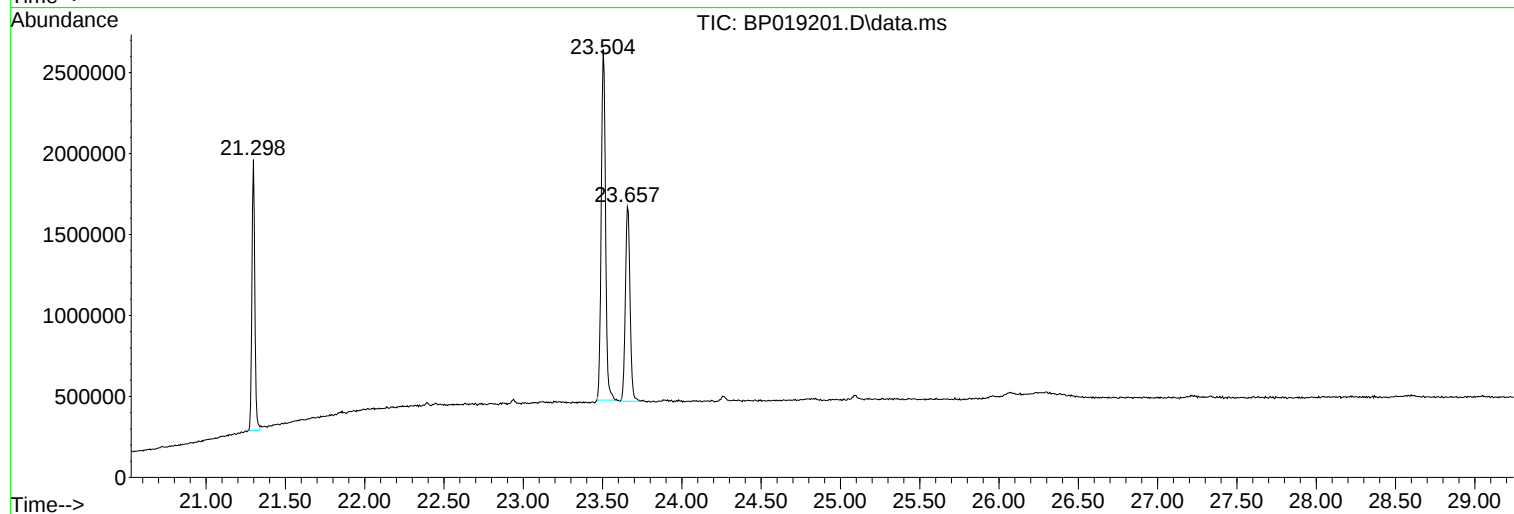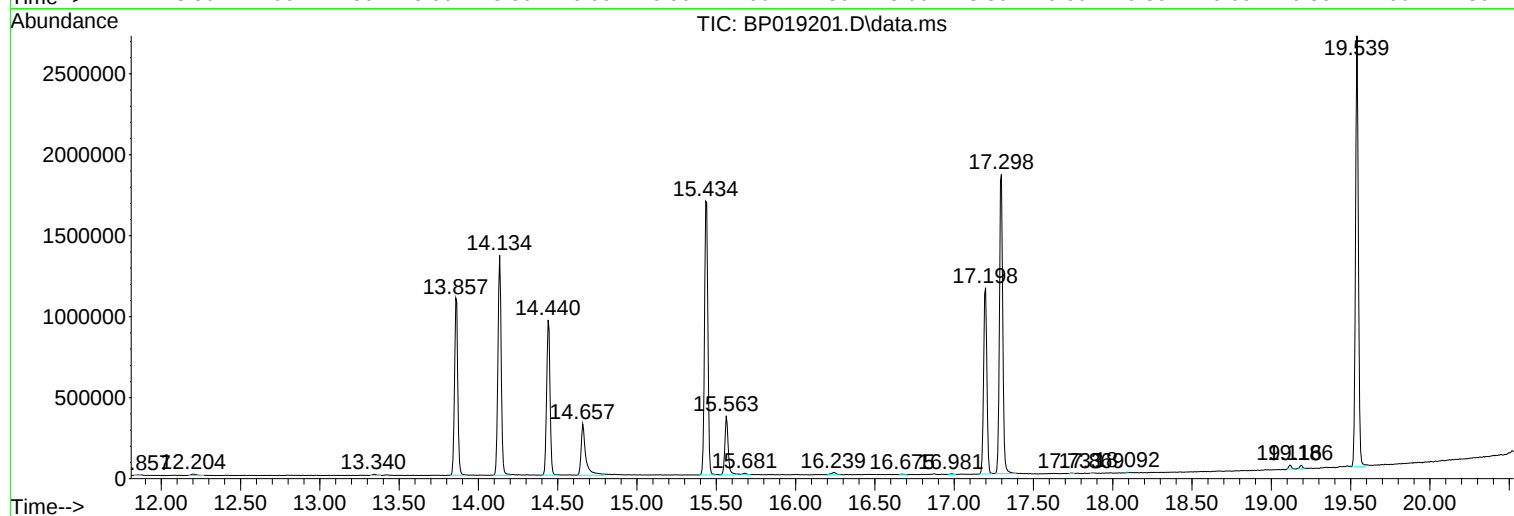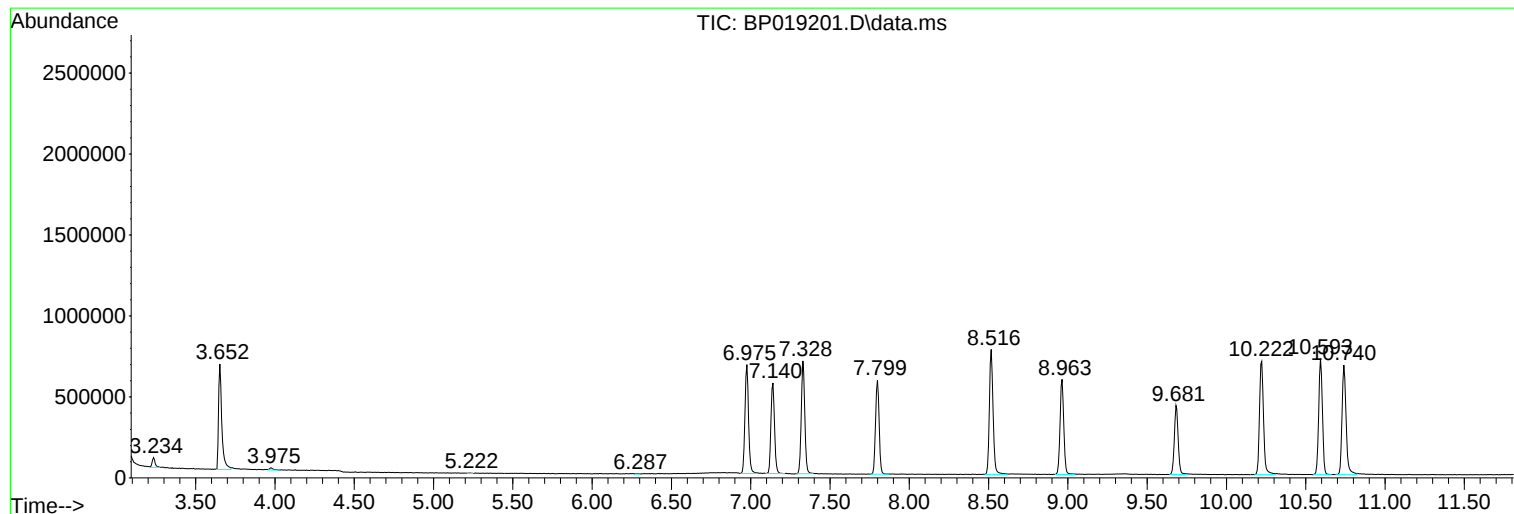

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019201.D
Acq On : 02 Jan 2024 10:59
Operator : MA/JU
Sample : PB158064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019201.D
Acq On : 02 Jan 2024 10:59
Operator : MA/JU
Sample : PB158064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------