

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019213.D
 Acq On : 02 Jan 2024 18:03
 Operator : MA/JU
 Sample : PB158101BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK101

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	36	rVB	56336	85494	1.83%	0.233%
2	3.658	93	97	113	rBV	563541	873288	18.70%	2.380%
3	3.975	148	151	157	rVB	9457	13164	0.28%	0.036%
4	6.975	655	661	673	rVB	639259	1017691	21.79%	2.773%
5	7.140	682	689	697	rBV	507900	800499	17.14%	2.182%
6	7.328	714	721	735	rBV	665530	1050731	22.50%	2.864%
7	7.799	791	801	808	rBV	461100	725954	15.54%	1.978%
8	8.516	914	923	936	rBV	752941	1217481	26.07%	3.318%
9	8.963	988	999	1011	rBV	557517	932343	19.96%	2.541%
10	9.681	1112	1121	1131	rBV	466269	758466	16.24%	2.067%
11	10.222	1205	1213	1232	rBV	724880	1270677	27.21%	3.463%
12	10.593	1268	1276	1284	rBV	556181	903106	19.34%	2.461%
13	10.740	1293	1301	1318	rBV	648532	1147987	24.58%	3.129%
14	12.193	1540	1548	1554	rVB3	10132	20101	0.43%	0.055%
15	12.404	1579	1584	1590	rBV10	2422	4777	0.10%	0.013%
16	12.769	1640	1646	1648	rBV6	6019	9500	0.20%	0.026%
17	12.840	1653	1658	1665	rVB4	10695	22090	0.47%	0.060%
18	13.340	1737	1743	1754	rBV7	11220	31056	0.66%	0.085%
19	13.451	1759	1762	1768	rVV8	5757	11543	0.25%	0.031%
20	13.522	1770	1774	1780	rVB7	4634	7800	0.17%	0.021%
21	13.698	1796	1804	1805	rBV8	2736	5422	0.12%	0.015%
22	13.857	1824	1831	1843	rBV	1135850	1565169	33.51%	4.265%
23	14.134	1868	1878	1892	rBV	1381927	2003775	42.91%	5.461%
24	14.439	1922	1930	1941	rBV	793361	1140615	24.42%	3.108%
25	14.663	1962	1968	1991	rBV	399137	791782	16.95%	2.158%
26	15.434	2091	2099	2107	rBV	1692489	2519252	53.94%	6.866%
27	15.563	2114	2121	2136	rBV	427799	633410	13.56%	1.726%
28	15.675	2136	2140	2144	rVB5	8199	12852	0.28%	0.035%
29	16.004	2194	2196	2201	rVB6	3482	4714	0.10%	0.013%
30	16.245	2229	2237	2241	rBV8	18786	36803	0.79%	0.100%
31	17.198	2392	2399	2408	rBV	984432	1448517	31.02%	3.948%
32	17.292	2409	2415	2431	rVV	2055290	2907720	62.26%	7.924%
33	19.116	2722	2725	2730	rBV5	31960	39139	0.84%	0.107%
34	19.186	2734	2737	2741	rVV	25660	31285	0.67%	0.085%
35	19.539	2791	2797	2804	rBV	2883178	3864879	82.76%	10.533%
36	21.298	3092	3096	3102	rBV	1558566	1923986	41.20%	5.243%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019213.D
Acq On : 02 Jan 2024 18:03
Operator : MA/JU
Sample : PB158101BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK101

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	23.510	3465	3472	3486	rVB2	2386564	4670190	100.00%	12.727%
38	23.662	3492	3498	3506	rVB	1118550	2190649	46.91%	5.970%




Sum of corrected areas: 36693907

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019213.D
Acq On : 02 Jan 2024 18:03
Operator : MA/JU
Sample : PB158101BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

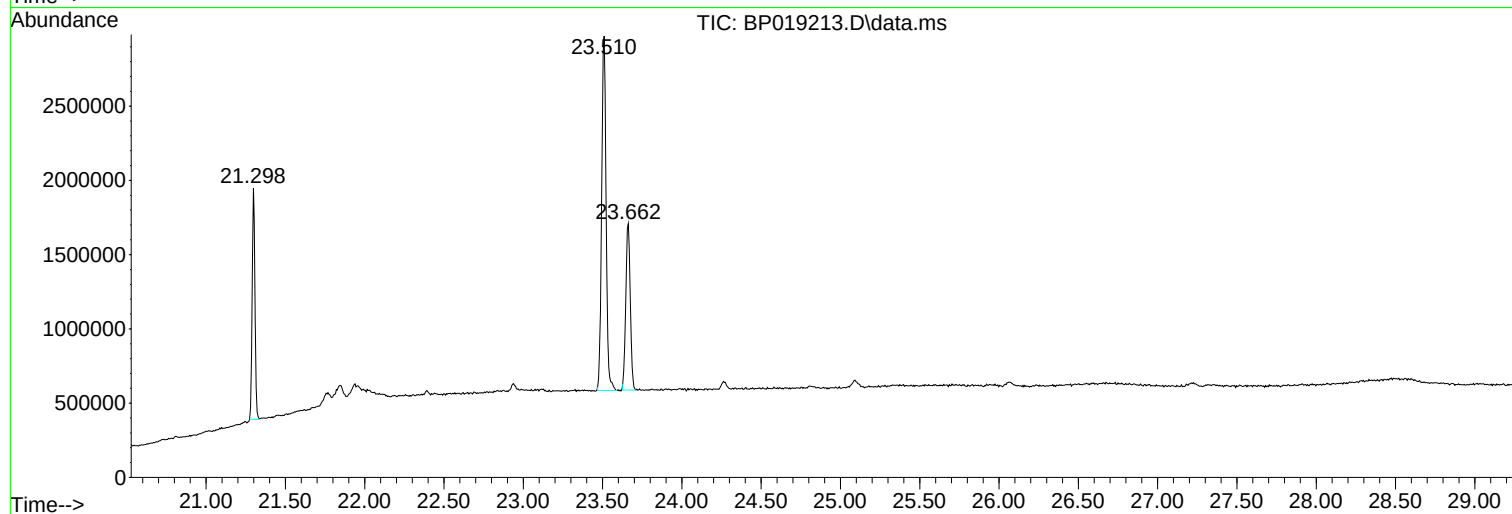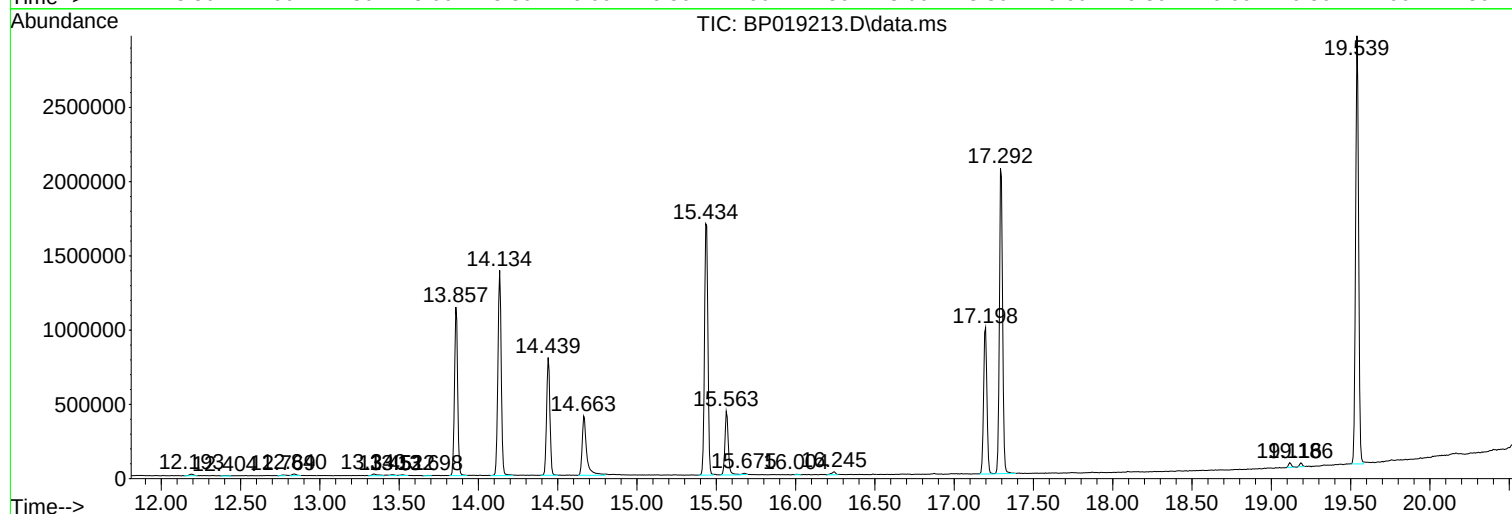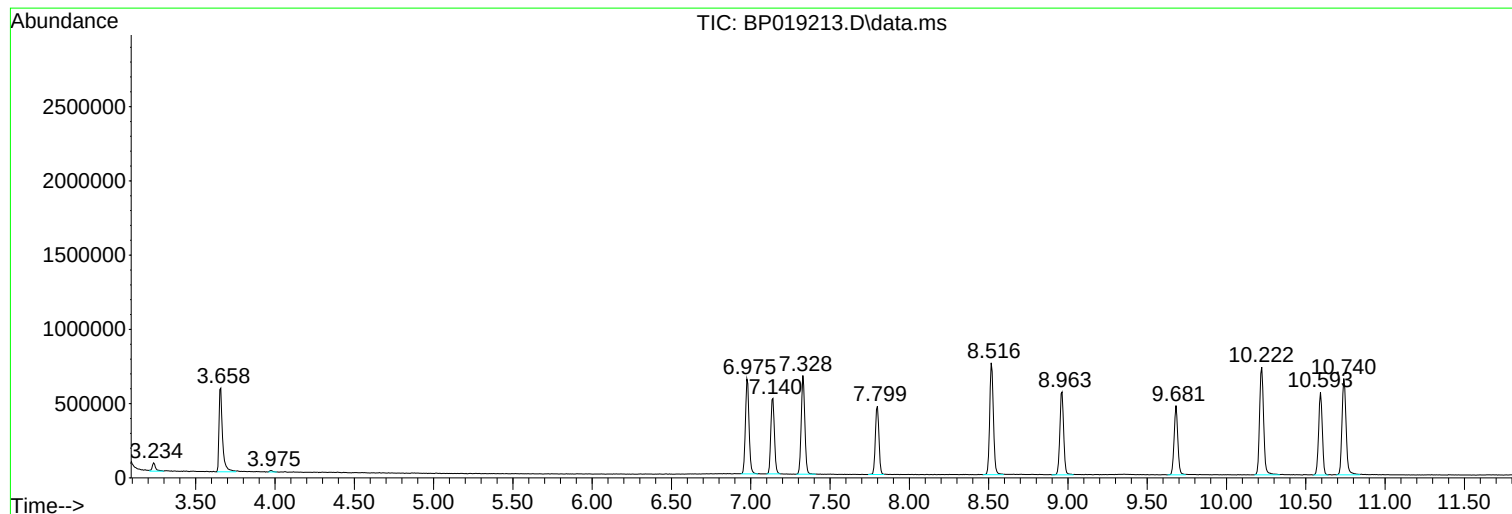

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019213.D
Acq On : 02 Jan 2024 18:03
Operator : MA/JU
Sample : PB158101BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019213.D
Acq On : 02 Jan 2024 18:03
Operator : MA/JU
Sample : PB158101BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK101

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------