

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
 Data File : BP019253.D
 Acq On : 03 Jan 2024 17:50
 Operator : MA/JU
 Sample : PB158128BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK128

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	32	rVB	61956	75326	1.48%	0.170%
2	3.658	93	97	118	rBV	675925	1036383	20.30%	2.341%
3	3.975	148	151	157	rVB	12312	14100	0.28%	0.032%
4	6.987	656	663	673	rBV	735955	1160714	22.73%	2.622%
5	7.140	682	689	699	rVB	561698	884061	17.32%	1.997%
6	7.334	715	722	732	rBV	744931	1179790	23.11%	2.665%
7	7.799	794	801	810	rVB	631115	992772	19.44%	2.243%
8	8.528	917	925	937	rBV	817690	1373352	26.90%	3.102%
9	8.963	991	999	1007	rBV	644600	1044546	20.46%	2.359%
10	9.681	1113	1121	1132	rBV	535196	865650	16.95%	1.955%
11	10.228	1206	1214	1229	rBV	829762	1432787	28.06%	3.236%
12	10.593	1267	1276	1288	rBV	802646	1284047	25.15%	2.901%
13	10.745	1294	1302	1317	rBV	733291	1310632	25.67%	2.961%
14	12.187	1539	1547	1555	rVB	14227	26197	0.51%	0.059%
15	13.339	1737	1743	1749	rBV3	11868	20461	0.40%	0.046%
16	13.857	1825	1831	1843	rBV	1307460	1814360	35.54%	4.098%
17	14.134	1871	1878	1892	rBV2	1619590	2359630	46.22%	5.330%
18	14.439	1921	1930	1941	rBV	1147738	1674088	32.79%	3.782%
19	14.681	1965	1971	1990	rBV	487877	951964	18.65%	2.150%
20	15.439	2092	2100	2113	rBV	2036249	2952341	57.83%	6.669%
21	15.569	2116	2122	2134	rVV	395461	563570	11.04%	1.273%
22	15.681	2137	2141	2145	rVB7	10617	14486	0.28%	0.033%
23	16.228	2230	2234	2238	rVB5	8286	12212	0.24%	0.028%
24	16.604	2295	2298	2301	rBV5	4272	6105	0.12%	0.014%
25	16.863	2337	2342	2347	rBV9	14409	26605	0.52%	0.060%
26	17.198	2393	2399	2407	rBV	1571245	2165191	42.41%	4.891%
27	17.298	2409	2416	2428	rBV	2504915	3395372	66.50%	7.670%
28	17.486	2445	2448	2454	rBV8	8202	15586	0.31%	0.035%
29	18.204	2566	2570	2576	rBV3	47801	78045	1.53%	0.176%
30	19.122	2722	2726	2731	rVB2	34569	43916	0.86%	0.099%
31	19.186	2734	2737	2742	rVV	30462	43159	0.85%	0.097%
32	19.545	2792	2798	2805	rBV	3423102	4399304	86.17%	9.937%
33	21.304	3092	3097	3103	rBV	2233512	2830669	55.44%	6.394%
34	23.515	3466	3473	3489	rVB2	2525764	5105631	100.00%	11.533%
35	23.668	3493	3499	3509	rVB	1553048	3116762	61.05%	7.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019253.D
Acq On : 03 Jan 2024 17:50
Operator : MA/JU
Sample : PB158128BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK128

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 44269814

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019253.D
Acq On : 03 Jan 2024 17:50
Operator : MA/JU
Sample : PB158128BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK128

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

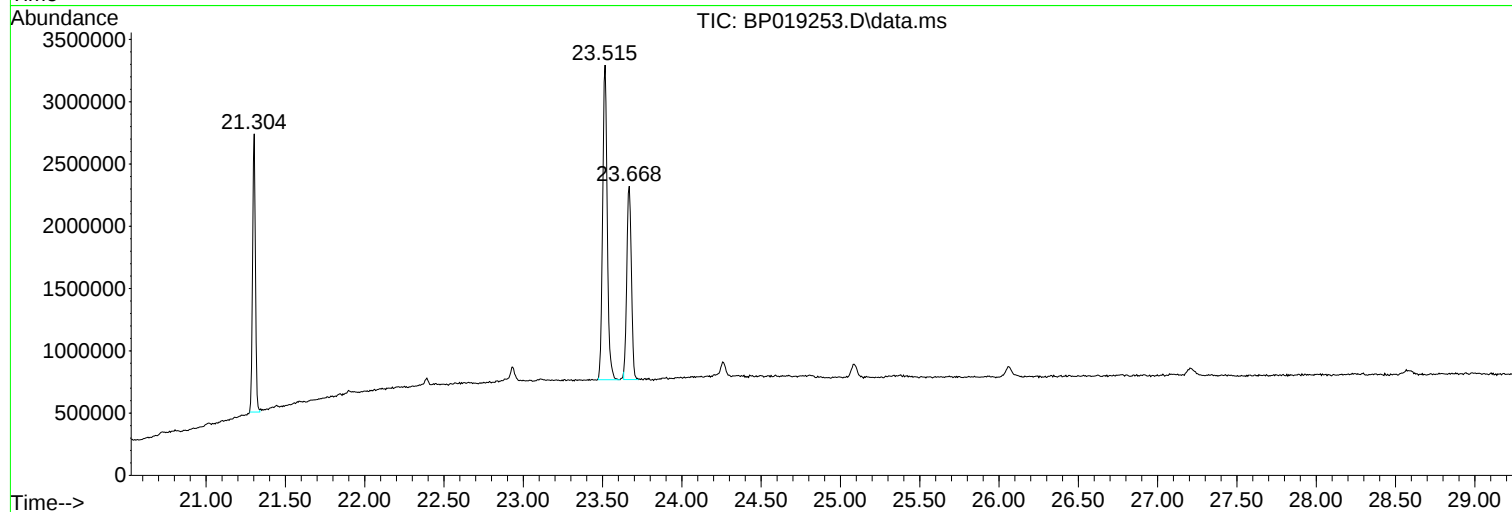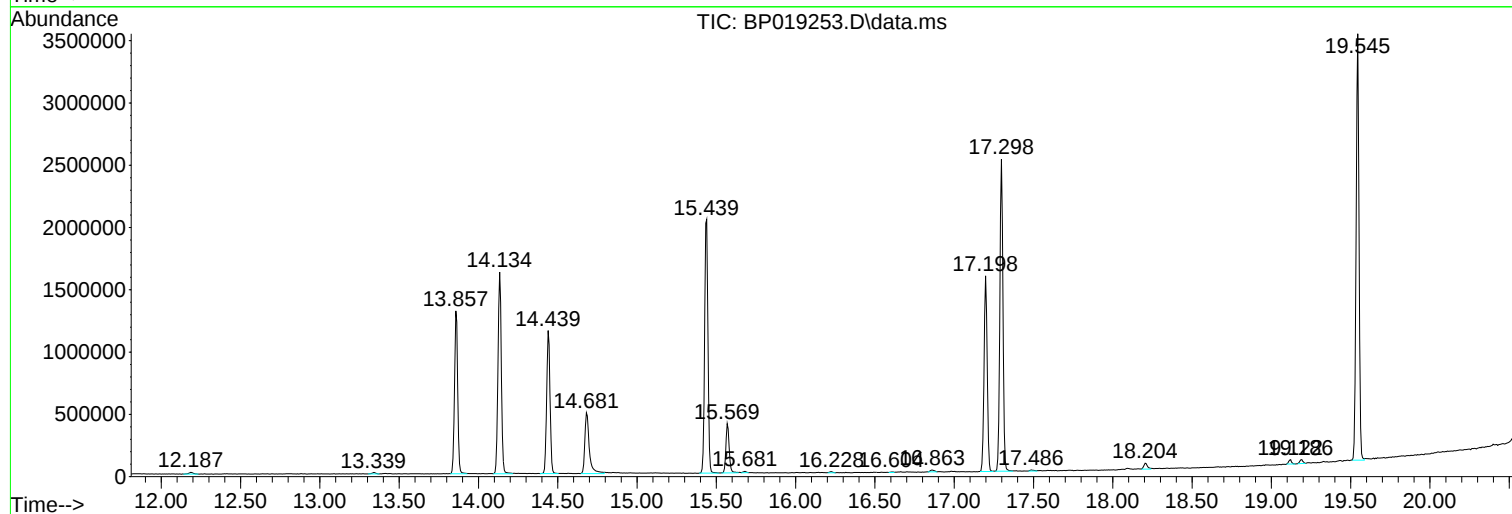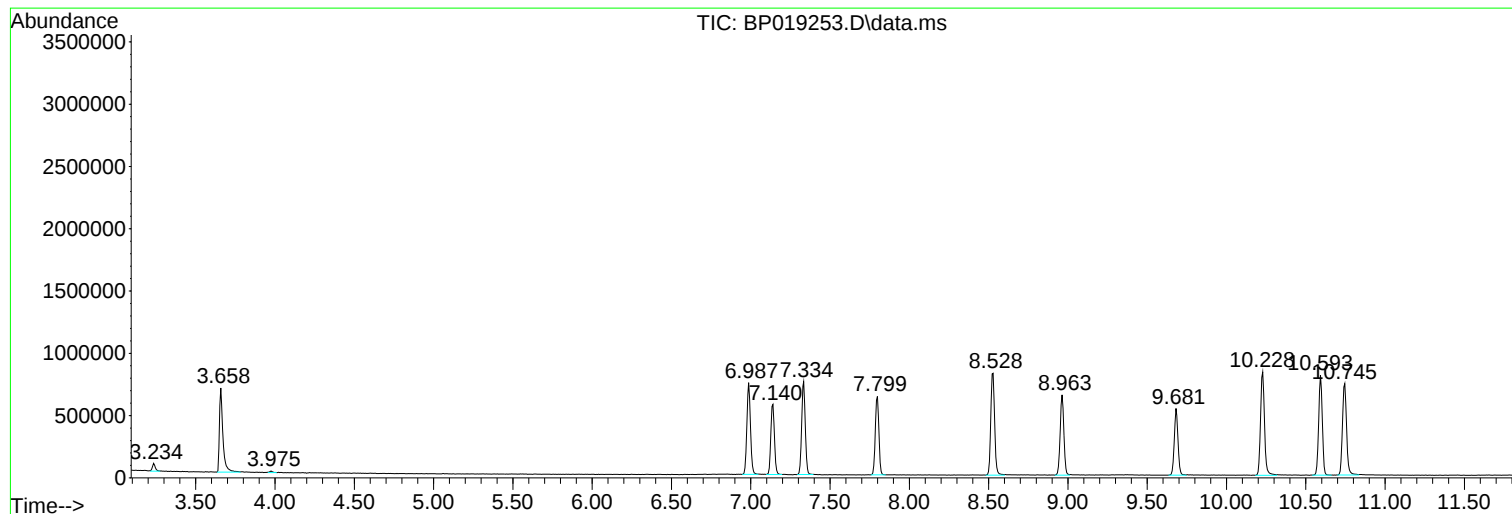

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019253.D
Acq On : 03 Jan 2024 17:50
Operator : MA/JU
Sample : PB158128BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK128

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010224\
Data File : BP019253.D
Acq On : 03 Jan 2024 17:50
Operator : MA/JU
Sample : PB158128BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK128

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------