
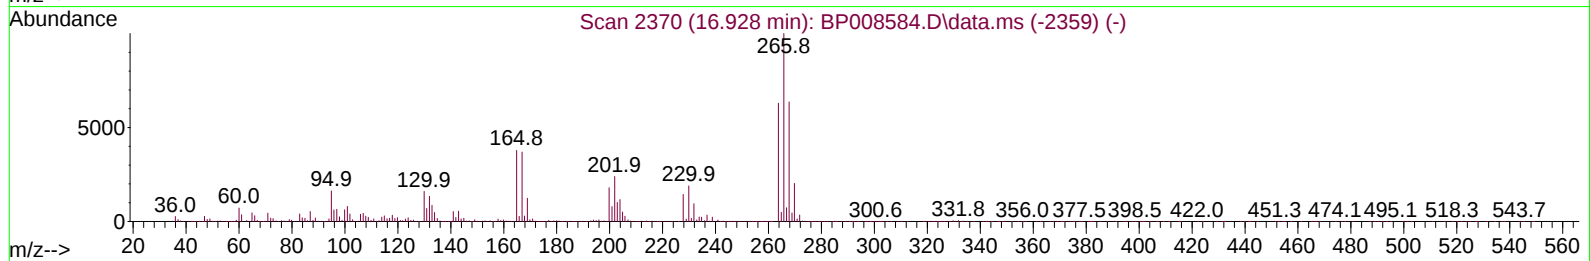
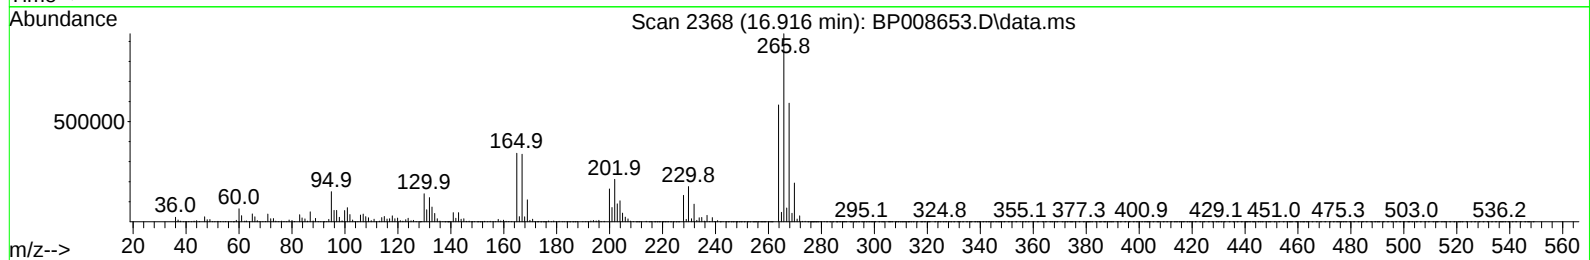


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008653.D
Acq On : 04 Jan 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 13:27:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

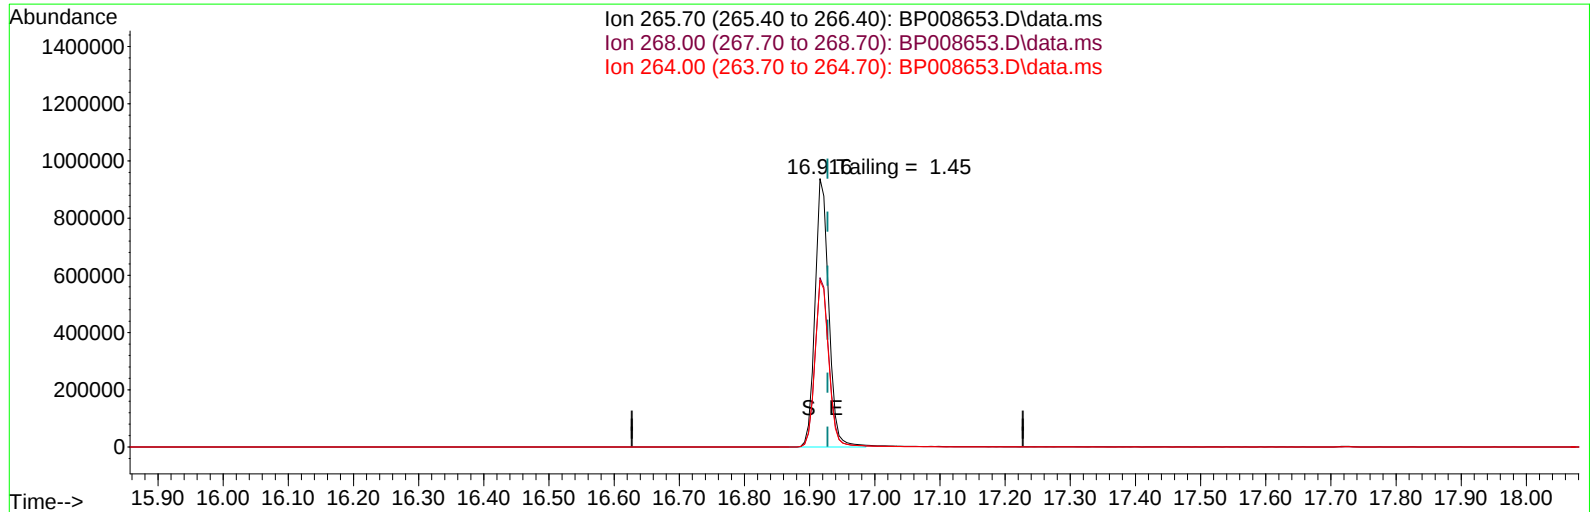

TIC: BP008653.D\data.ms

(70) Pentachlorophenol (C)




16.916min (-0.012) 851337.72 ng

response 1388886

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.10
264.00	62.90	62.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008653.D
Acq On : 04 Jan 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 13:27:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

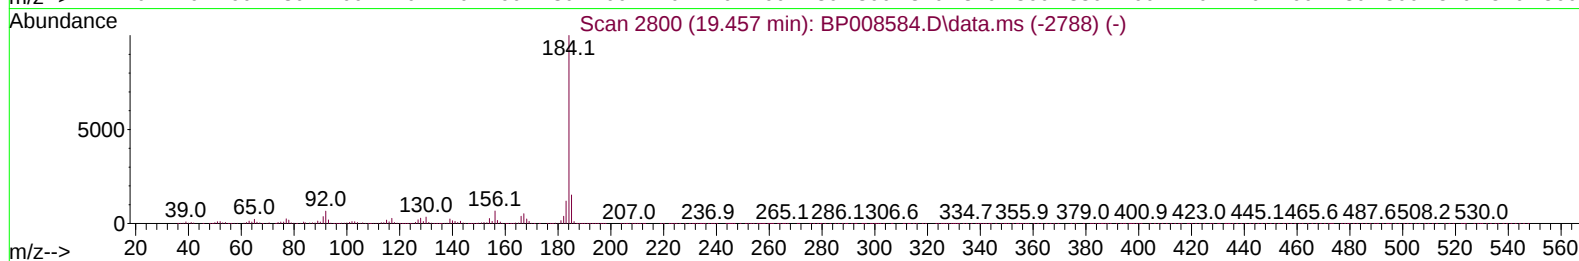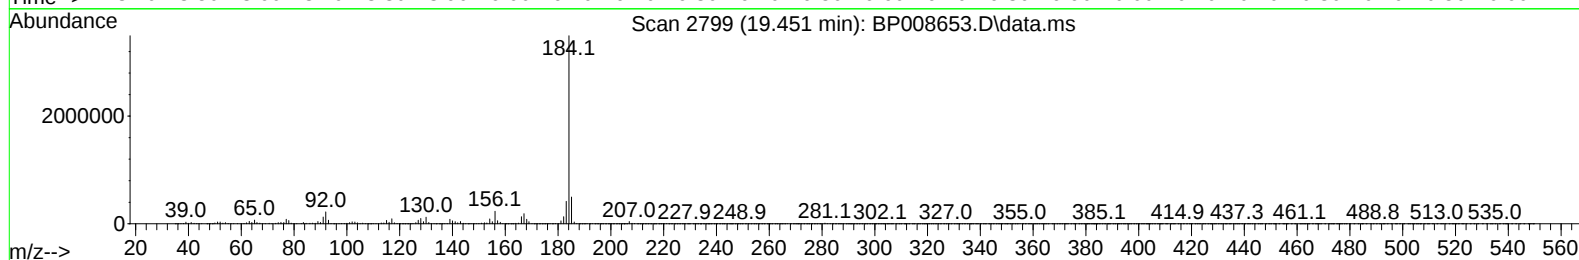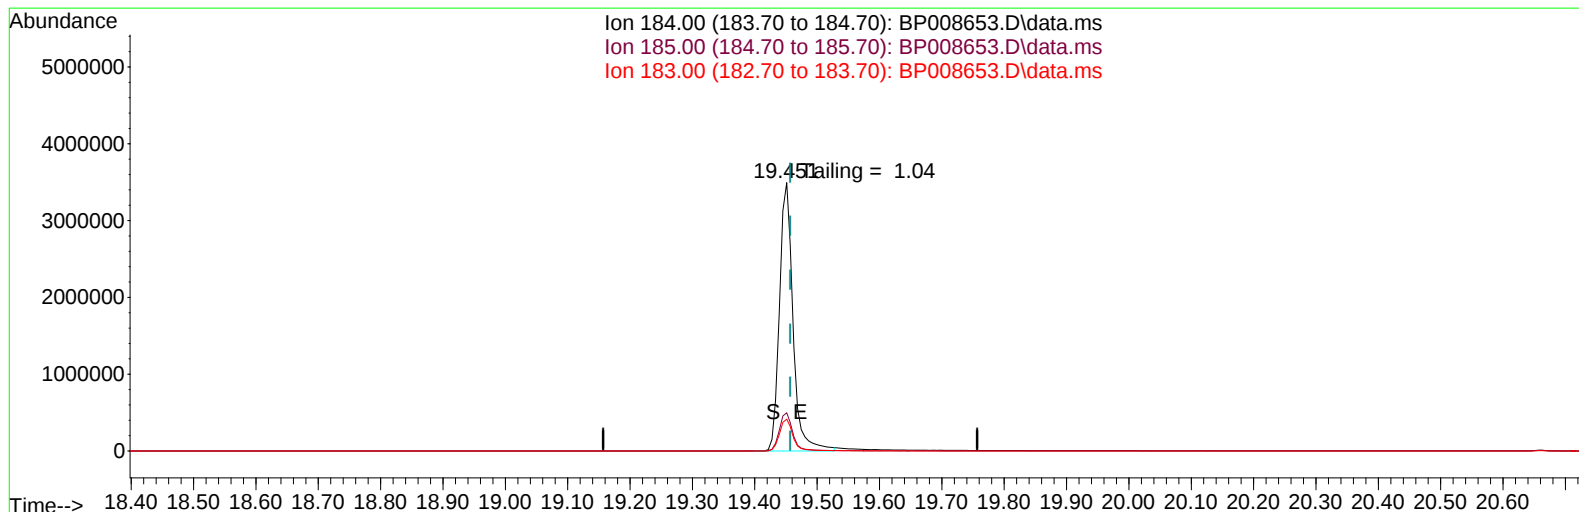

TIC: BP008653.D\data.ms

(77) Benzidine**19.451min (-0.006) 369849.25 ng****response 5433550**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.25
183.00	11.90	11.89
0.00	0.00	0.00