
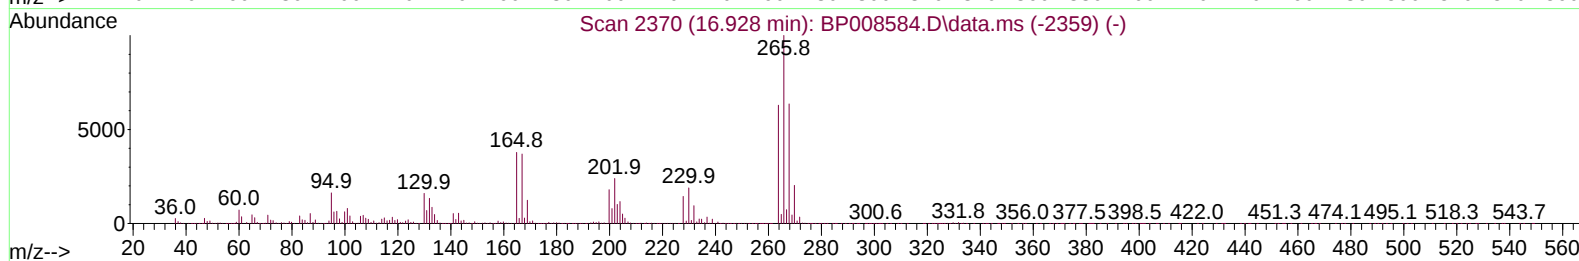
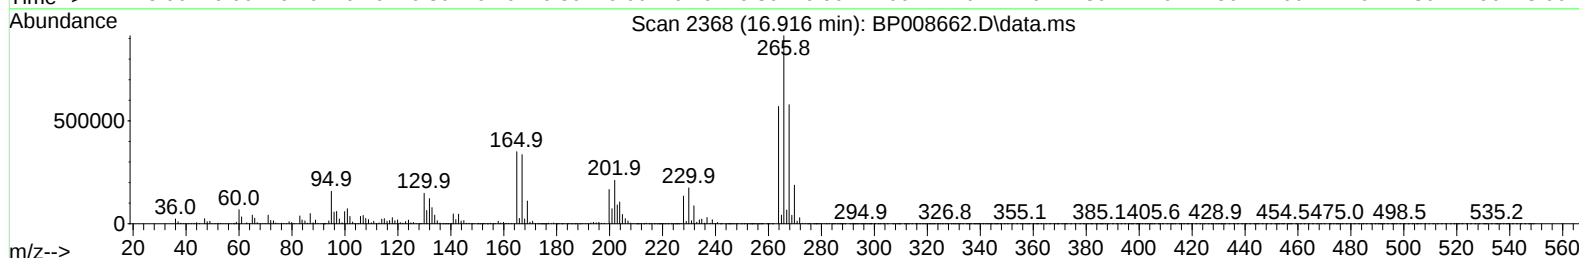


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008662.D
Acq On : 04 Jan 2022 15:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 05:45:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

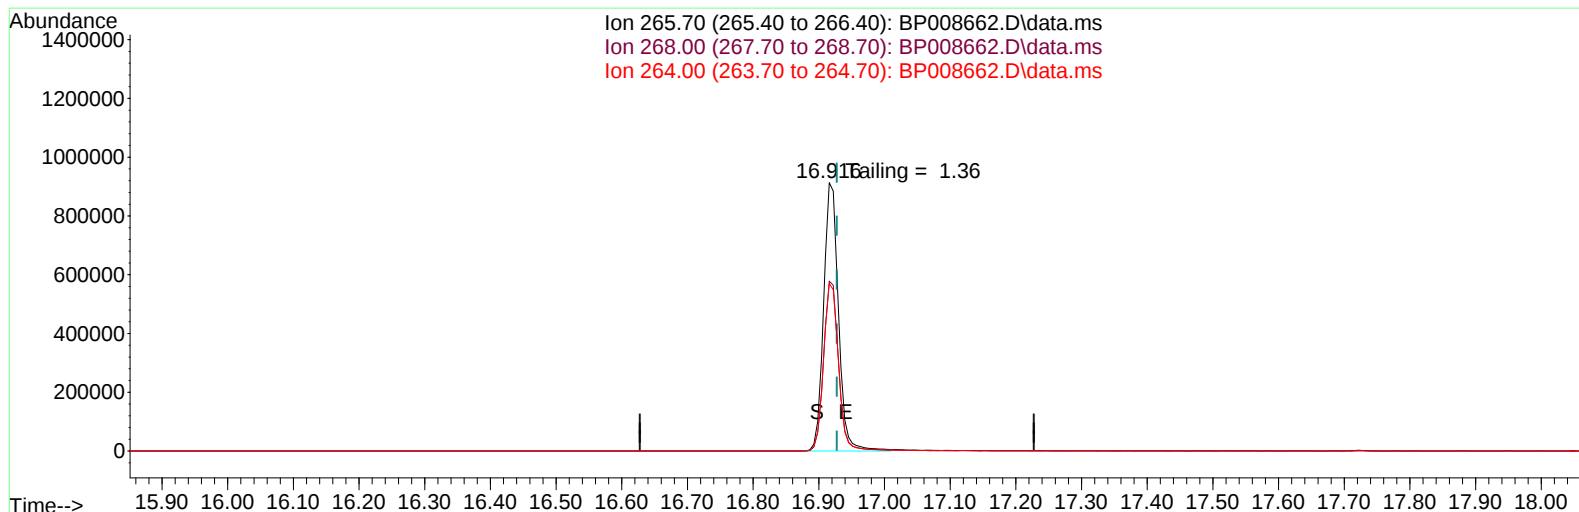

TIC: BP008662.D\data.ms

(70) Pentachlorophenol (C)




16.916min (-0.012) 173056.06 ng

response 1439485

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.35
264.00	62.90	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
 Data File : BP008662.D
 Acq On : 04 Jan 2022 15:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 05:45:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

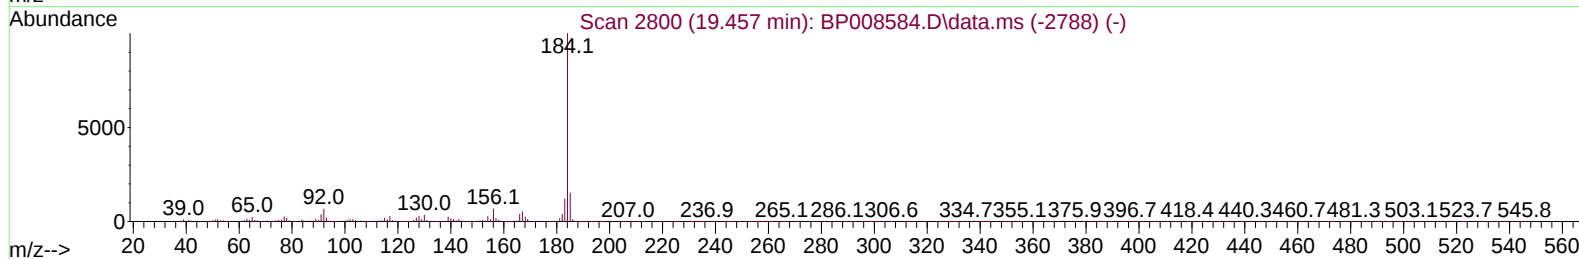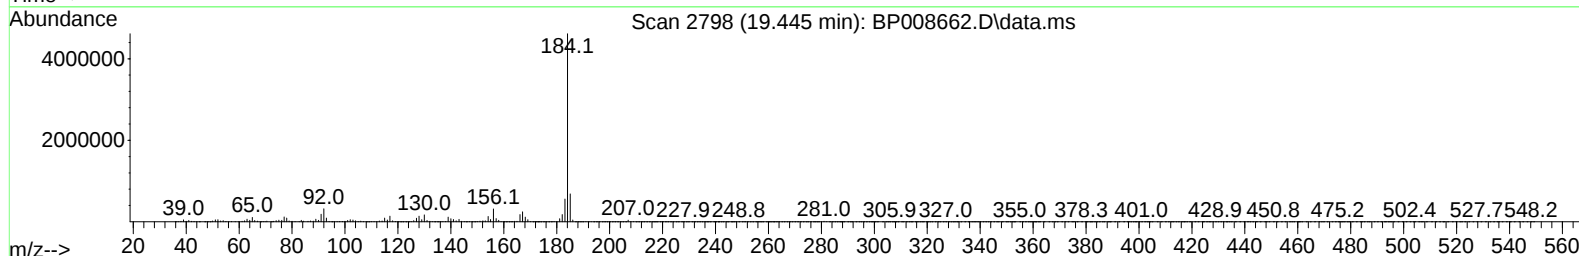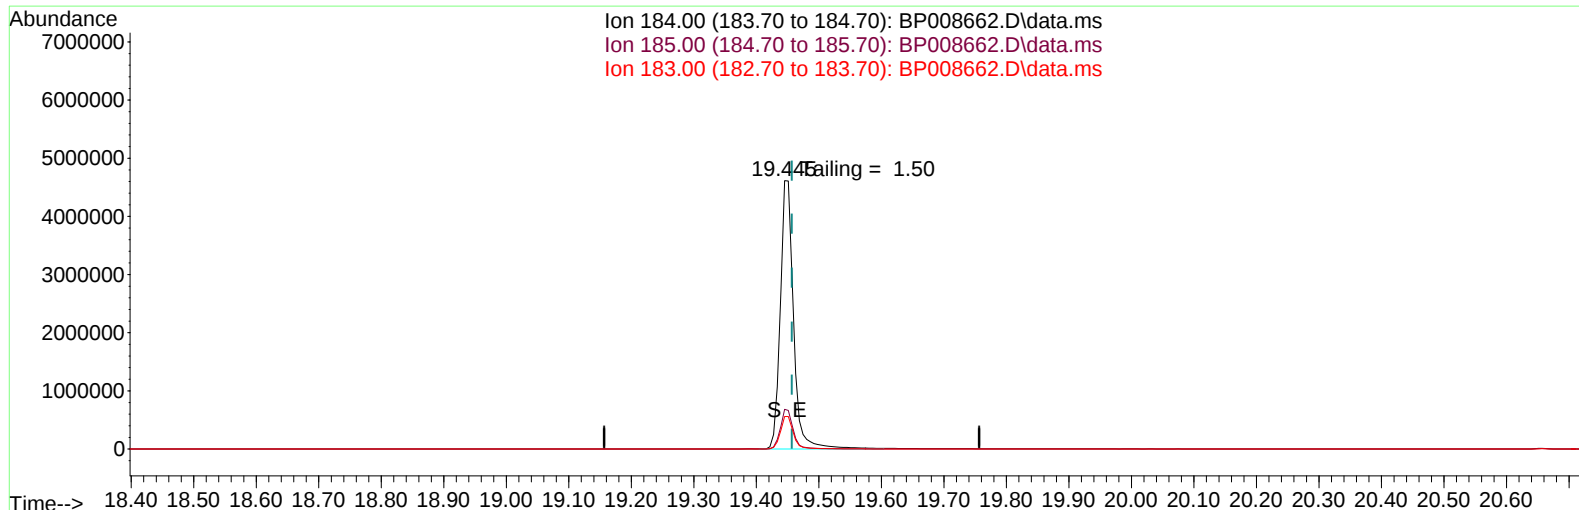

TIC: BP008662.D\data.ms

(77) Benzidine**19.445min (-0.012) 56830.30 ng****response 6858543**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.83
183.00	11.90	12.12
0.00	0.00	0.00