

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
 Data File : BP008655.D
 Acq On : 04 Jan 2022 11:05
 Operator : CG/JU
 Sample : PB141549BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141549BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	415	422	432	rBV	7718223	11695306	31.43%	8.157%
2	7.058	684	692	707	rBV	7050211	11768268	31.62%	8.208%
3	7.887	826	833	841	rBV	1569973	2527378	6.79%	1.763%
4	9.046	1021	1030	1047	rBV	4601123	7675496	20.63%	5.354%
5	10.687	1301	1309	1318	rBV	2097786	3547223	9.53%	2.474%
6	13.146	1718	1727	1743	rBV	13627991	20654355	55.50%	14.406%
7	14.516	1954	1960	1980	rBV	3249713	5135429	13.80%	3.582%
8	16.004	2206	2213	2236	rBV	10973636	17532598	47.11%	12.229%
9	17.269	2421	2428	2439	rBV	4608344	6769777	18.19%	4.722%
10	19.828	2857	2863	2874	rBV2	28055347	37212958	100.00%	25.956%
11	21.351	3117	3122	3131	rBV	6745258	8913586	23.95%	6.217%
12	23.774	3527	3534	3550	rVB2	4709197	9937470	26.70%	6.931%


Sum of corrected areas: 143369844

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008655.D
Acq On : 04 Jan 2022 11:05
Operator : CG/JU
Sample : PB141549BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141549BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

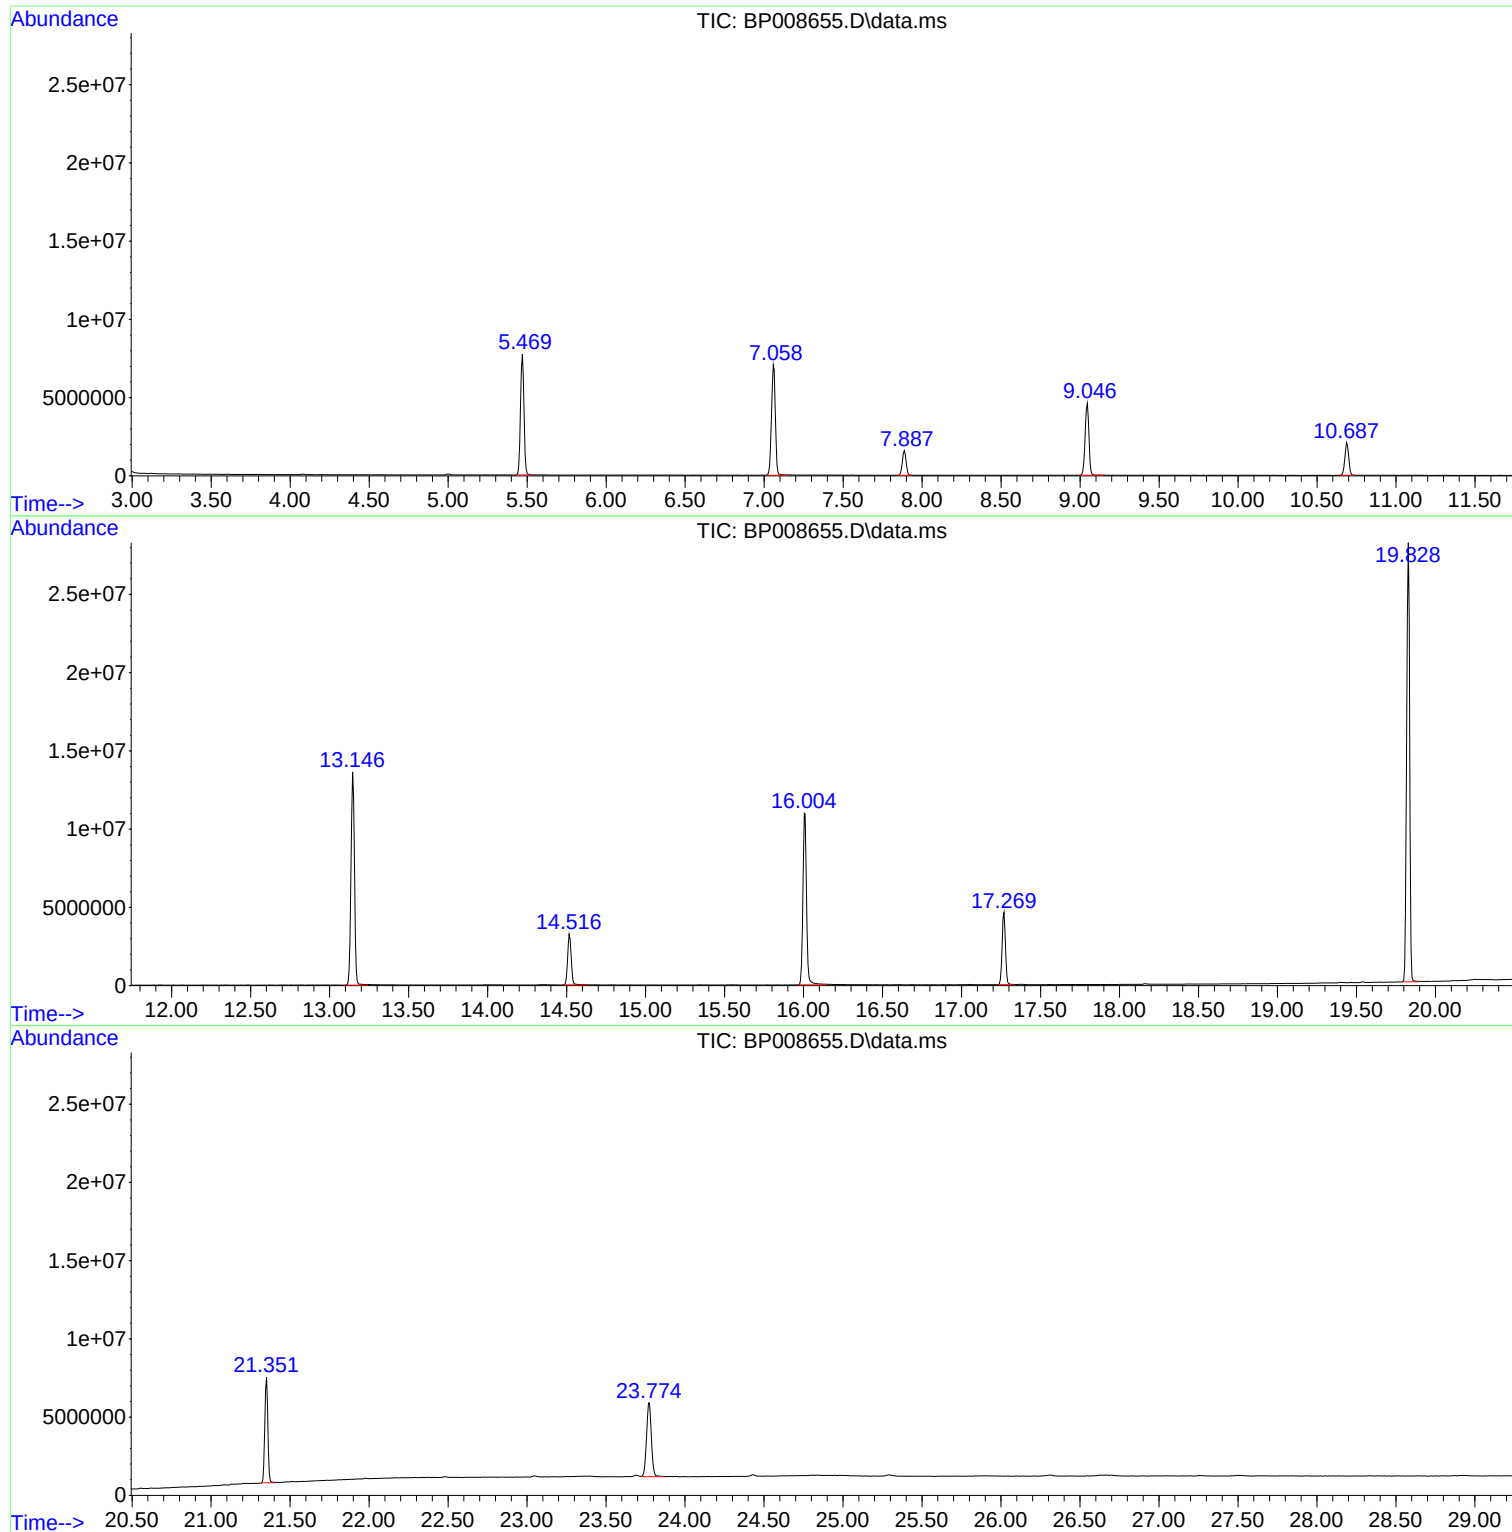

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008655.D
Acq On : 04 Jan 2022 11:05
Operator : CG/JU
Sample : PB141549BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141549BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008655.D
Acq On : 04 Jan 2022 11:05
Operator : CG/JU
Sample : PB141549BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141549BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------