

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
 Data File : BP008664.D
 Acq On : 04 Jan 2022 16:25
 Operator : CG/JU
 Sample : PB141778BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141778BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	415	422	438	rBV	7271252	11165494	28.07%	7.715%
2	7.057	684	692	706	rBV	6957791	11295062	28.40%	7.805%
3	7.887	825	833	843	rVB	1468907	2394648	6.02%	1.655%
4	9.040	1021	1029	1050	rBV	4234160	7353379	18.49%	5.081%
5	10.687	1301	1309	1319	rBV	2016287	3397908	8.54%	2.348%
6	13.145	1719	1727	1742	rBV	13628038	20111239	50.56%	13.897%
7	14.516	1953	1960	1985	rBV	3286756	5061872	12.73%	3.498%
8	16.004	2205	2213	2252	rBV	10863805	17590902	44.23%	12.155%
9	17.263	2420	2427	2438	rBV	4542639	6882434	17.30%	4.756%
10	19.827	2856	2863	2876	rBV	29166972	39773103	100.00%	27.483%
11	21.345	3116	3121	3131	rBV	7043387	9392969	23.62%	6.490%
12	23.768	3526	3533	3548	rVB2	4806557	10300387	25.90%	7.117%


Sum of corrected areas: 144719397

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008664.D
Acq On : 04 Jan 2022 16:25
Operator : CG/JU
Sample : PB141778BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141778BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

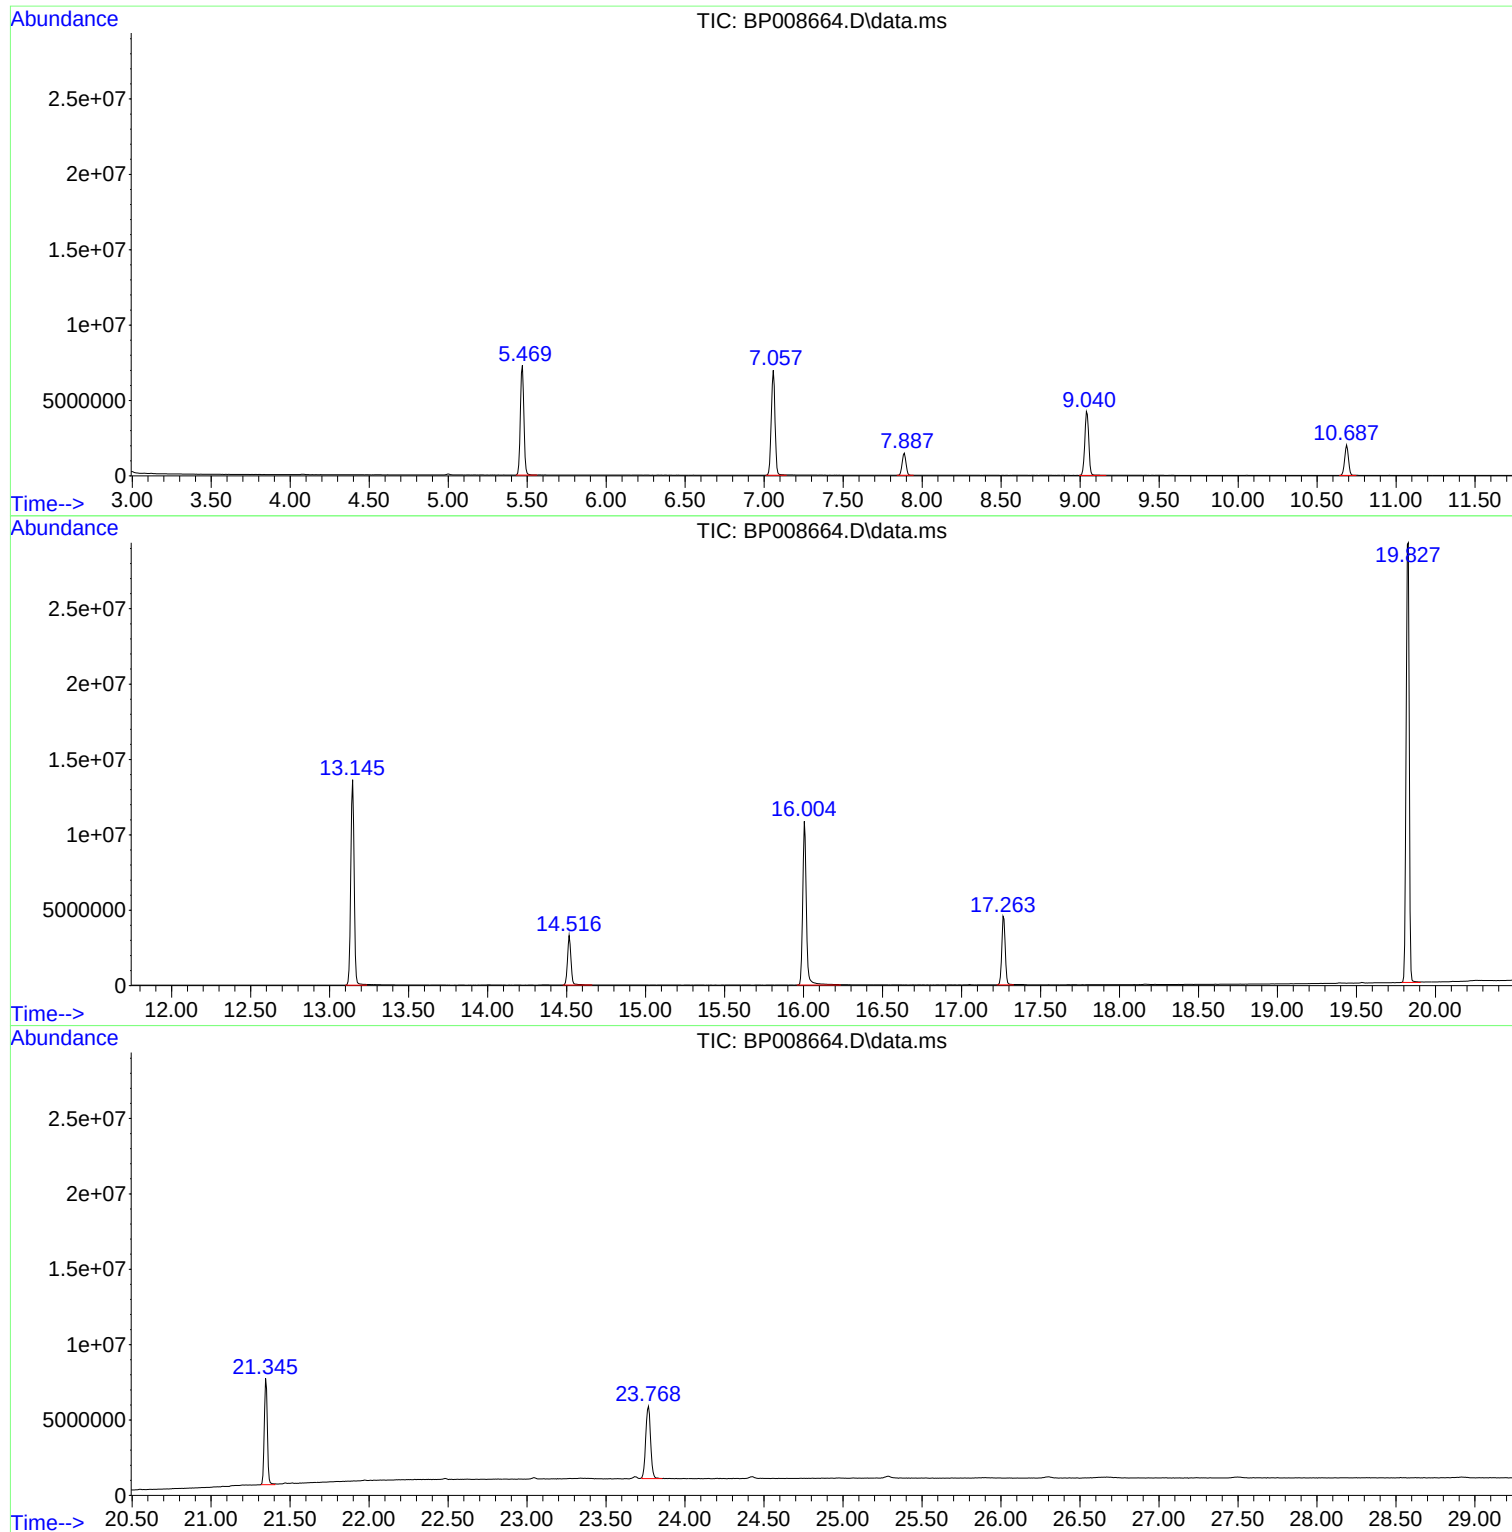

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008664.D
Acq On : 04 Jan 2022 16:25
Operator : CG/JU
Sample : PB141778BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141778BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008664.D
Acq On : 04 Jan 2022 16:25
Operator : CG/JU
Sample : PB141778BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141778BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------