

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
 Data File : BP008682.D
 Acq On : 05 Jan 2022 02:36
 Operator : CG/JU
 Sample : M5340-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BAYSHORE-FILL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.005	337	343	352	rVB	510050	760553	2.94%	0.894%
2	7.058	684	692	706	rBV	602962	1055014	4.08%	1.240%
3	7.887	824	833	841	rBV	2643685	4283731	16.56%	5.036%
4	9.040	1023	1029	1038	rVB	442614	763234	2.95%	0.897%
5	10.687	1300	1309	1315	rBV	3400907	6030099	23.31%	7.088%
6	10.740	1315	1318	1326	rVB	406494	641616	2.48%	0.754%
7	12.351	1585	1592	1601	rVB	332958	576060	2.23%	0.677%
8	12.569	1619	1629	1640	rBV	254742	437219	1.69%	0.514%
9	13.146	1720	1727	1740	rBV	1587180	2381996	9.21%	2.800%
10	13.698	1812	1821	1827	rBV4	105154	298811	1.15%	0.351%
11	13.845	1840	1846	1851	rBV	199388	338851	1.31%	0.398%
12	14.245	1908	1914	1926	rBV	164838	298439	1.15%	0.351%
13	14.522	1952	1961	1967	rBV	5035207	7620316	29.45%	8.958%
14	14.581	1967	1971	1980	rVB	185265	362558	1.40%	0.426%
15	14.922	2024	2029	2036	rVB	164754	289532	1.12%	0.340%
16	15.569	2134	2139	2144	rBV	278776	421398	1.63%	0.495%
17	17.092	2394	2398	2406	rVB2	170376	286877	1.11%	0.337%
18	17.269	2422	2428	2433	rBV	5169619	7811370	30.19%	9.182%
19	17.310	2433	2435	2441	rVB	1207629	1640014	6.34%	1.928%
20	17.404	2447	2451	2456	rVB	321739	439562	1.70%	0.517%
21	18.139	2572	2576	2579	rBV	224021	338171	1.31%	0.398%
22	18.181	2580	2583	2588	rVB	281577	406847	1.57%	0.478%
23	18.322	2603	2607	2611	rBV3	351581	596325	2.30%	0.701%
24	18.357	2611	2613	2619	rVB	196546	268688	1.04%	0.316%
25	19.022	2723	2726	2730	rBV	174072	261348	1.01%	0.307%
26	19.275	2765	2769	2775	rBV	1420464	1947354	7.53%	2.289%
27	19.628	2825	2829	2838	rVB	1282643	1849615	7.15%	2.174%
28	19.822	2858	2862	2867	rVB	1871770	2325762	8.99%	2.734%
29	21.351	3117	3122	3127	rBV	4995770	7177126	27.74%	8.437%
30	21.474	3137	3143	3160	rBV	16650585	25871203	100.00%	30.411%
31	23.780	3529	3535	3545	rVB2	3331375	7290844	28.18%	8.570%




Sum of corrected areas: 85070533

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008682.D
Acq On : 05 Jan 2022 02:36
Operator : CG/JU
Sample : M5340-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BAYSHORE-FILL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

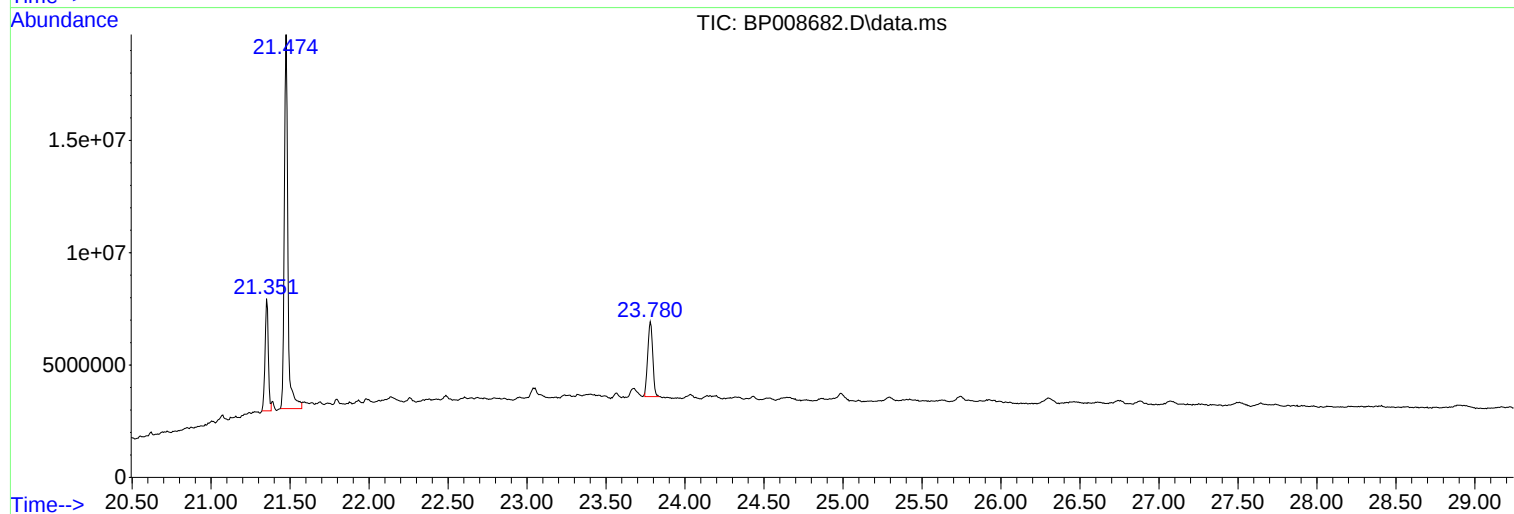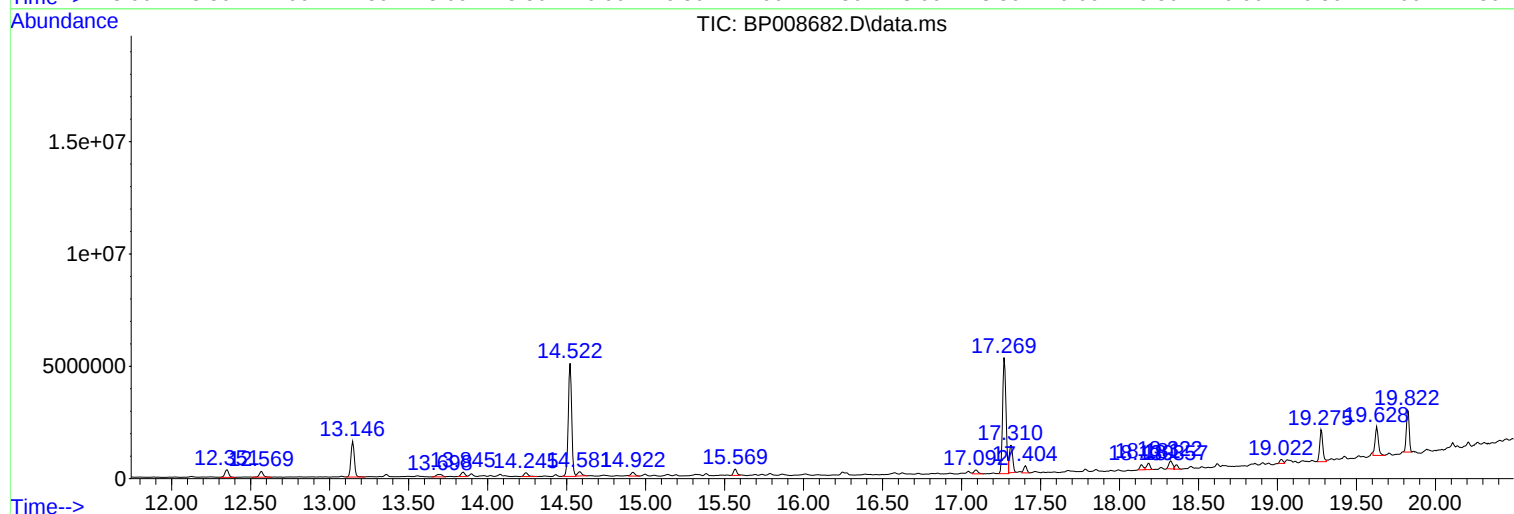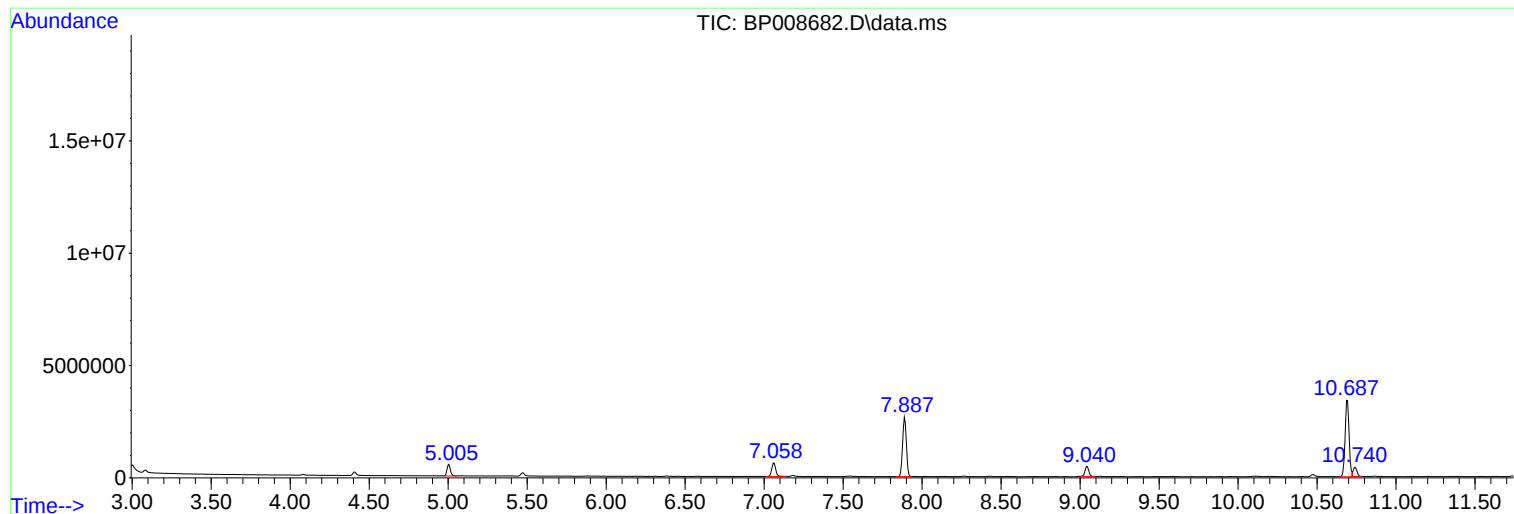

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008682.D
Acq On : 05 Jan 2022 02:36
Operator : CG/JU
Sample : M5340-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BAYSHORE-FILL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.005	3.55 ng	760553	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
3			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9

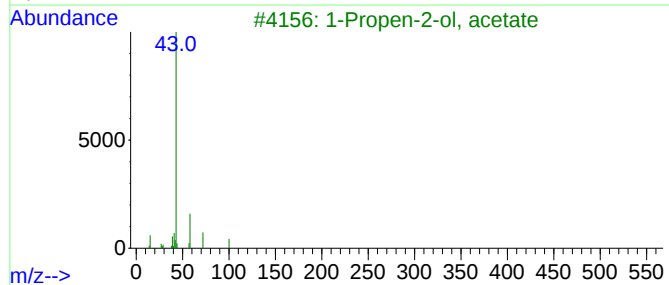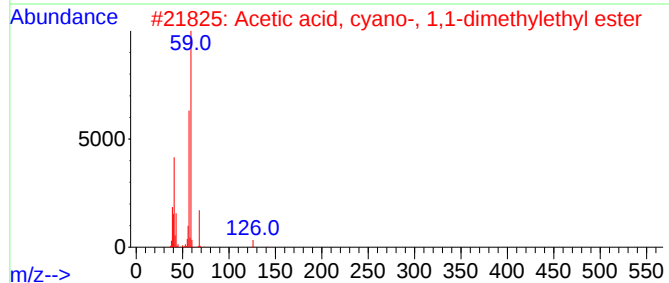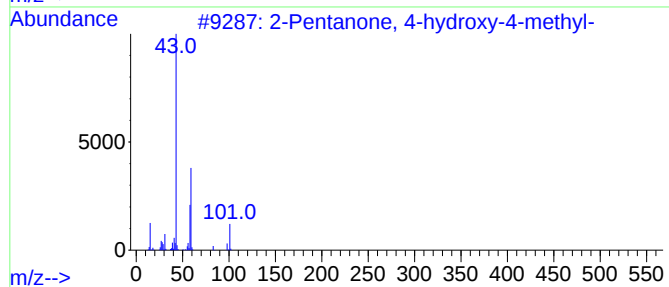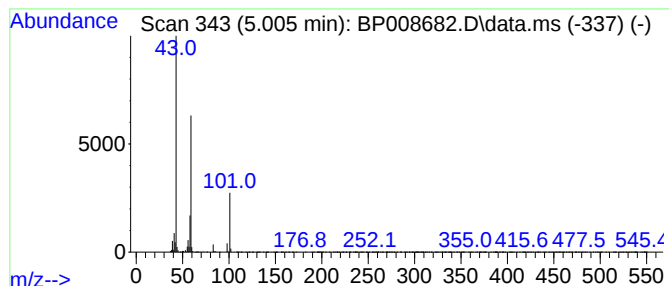

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008682.D
Acq On : 05 Jan 2022 02:36
Operator : CG/JU
Sample : M5340-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BAYSHORE-FILL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.474	72.09 ng	25871200	Chrysene-d12	21.351

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	47
4			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	28
5			5-quinolinol, 8-[2-(3,5-dimethyl...	277	C17H15N3O	1000397-10-2	9

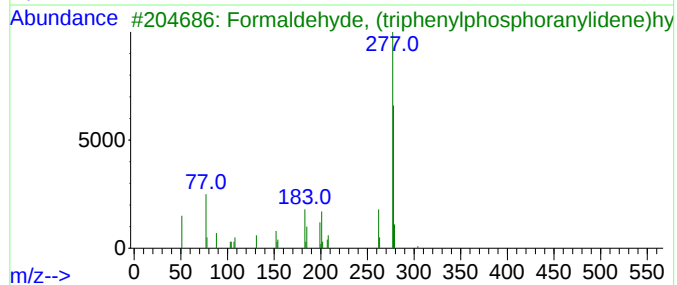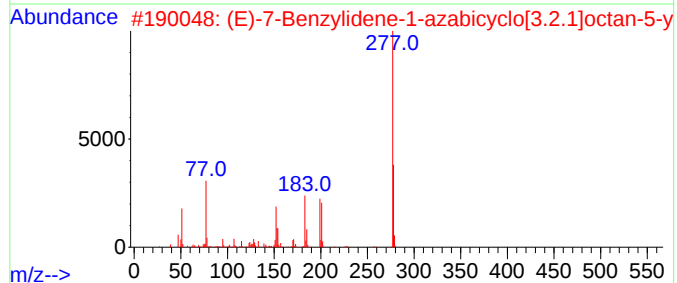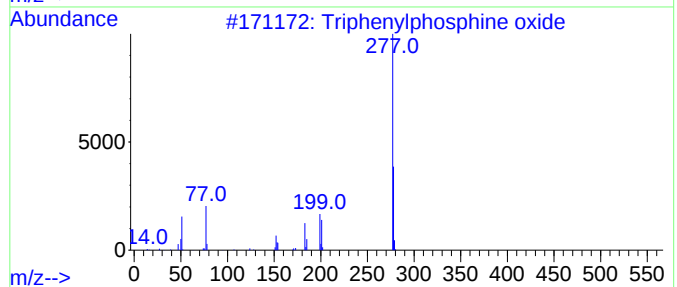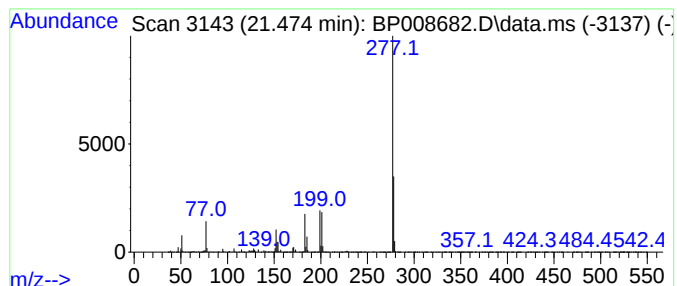

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008682.D
Acq On : 05 Jan 2022 02:36
Operator : CG/JU
Sample : M5340-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BAYSHORE-FILL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.005	3.5	ng	760553	1	7.887	4283730	20.0
Triphenylphosph...	21.474	72.1	ng	25871200	5	21.351	7177130	20.0