
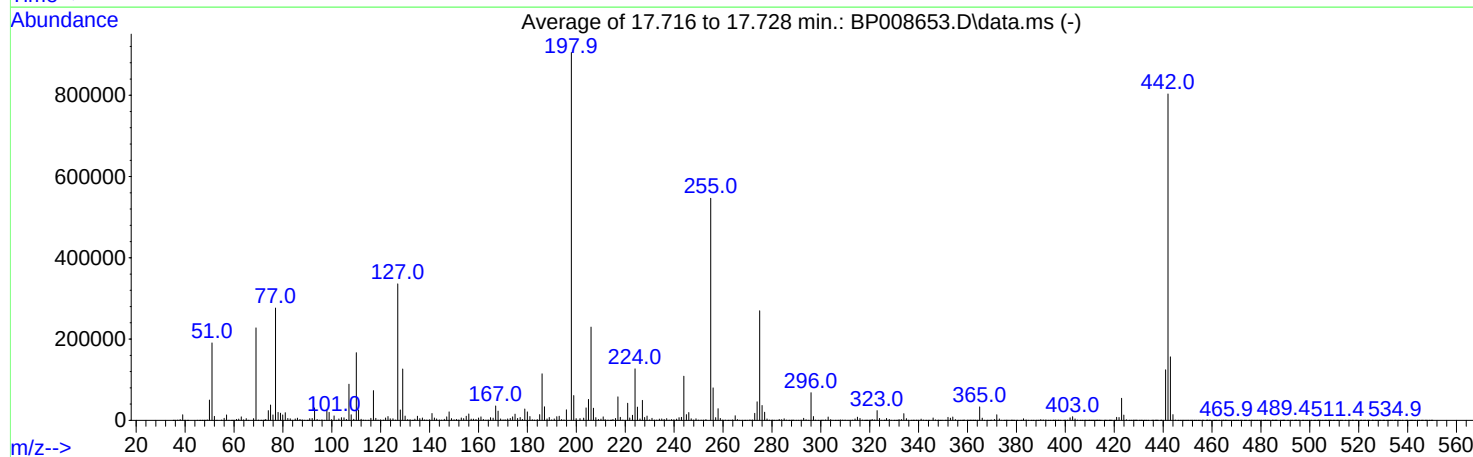


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
 Data File : BP008653.D
 Acq On : 04 Jan 2022 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 08:44:33 2021

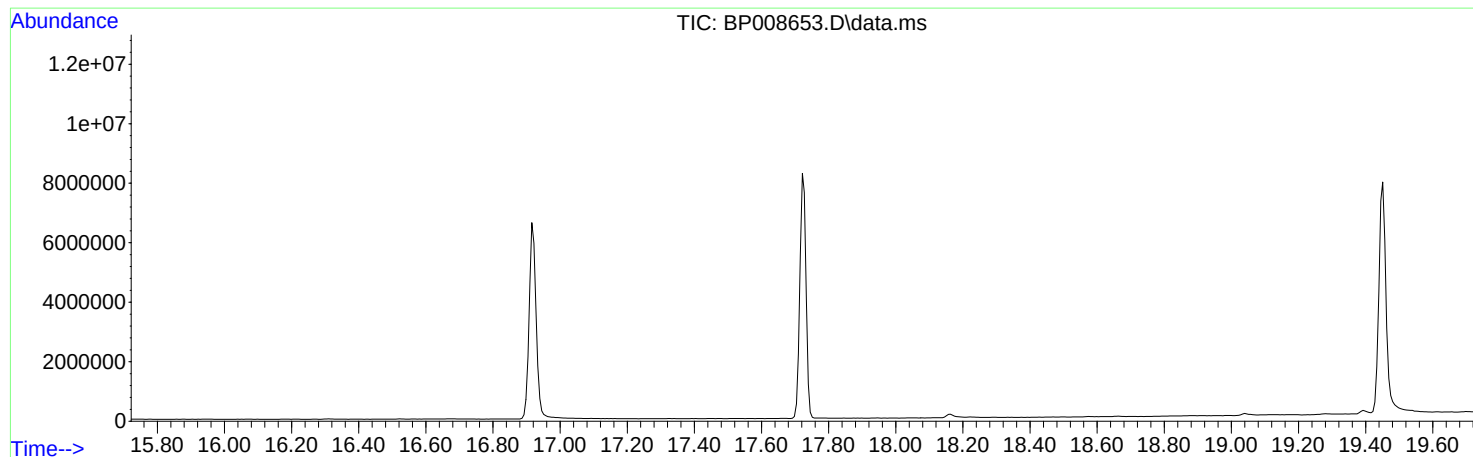




AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	190530	PASS
68	69	0.00	2	1.8	4189	PASS
69	198	0.00	100	25.2	227708	PASS
70	69	0.00	2	0.4	902	PASS
127	198	10	80	37.1	335844	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	905218	PASS
199	198	5	9	6.8	61106	PASS
275	198	10	60	29.8	269568	PASS
365	198	1	100	3.7	33267	PASS
441	198	0.01	100	13.8	124471	PASS
442	442	100	100	100.0	803349	PASS
443	442	15	24	19.5	156466	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008653.D
Acq On : 04 Jan 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 04 13:27:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

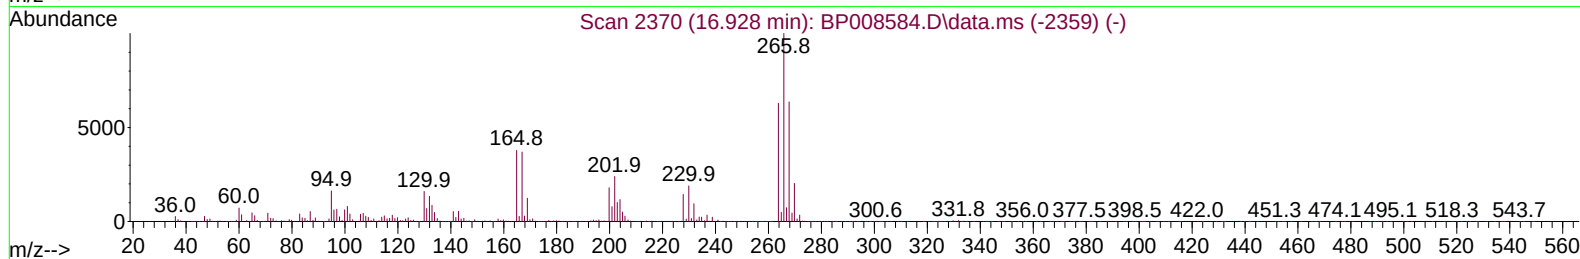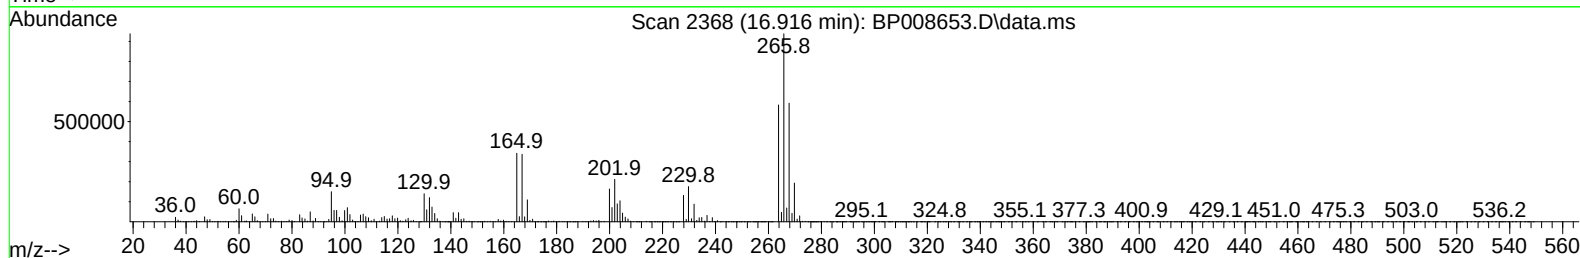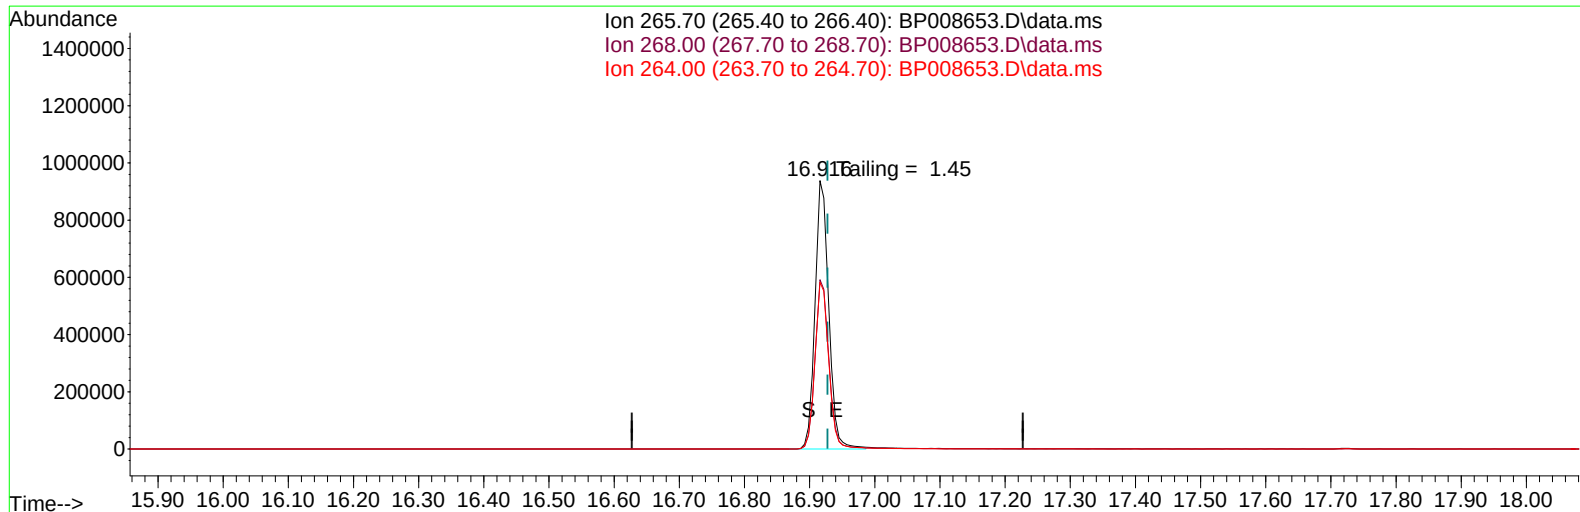

TIC: BP008653.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.012) 851337.72 ng




response 1388886

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.10
264.00	62.90	62.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
 Data File : BP008653.D
 Acq On : 04 Jan 2022 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 04 13:27:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

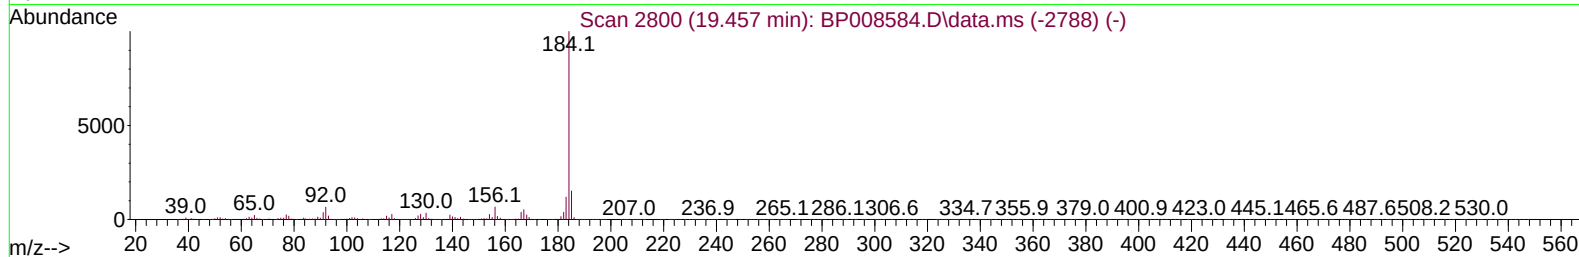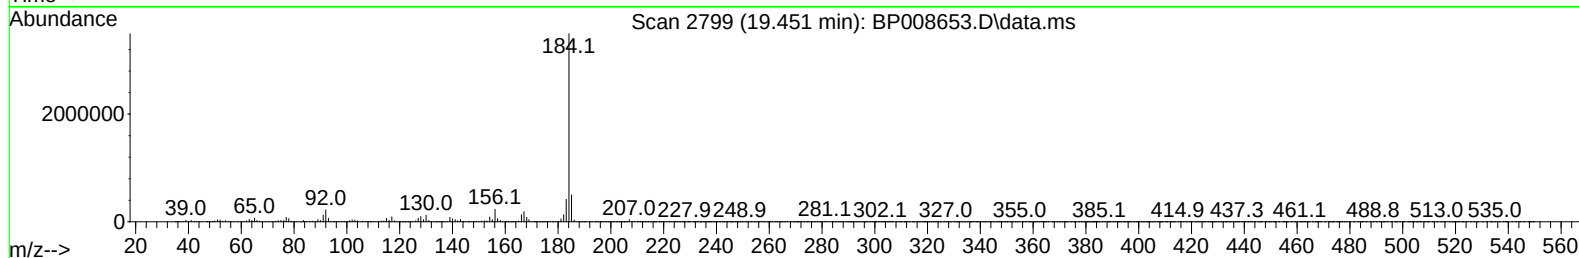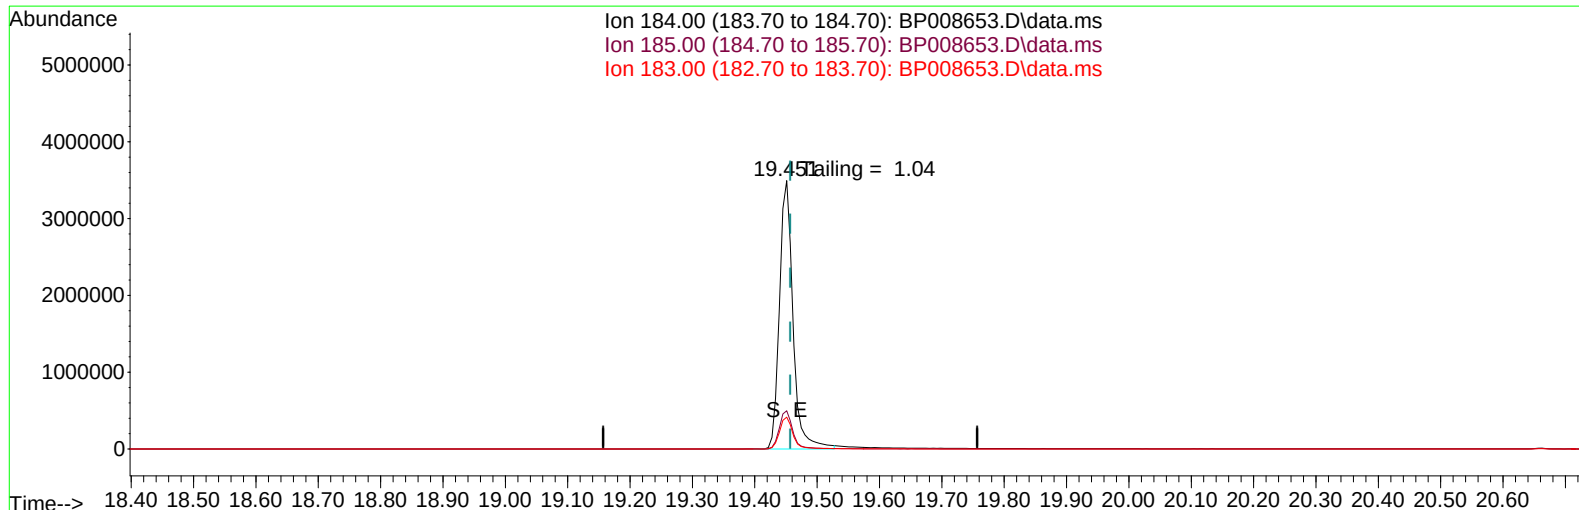

TIC: BP008653.D\data.ms

(77) Benzidine

19.451min (-0.006) 369849.25 ng

response 5433550

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.25
183.00	11.90	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/4/2022	BNA_P	<u>BP008653.D</u>
Compound Name	Response	Retention Time
DDT	3364841	20.66
DDD	95716	20.22
DDE	4998	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
100714	3465555	2.91