
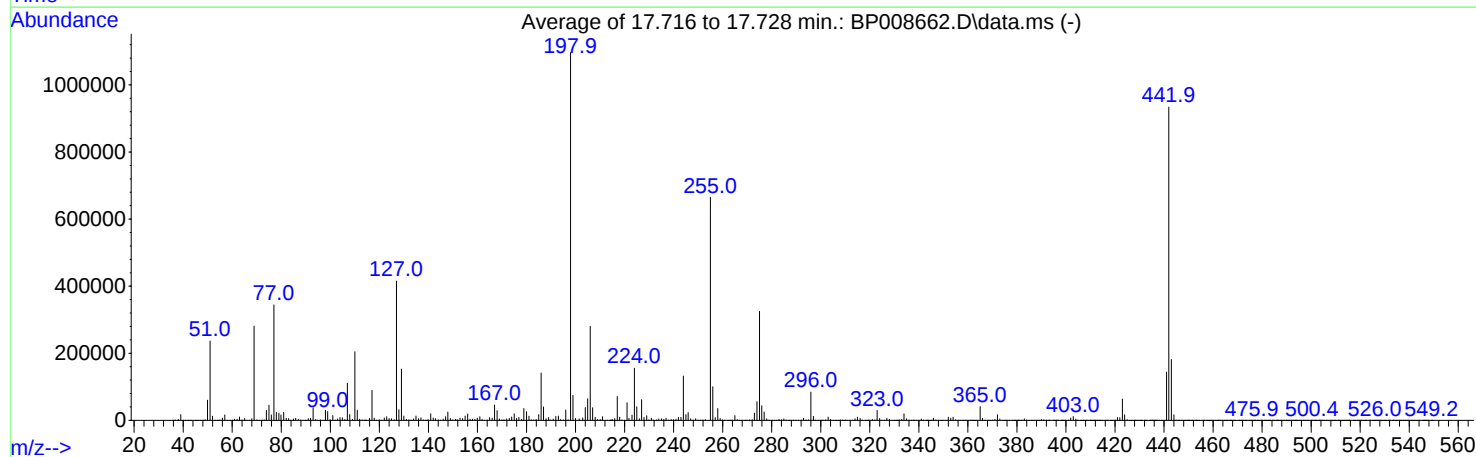


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
 Data File : BP008662.D
 Acq On : 04 Jan 2022 15:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 08:44:33 2021

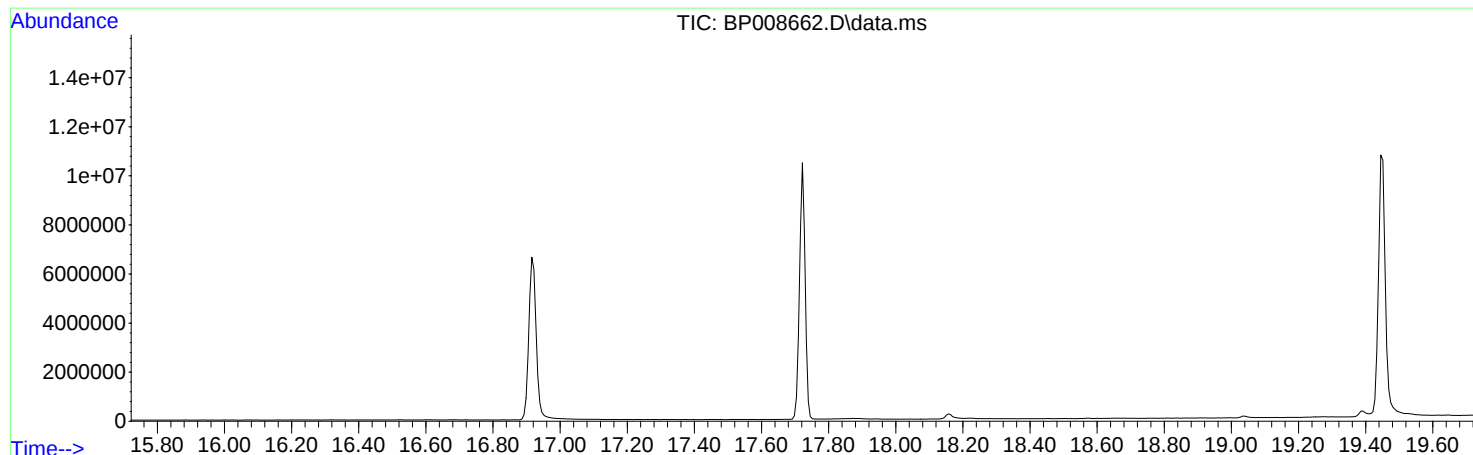

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.6	236562	PASS
68	69	0.00	2	1.8	4941	PASS
69	198	0.00	100	25.6	280903	PASS
70	69	0.00	2	0.6	1640	PASS
127	198	10	80	37.9	415265	PASS
197	198	0.00	2	0.1	1413	PASS
198	198	100	100	100.0	1096629	PASS
199	198	5	9	6.8	74387	PASS
275	198	10	60	29.6	324693	PASS
365	198	1	100	3.7	40912	PASS
441	198	0.01	100	13.1	144198	PASS
442	442	100	100	100.0	934186	PASS
443	442	15	24	19.4	181437	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/4/2022	BNA_P	<u>BP008662.D</u>
Compound Name	Response	Retention Time
DDT	3877054	20.657
DDD	83795	20.227
DDE	3543	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
87338	3964392	2.20

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
 Data File : BP008662.D
 Acq On : 04 Jan 2022 15:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 05 05:45:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

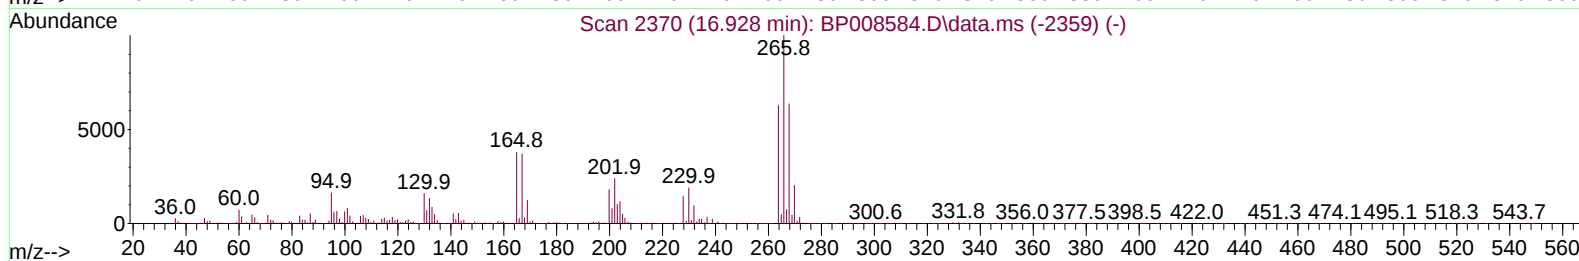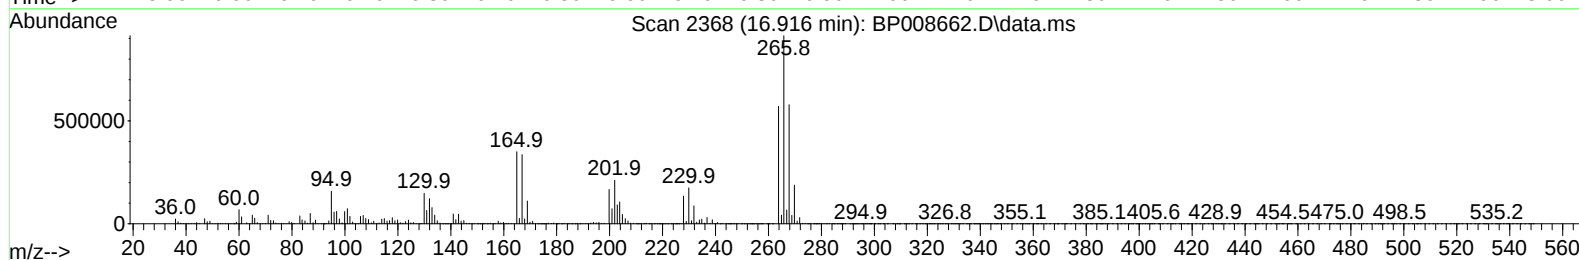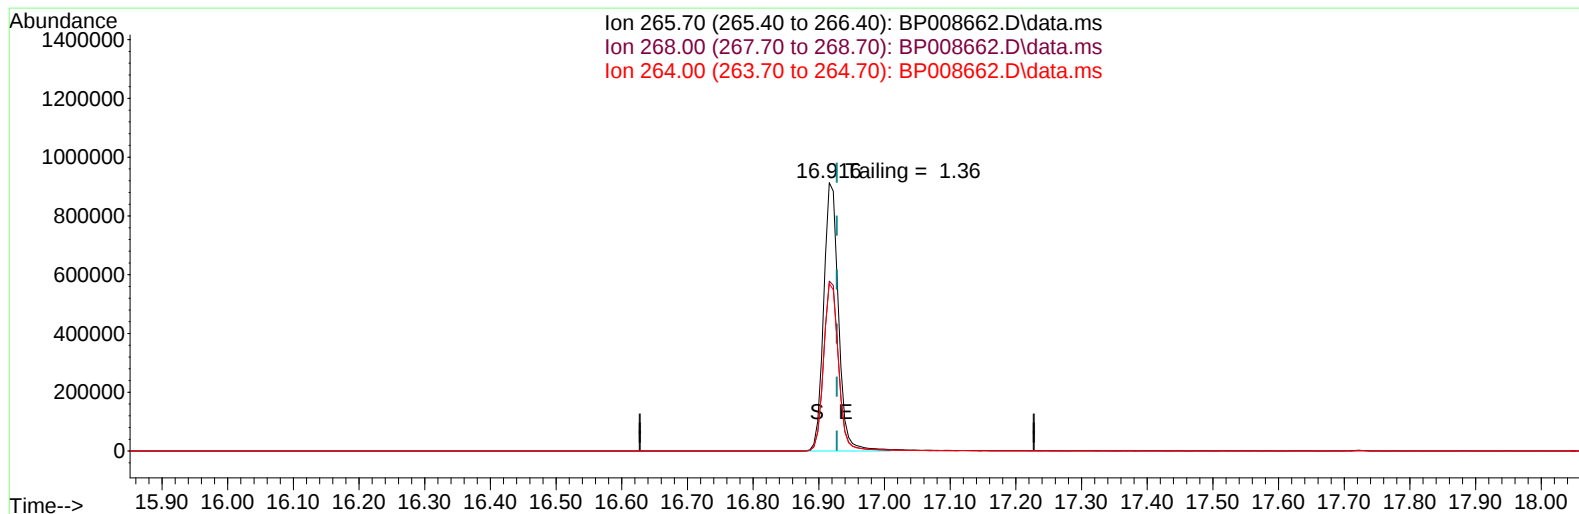

TIC: BP008662.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.012) 173056.06 ng




response 1439485

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.35
264.00	62.90	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010422\
Data File : BP008662.D
Acq On : 04 Jan 2022 15:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 05 05:45:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

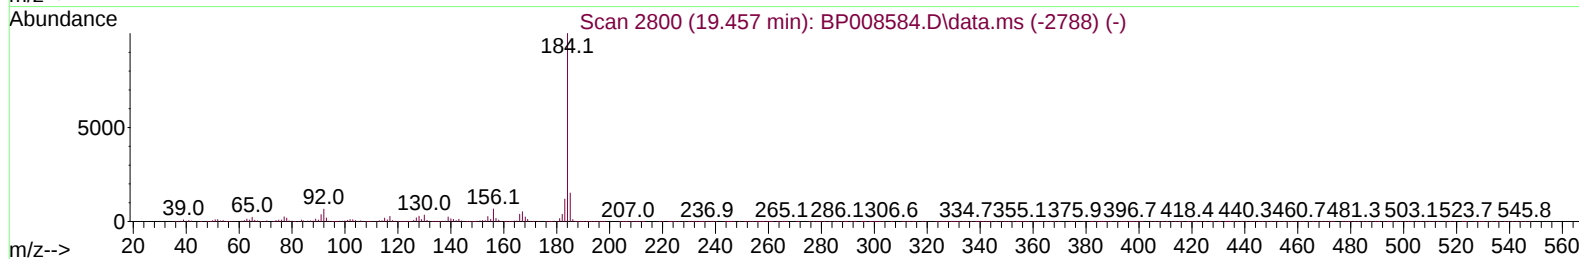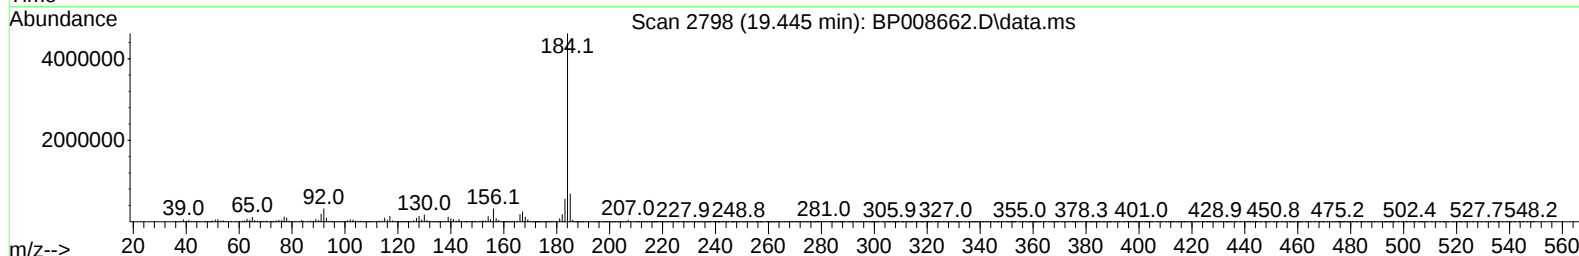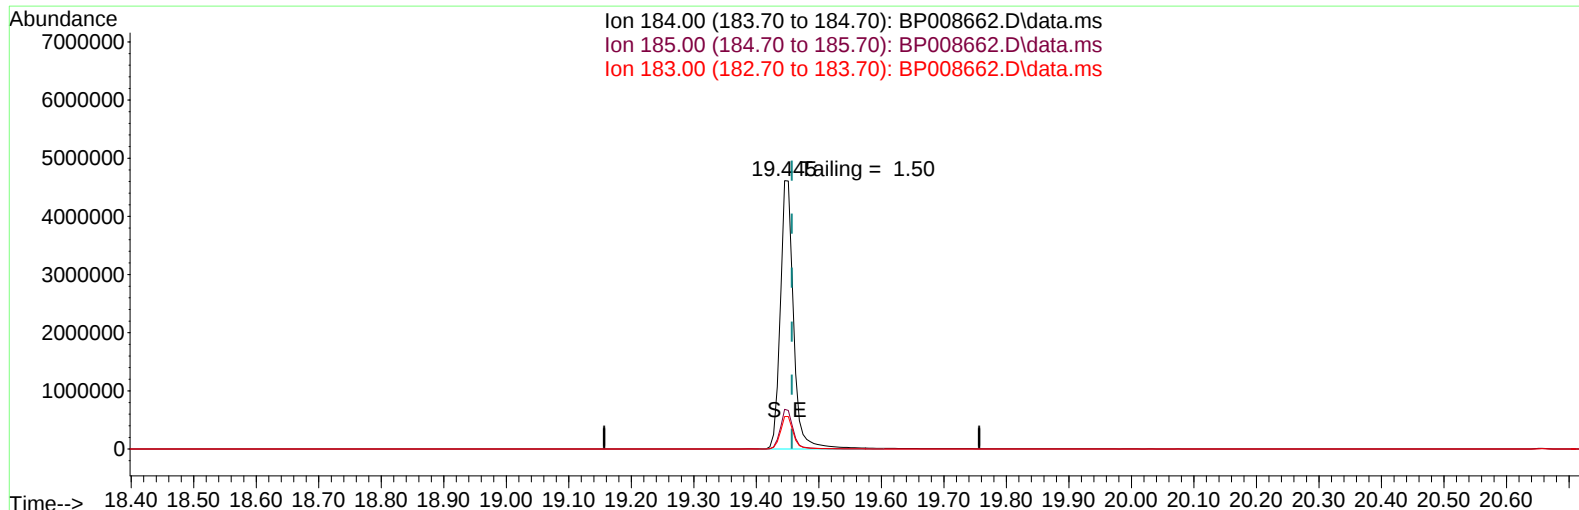

TIC: BP008662.D\data.ms

(77) Benzidine

19.445min (-0.012) 56830.30 ng

response 6858543

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.83
183.00	11.90	12.12
0.00	0.00	0.00