
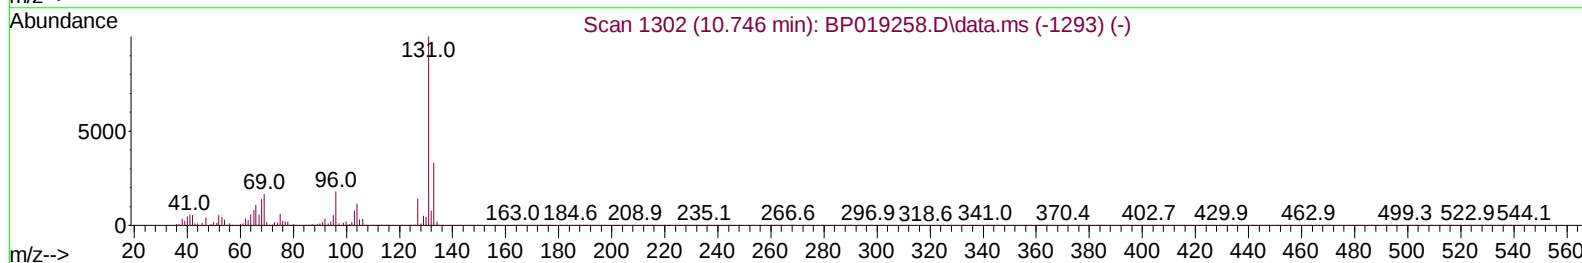
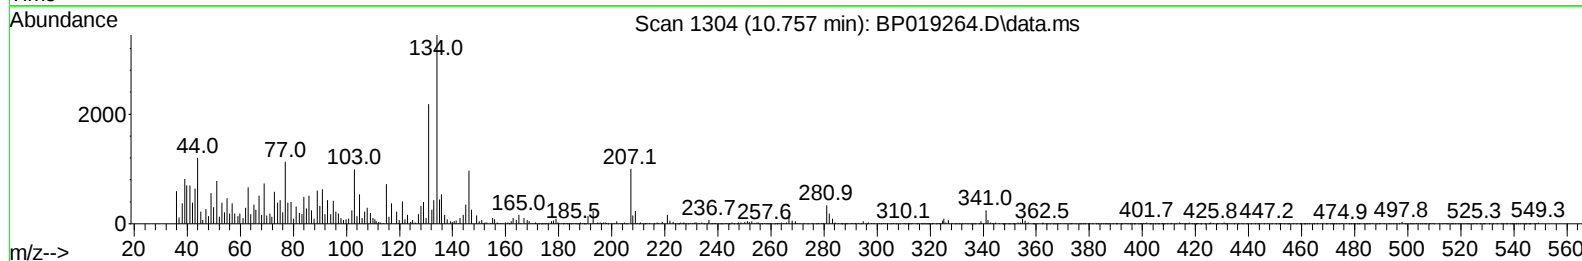


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019264.D
Acq On : 04 Jan 2024 15:24
Operator : MA/JU
Sample : 05951-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 04 15:51:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

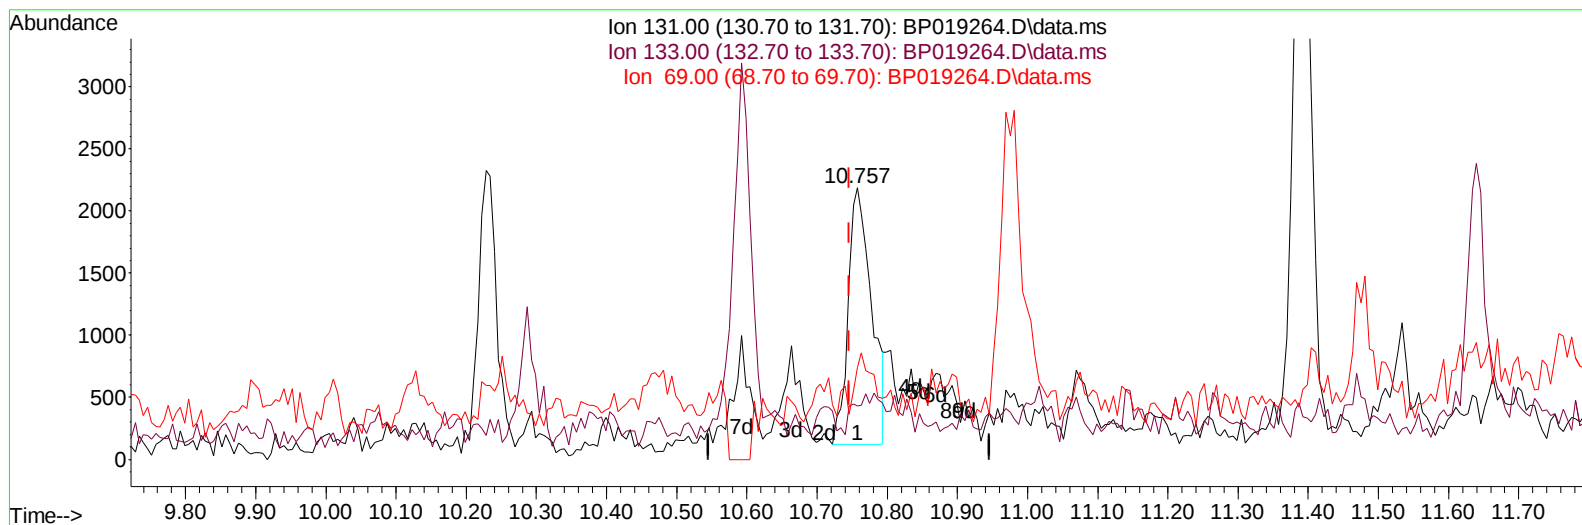

TIC: BP019264.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.757min (+ 0.012) 0.34 ng/ul

response 4791

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	19.67#
69.00	16.10	33.90#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019264.D
Acq On : 04 Jan 2024 15:24
Operator : MA/JU
Sample : 05951-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 04 15:51:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

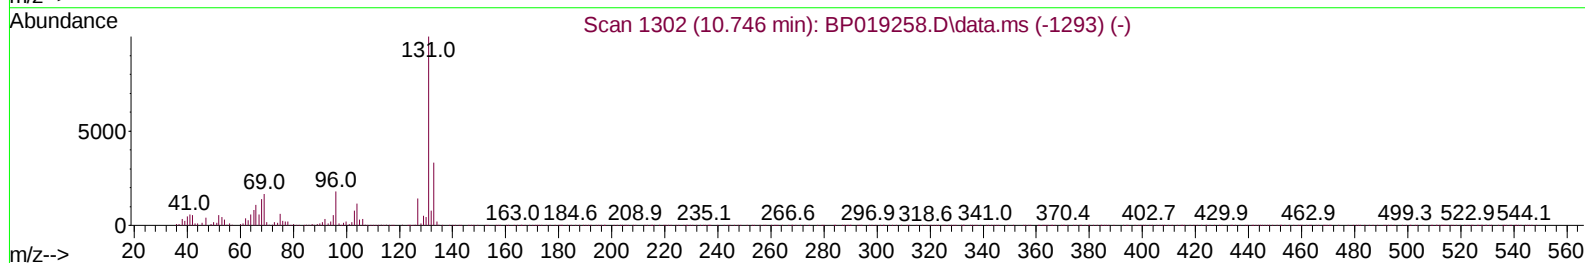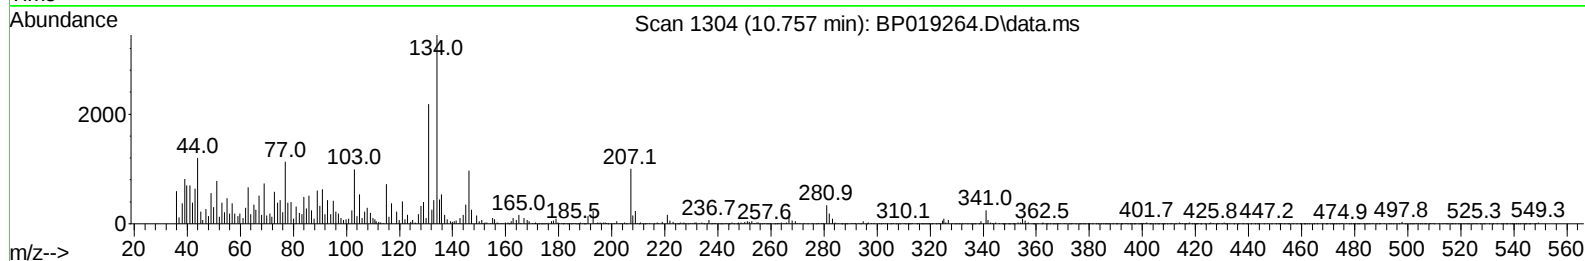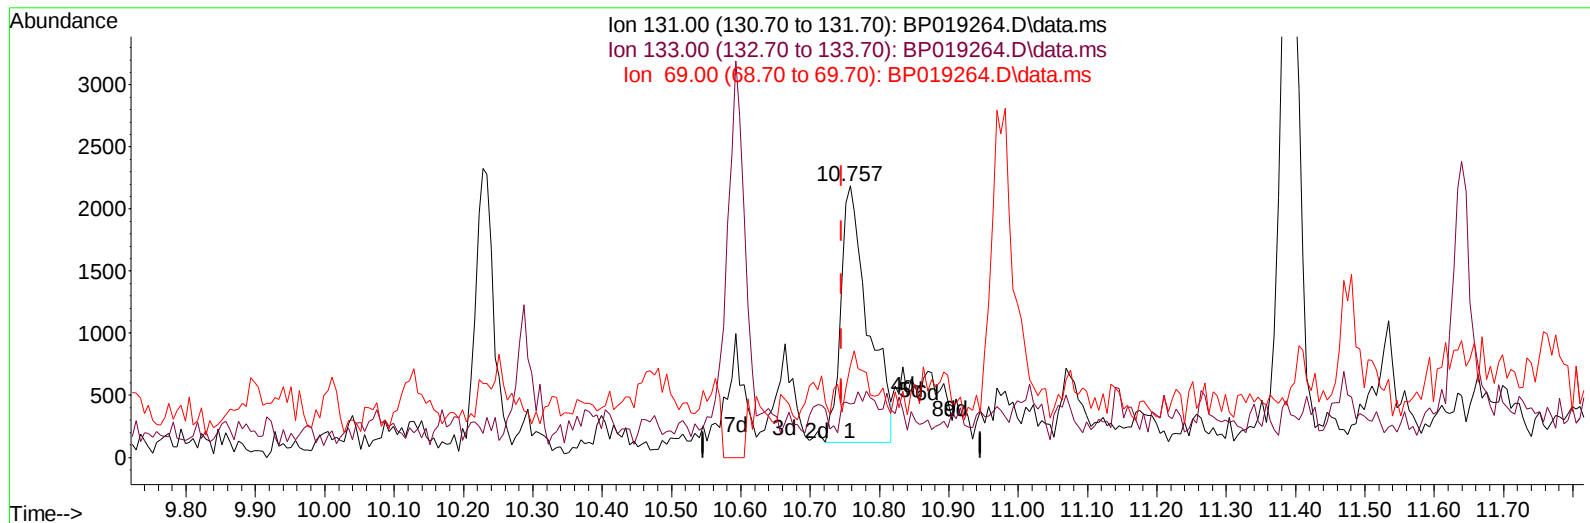

TIC: BP019264.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.757min (+ 0.012) 0.39 ng/ul m

response 5610

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	19.67#
69.00	16.10	33.90#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019264.D
Acq On : 04 Jan 2024 15:24
Operator : MA/JU
Sample : 05951-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 04 15:51:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

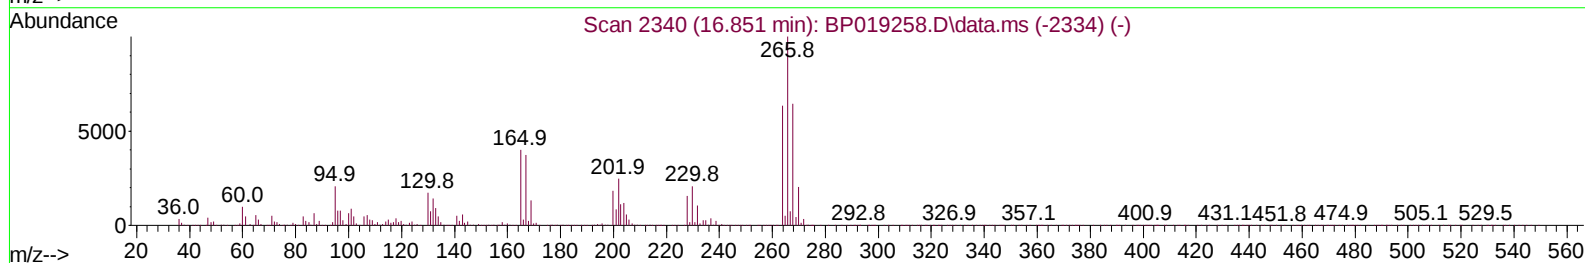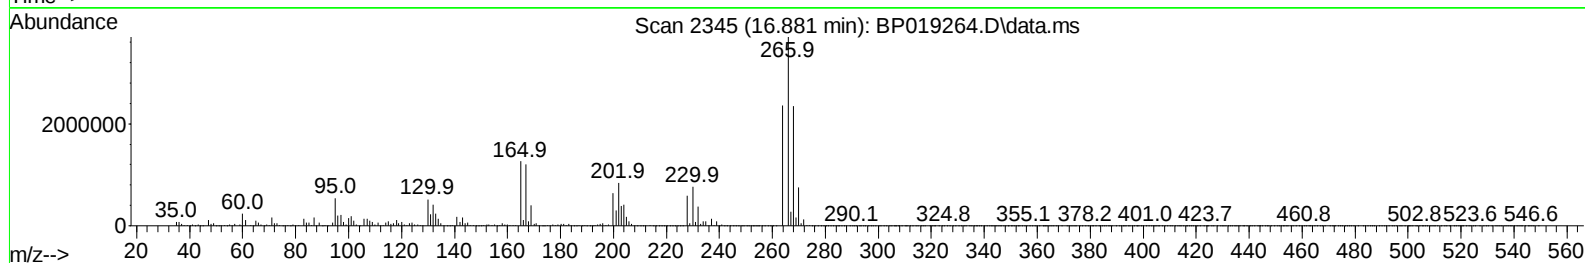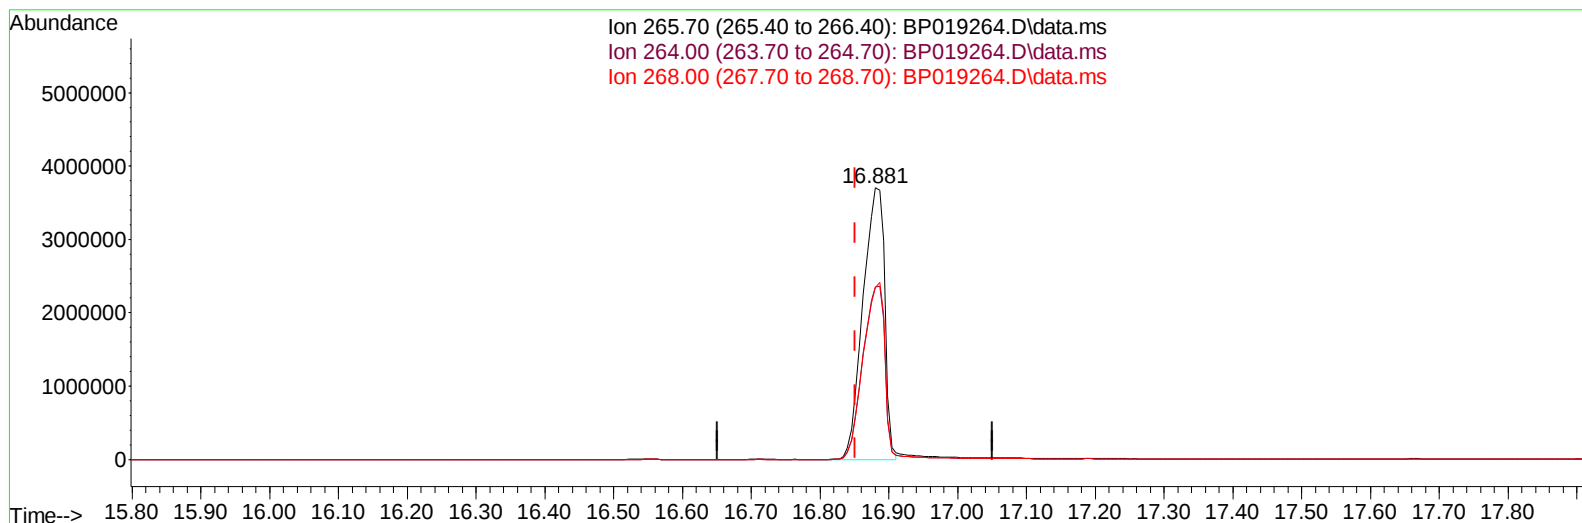

TIC: BP019264.D\data.ms

(71) Pentachlorophenol (C)




16.881min (+ 0.029) 1129.24 ng/u1

response 8103756

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	62.50	63.60
268.00	66.00	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019264.D
Acq On : 04 Jan 2024 15:24
Operator : MA/JU
Sample : 05951-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 04 15:51:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

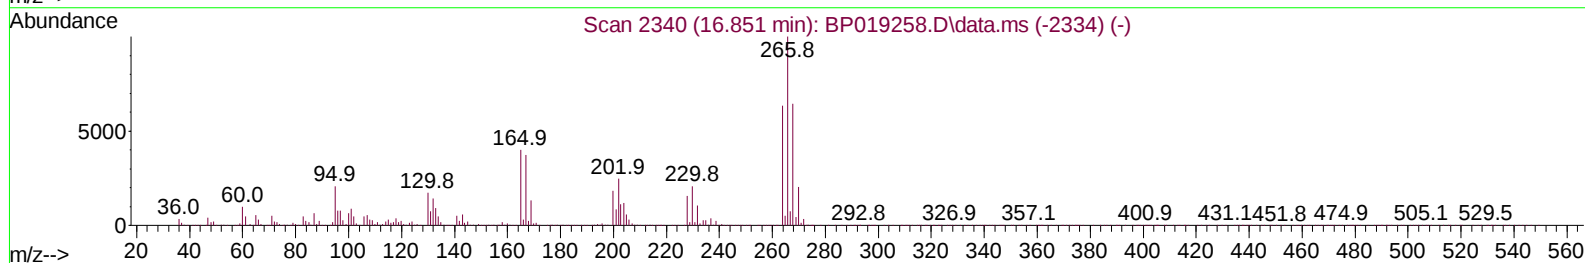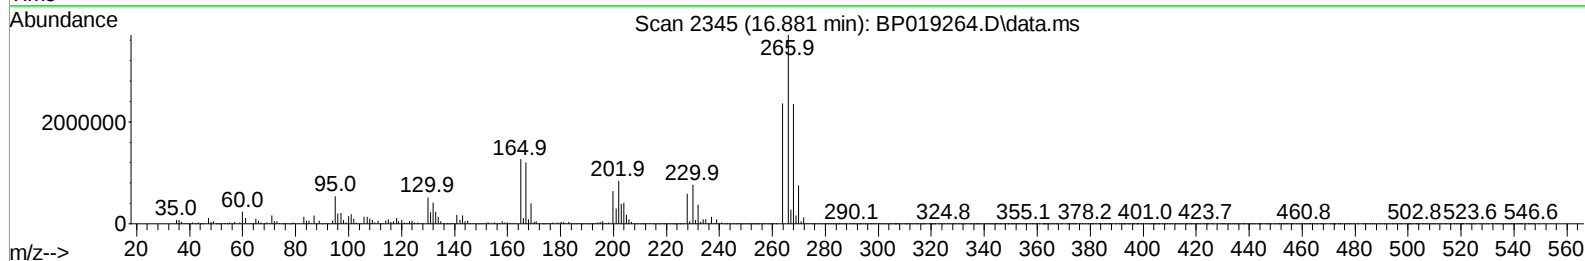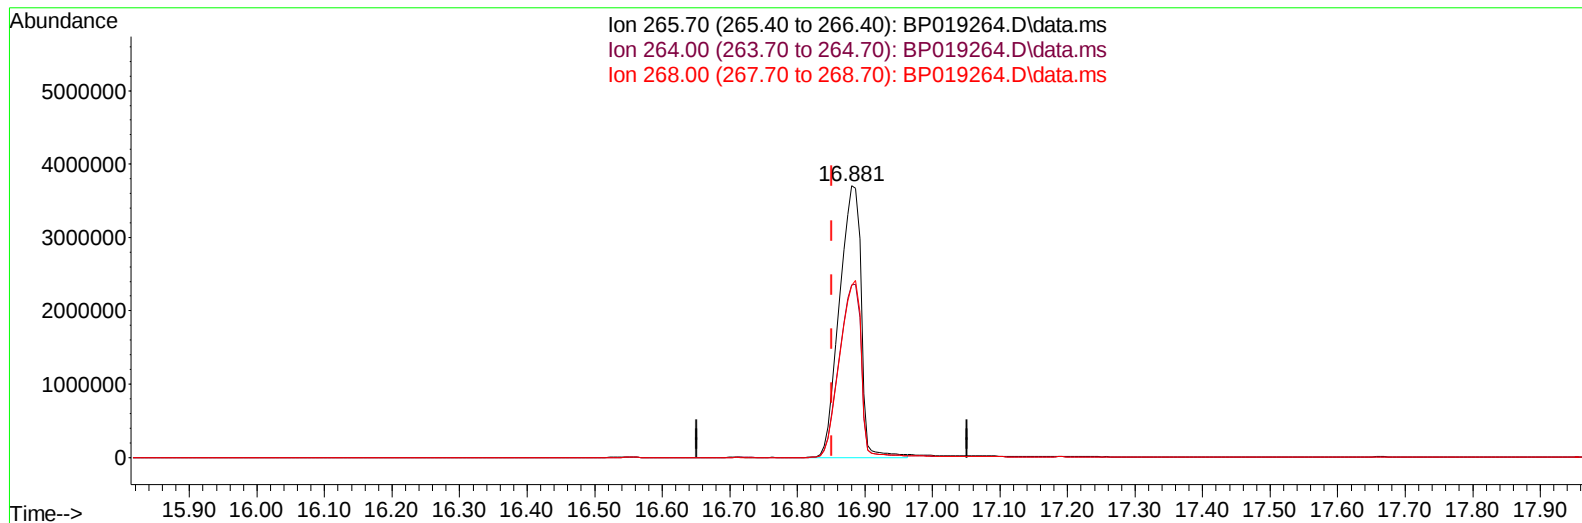

TIC: BP019264.D\data.ms

(71) Pentachlorophenol (C)




16.881min (+ 0.029) 1152.92 ng/ul m

response 8273697

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	62.50	63.60
268.00	66.00	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019264.D
Acq On : 04 Jan 2024 15:24
Operator : MA/JU
Sample : 05951-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 04 15:51:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

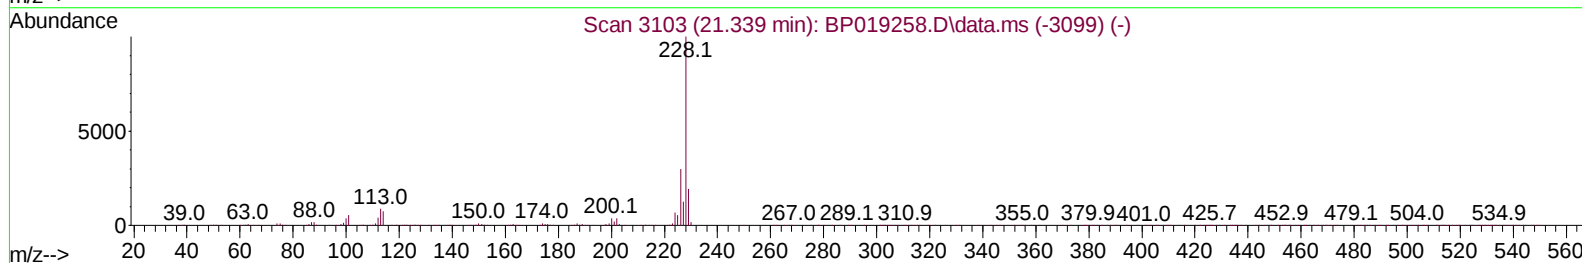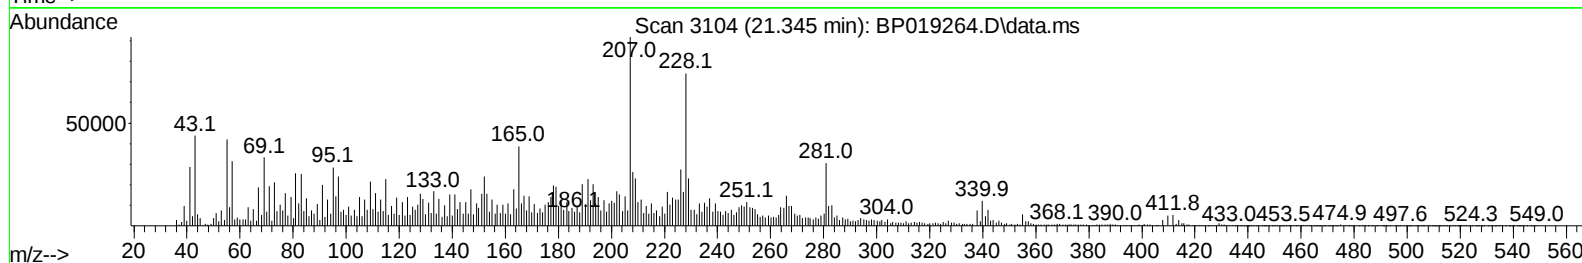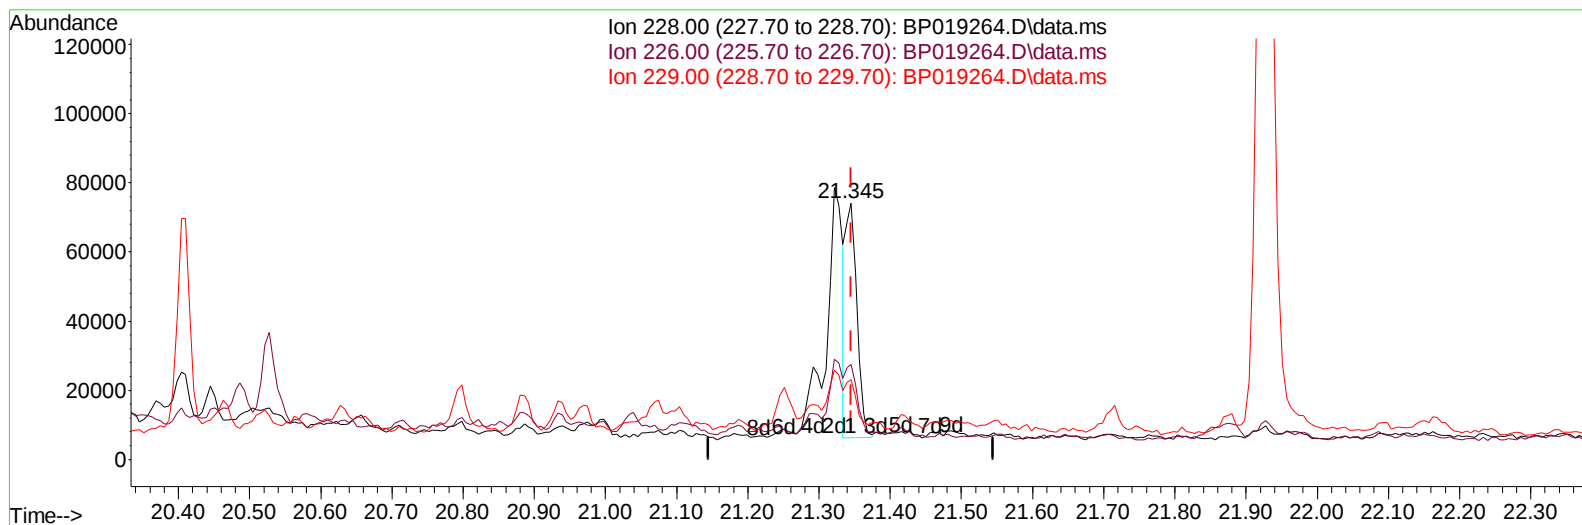




TIC: BP019264.D\data.ms

(87) Chrysene**21.345min (-0.000) 1.06 ng/u1****response 73980**

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.30	37.03#
229.00	19.50	31.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019264.D
Acq On : 04 Jan 2024 15:24
Operator : MA/JU
Sample : 05951-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 04 15:51:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

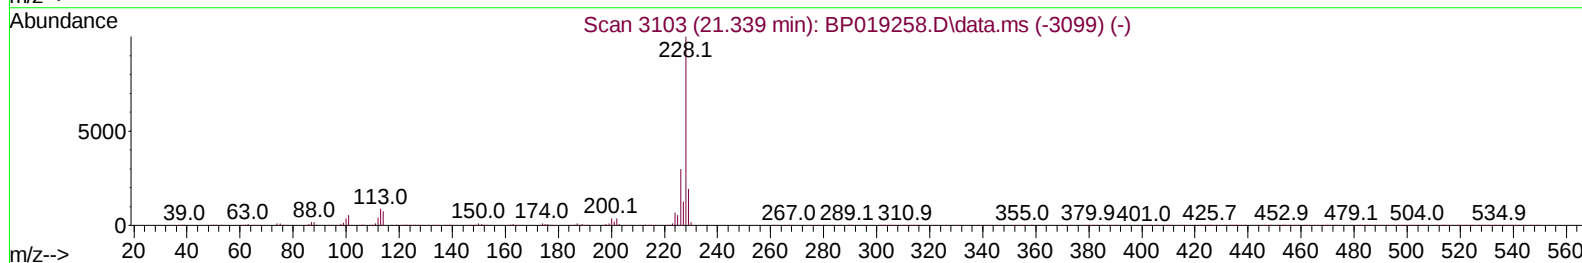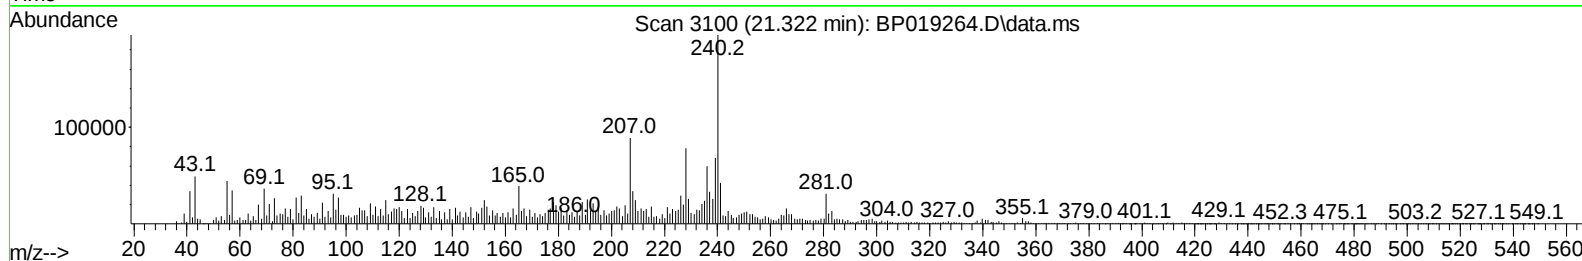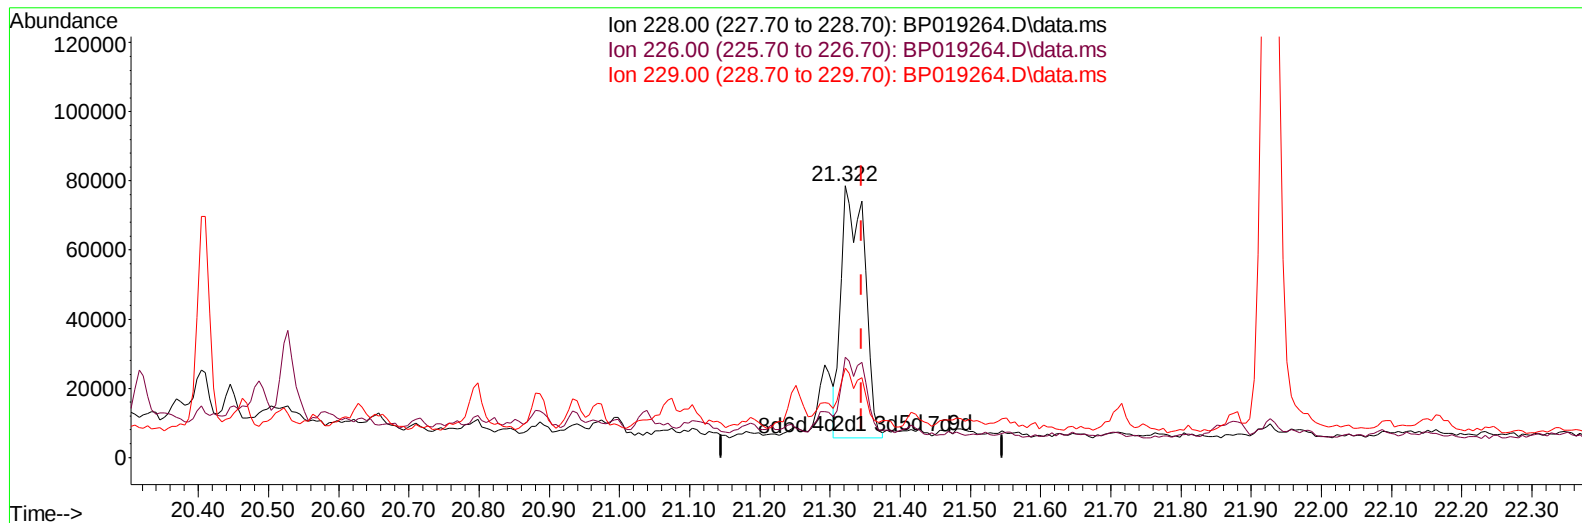

TIC: BP019264.D\data.ms

(87) Chrysene

21.322min (-0.024) 2.42 ng/u1 m

response 168716

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.30	36.97#
229.00	19.50	32.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
 Data File : BP019264.D
 Acq On : 04 Jan 2024 15:24
 Operator : MA/JU
 Sample : 05951-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 05 01:17:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	172843	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.593	136	615544	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.440	164	379204	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	804701	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	945485	20.000	ng/ul	0.00
88) Perylene-d12	23.680	264	1136378	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	7791	1.539	ng/uL	0.00
4) Pyridine-d5	3.670	84	48412	3.811	ng/ul	0.02
7) Phenol-d5	6.987	99	152865	9.862	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	90373	10.078	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	122618	9.813	ng/ul	0.00
15) 4-Methylphenol-d8	8.528	113	114426	9.482	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	57627	10.830	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	65858	11.452	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	123881	10.668	ng/ul	0.00
31) 4-Chloroaniline-d4	10.757	131	5610m	0.393	ng/ul	0.01
46) Dimethylphthalate-d6	13.857	166	354665	10.589	ng/ul	-0.01
49) Acenaphthylene-d8	14.134	160	437400	12.035	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	59558	10.530	ng/ul	0.02
60) Fluorene-d10	15.440	176	322841	11.157	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	55515	10.523	ng/ul	0.00
73) Anthracene-d10	17.304	188	497217	11.832	ng/ul	0.00
81) Pyrene-d10	19.551	212	649267	11.268	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.527	264	744353	11.396	ng/ul	0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.628	105	32578	1.803	ng/ul	91
50) Acenaphthylene	14.163	152	91398	2.235	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.081	232	196907	22.779	ng/ul#	98
71) Pentachlorophenol	16.881	266	8273697m	1152.919	ng/ul	
72) Phenanthrene	17.251	178	199285	4.087	ng/ul#	83
74) Anthracene	17.339	178	258463	5.324	ng/ul#	90
77) Carbazole	17.622	167	118646	2.938	ng/ul#	65
82) Pyrene	19.581	202	302708	4.370	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.216	149	74709	2.050	ng/ul#	77
87) Chrysene	21.322	228	168716m	2.422	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019264.D
Acq On : 04 Jan 2024 15:24
Operator : MA/JU
Sample : 05951-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 05 01:17:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

