
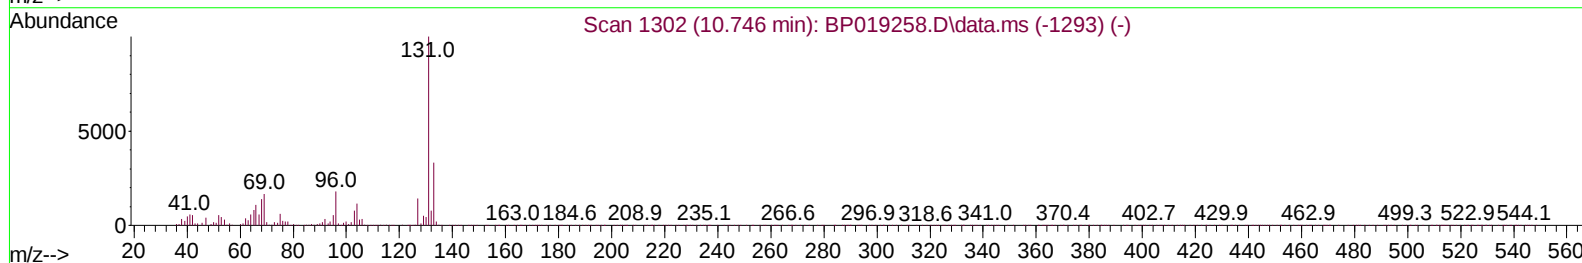
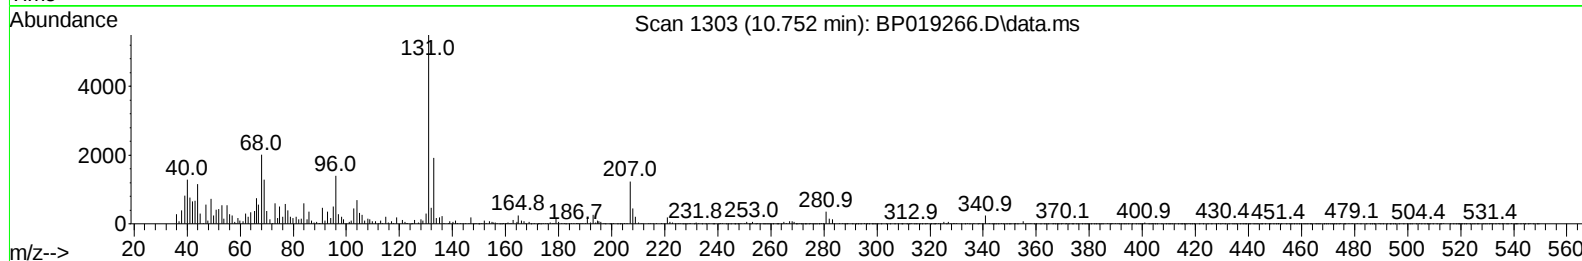


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019266.D
Acq On : 04 Jan 2024 16:32
Operator : MA/JU
Sample : 05951-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 04 17:00:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

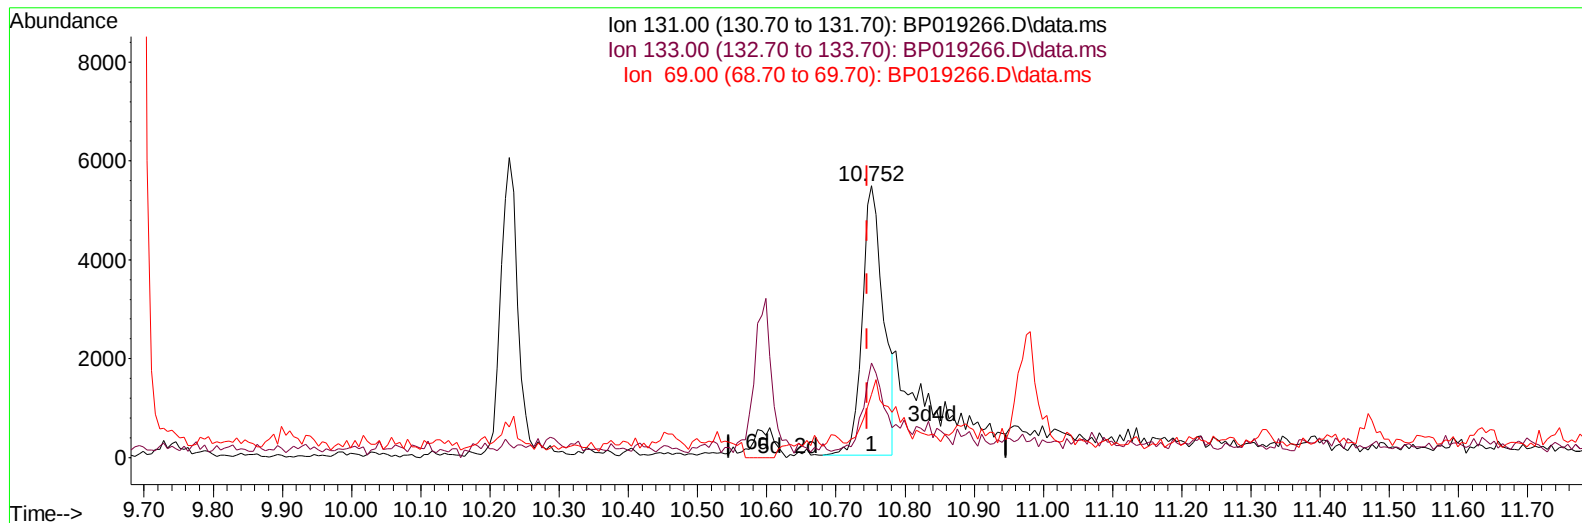

TIC: BP019266.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.752min (+ 0.006) 0.78 ng/u1

response 11568

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	34.87
69.00	16.10	23.33#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019266.D
Acq On : 04 Jan 2024 16:32
Operator : MA/JU
Sample : 05951-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 04 17:00:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

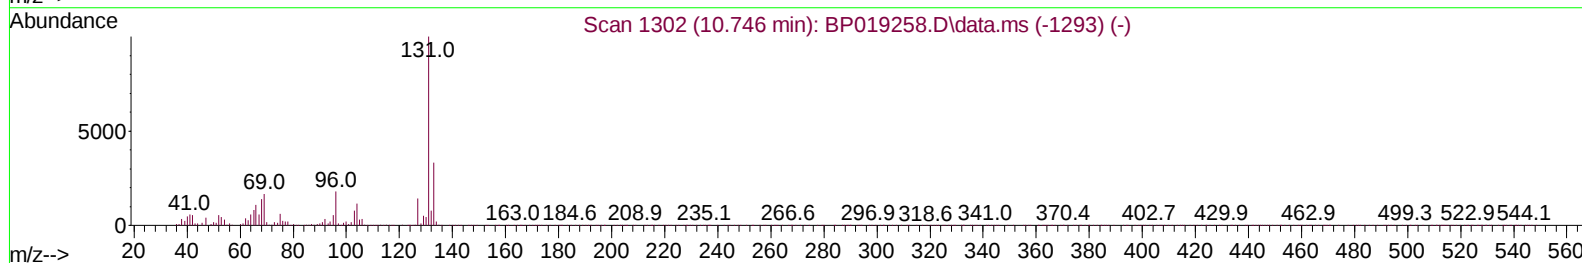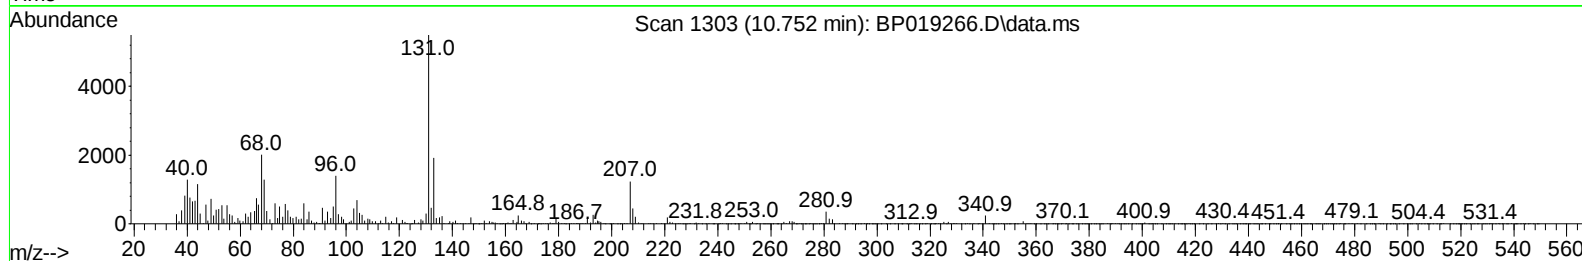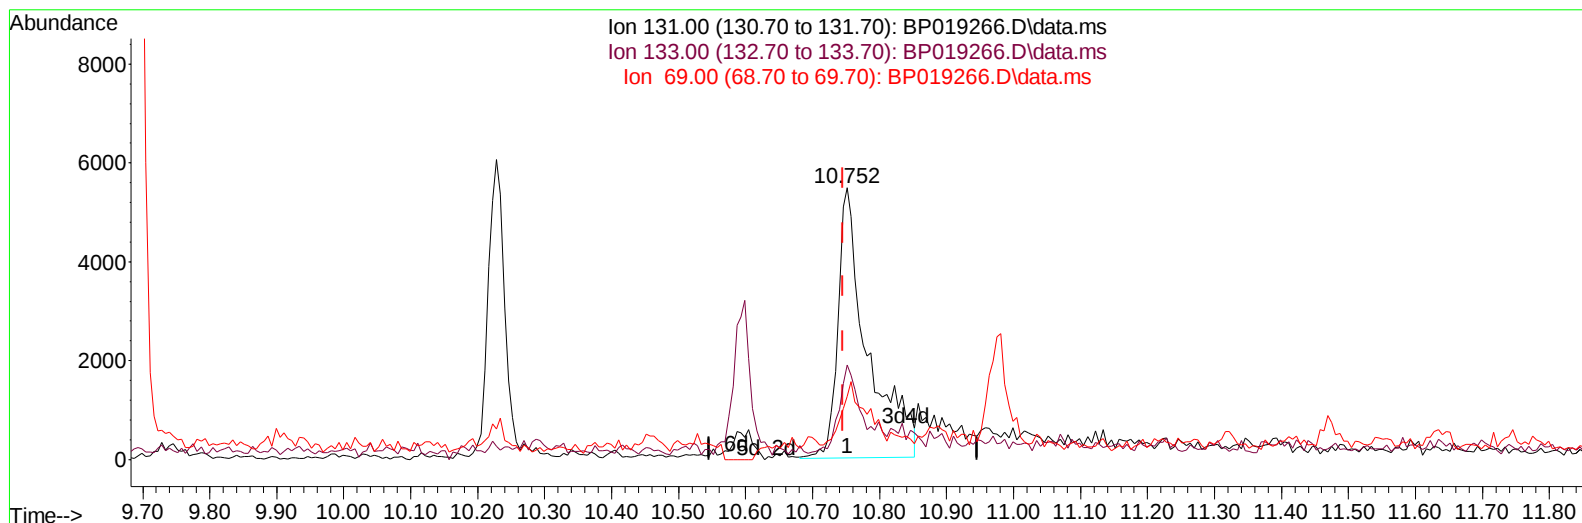

TIC: BP019266.D\data.ms

(31) 4-Chloroaniline-d4 (S)**10.752min (+ 0.006) 1.13 ng/ul m****response 16740**

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	34.87
69.00	16.10	23.33#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
 Data File : BP019266.D
 Acq On : 04 Jan 2024 16:32
 Operator : MA/JU
 Sample : 05951-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 04 17:01:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	167186	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.593	136	637742	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.440	164	391911	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	927384	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	966691	20.000	ng/ul	0.00
88) Perylene-d12	23.674	264	1164882	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	19023	3.886	ng/uL	0.00
4) Pyridine-d5	3.658	84	254314	20.698	ng/ul	0.00
7) Phenol-d5	6.987	99	386568	25.783	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	224274	25.857	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	303779	25.133	ng/ul	0.00
15) 4-Methylphenol-d8	8.528	113	284212	24.349	ng/ul	0.00
21) Nitrobenzene-d5	8.963	128	151753	27.527	ng/ul	0.00
24) 2-Nitrophenol-d4	9.681	143	174590	29.303	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	315492	26.223	ng/ul	0.00
31) 4-Chloroaniline-d4	10.752	131	16740m	1.131	ng/ul	0.00
46) Dimethylphthalate-d6	13.857	166	874428	25.260	ng/ul	-0.01
49) Acenaphthylene-d8	14.134	160	1046734	27.868	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	149295	25.540	ng/ul	0.02
60) Fluorene-d10	15.440	176	804433	26.899	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	115992	19.079	ng/ul	0.00
73) Anthracene-d10	17.298	188	1214717	25.081	ng/ul	0.00
81) Pyrene-d10	19.545	212	1619446	27.488	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.516	264	1740065	25.988	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.857	266	92713	11.210	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019266.D
Acq On : 04 Jan 2024 16:32
Operator : MA/JU
Sample : 05951-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jan 04 17:01:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

