

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
 Data File : BP019267.D
 Acq On : 04 Jan 2024 17:06
 Operator : MA/JU
 Sample : 05951-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF79

Quant Time: Jan 04 17:46:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	163324	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.593	136	628025	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.440	164	404221	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	952374	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	1035938	20.000	ng/u1	0.00
88) Perylene-d12	23.668	264	1250063	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	11907	2.490	ng/uL	0.00
4) Pyridine-d5	3.664	84	29264	2.438	ng/u1	0.01
7) Phenol-d5	6.987	99	251822	17.193	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	146122	17.245	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	199172	16.868	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	197770	17.344	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	99156	18.264	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	110307	18.800	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	208306	17.582	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	192543	13.212	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	598323	16.758	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	765426	19.758	ng/u1	0.00
54) 4-Nitrophenol-d4	14.692	143	80721	13.389	ng/u1	0.03
60) Fluorene-d10	15.439	176	600365	19.464	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	68758	11.013	ng/u1	0.00
73) Anthracene-d10	17.298	188	898388	18.063	ng/u1	0.00
81) Pyrene-d10	19.545	212	1247089	19.753	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.515	264	1363746	18.980	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.851	266	184838	21.763	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019267.D
Acq On : 04 Jan 2024 17:06
Operator : MA/JU
Sample : 05951-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF79

Quant Time: Jan 04 17:46:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

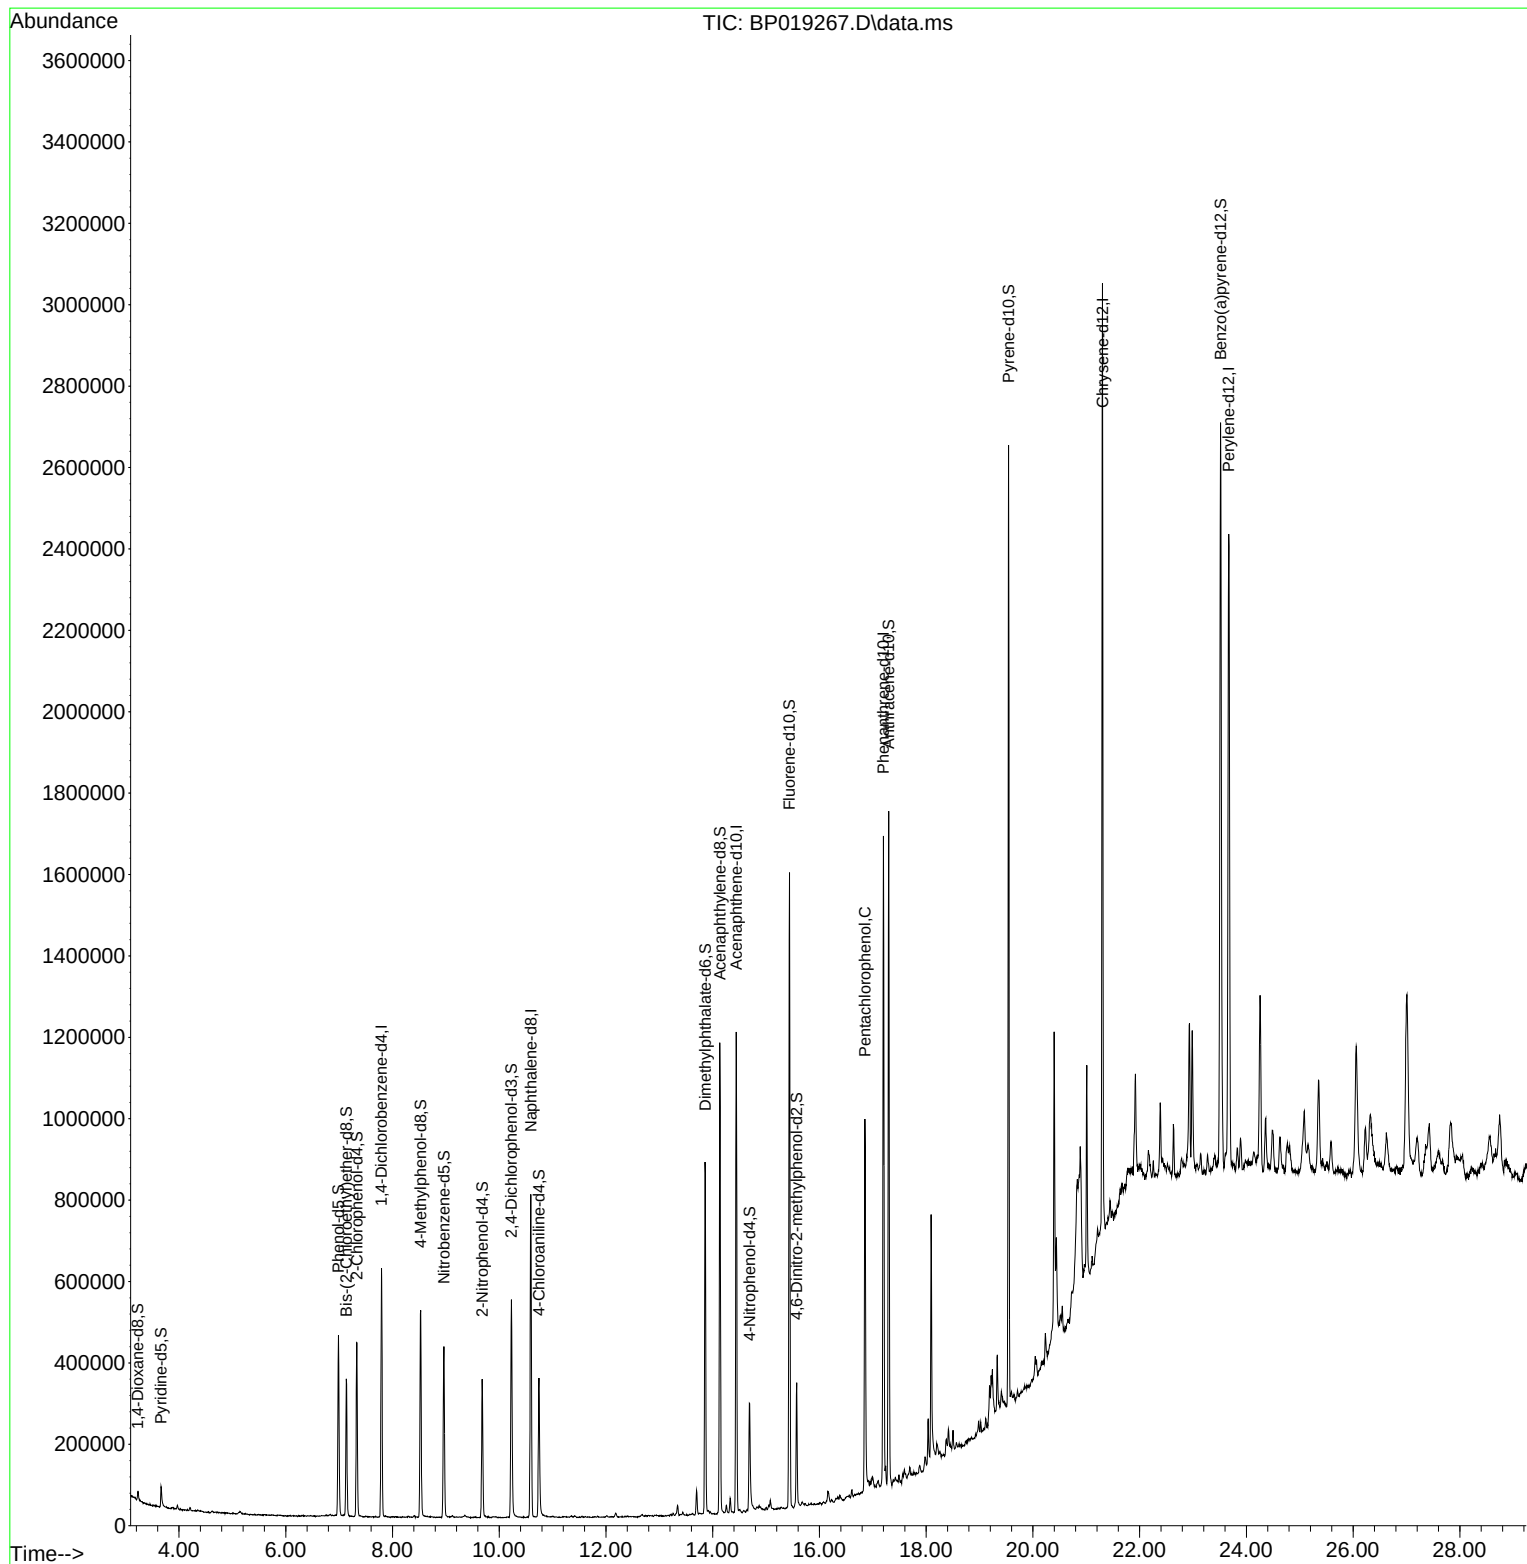

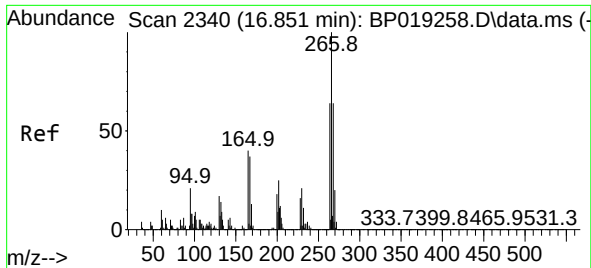

#71
 Pentachlorophenol
 Concen: 21.763 ng/ul
 RT: 16.851 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP019267.D
 Acq: 04 Jan 2024 17:06

Instrument :
 BNA_P
 ClientSampleId :
 GCF79

Tgt Ion:266 Resp: 184838
 Ion Ratio Lower Upper
 266 100
 264 62.0 50.0 75.0
 268 64.1 52.8 79.2

