

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
 Data File : BP019268.D
 Acq On : 04 Jan 2024 17:40
 Operator : MA/JU
 Sample : 05951-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF80

Quant Time: Jan 04 18:08:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 29 03:48:11 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	135483	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.593	136	512593	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.440	164	324894	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.198	188	763914	20.000	ng/u1	0.00
79) Chrysene-d12	21.304	240	809912	20.000	ng/u1	0.00
88) Perylene-d12	23.669	264	957335	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	13509	3.405	ng/uL	0.00
4) Pyridine-d5	3.652	84	162310	16.301	ng/u1	0.00
7) Phenol-d5	6.987	99	246296	20.272	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	136058	19.357	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	192408	19.644	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	177929	18.810	ng/u1	0.00
21) Nitrobenzene-d5	8.963	128	91191	20.580	ng/u1	0.00
24) 2-Nitrophenol-d4	9.681	143	105942	22.123	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.228	165	197870	20.462	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	173635	14.598	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	568228	19.801	ng/u1	0.00
49) Acenaphthylene-d8	14.134	160	664530	21.341	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	89534	18.476	ng/u1	0.02
60) Fluorene-d10	15.434	176	516099	20.817	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.575	200	75311	15.038	ng/u1	0.00
73) Anthracene-d10	17.298	188	818651	20.521	ng/u1	0.00
81) Pyrene-d10	19.545	212	1063633	21.549	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.516	264	1126814	20.477	ng/u1	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.851	266	86675	12.723	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019268.D
Acq On : 04 Jan 2024 17:40
Operator : MA/JU
Sample : 05951-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF80

Quant Time: Jan 04 18:08:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 29 03:48:11 2023
Response via : Initial Calibration

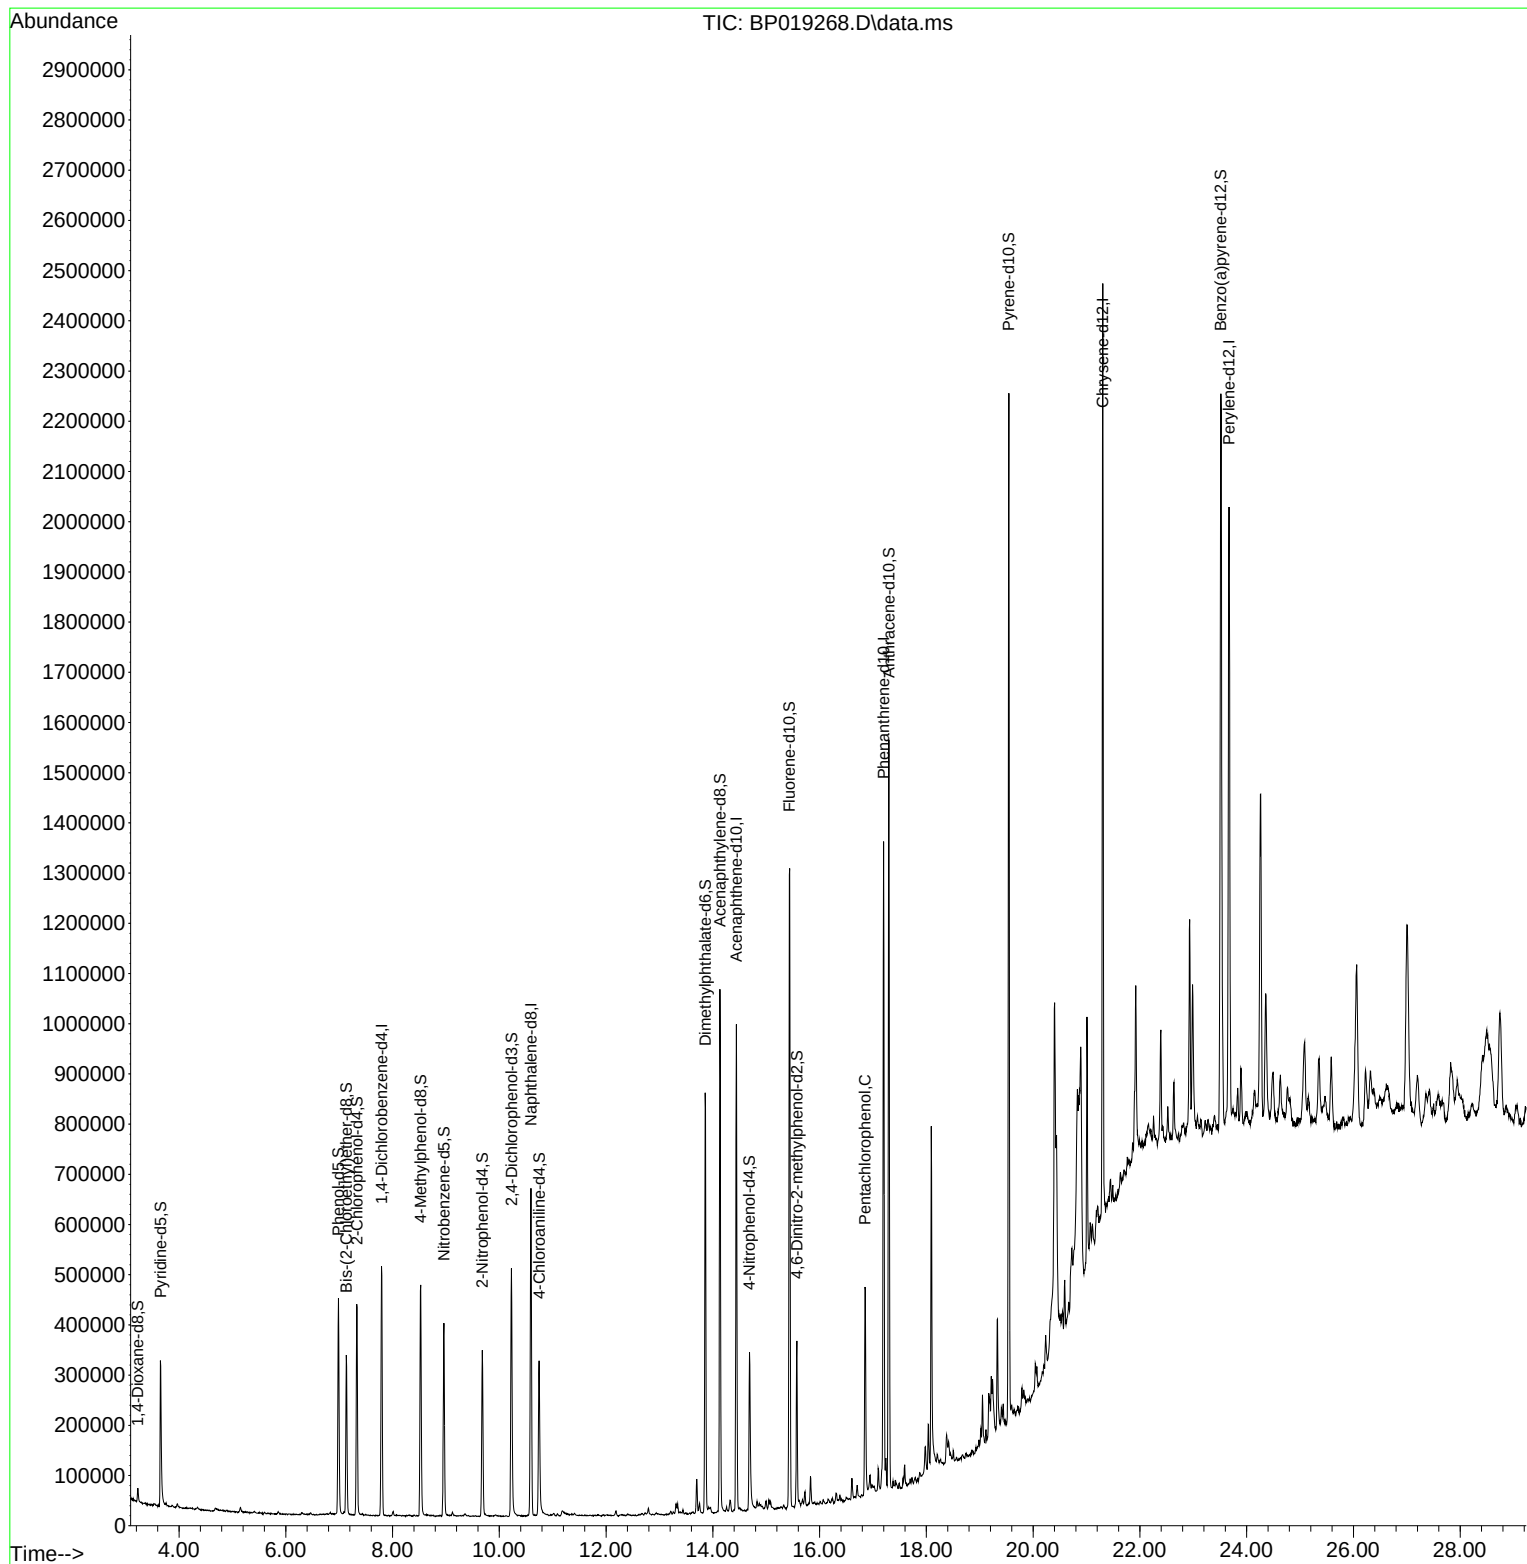

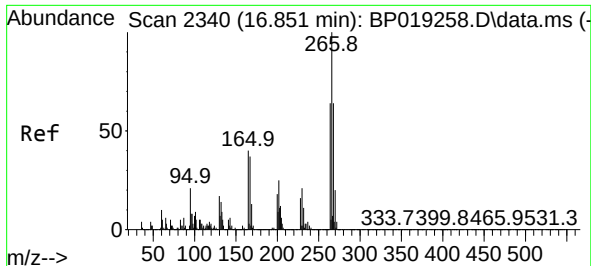

#71
 Pentachlorophenol
 Concen: 12.723 ng/ul
 RT: 16.851 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP019268.D
 Acq: 04 Jan 2024 17:40

Instrument :
 BNA_P
 ClientSampleId :
 GCF80

Tgt Ion:266 Resp: 86675
 Ion Ratio Lower Upper
 266 100
 264 63.3 50.0 75.0
 268 63.9 52.8 79.2

