

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
 Data File : BP019265.D
 Acq On : 04 Jan 2024 15:58
 Operator : MA/JU
 Sample : 05951-09DL 20X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCF73DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.975	147	151	156	rVB2	10410	13045	0.56%	0.108%
2	4.287	202	204	206	rBV3	3625	3237	0.14%	0.027%
3	4.981	319	322	326	rBV6	2183	2823	0.12%	0.023%
4	5.587	423	425	429	rVB5	2884	3278	0.14%	0.027%
5	6.463	571	574	575	rBV3	2645	3449	0.15%	0.029%
6	6.993	658	664	674	rVB	13725	27816	1.19%	0.231%
7	7.140	684	689	693	rBV	11730	17193	0.74%	0.143%
8	7.334	715	722	730	rBV	13896	24928	1.07%	0.207%
9	7.740	787	791	793	rBV5	2398	3177	0.14%	0.026%
10	7.793	793	800	809	rBV	488871	799096	34.22%	6.630%
11	8.010	835	837	843	rVB7	2082	3327	0.14%	0.028%
12	8.534	920	926	932	rBV2	12760	23765	1.02%	0.197%
13	8.969	993	1000	1006	rBV2	11495	21653	0.93%	0.180%
14	9.687	1118	1122	1128	rBV6	8691	16477	0.71%	0.137%
15	10.246	1210	1217	1224	rBV5	12484	34010	1.46%	0.282%
16	10.593	1269	1276	1286	rBV	607811	1005647	43.06%	8.344%
17	10.752	1296	1303	1306	rBV9	3383	7137	0.31%	0.059%
18	11.428	1415	1418	1421	rVB5	2425	2698	0.12%	0.022%
19	11.840	1485	1488	1494	rVB8	2915	5563	0.24%	0.046%
20	11.951	1504	1507	1510	rBV5	1858	2970	0.13%	0.025%
21	12.304	1563	1567	1569	rBV5	2016	2939	0.13%	0.024%
22	12.598	1613	1617	1619	rBV5	2509	3844	0.16%	0.032%
23	12.787	1648	1649	1653	rBV4	3214	4297	0.18%	0.036%
24	13.169	1712	1714	1718	rBV5	2695	3648	0.16%	0.030%
25	13.345	1741	1744	1748	rVB5	5632	5866	0.25%	0.049%
26	13.434	1757	1759	1760	rBV2	3911	3251	0.14%	0.027%
27	13.581	1780	1784	1786	rBV5	3386	3890	0.17%	0.032%
28	13.704	1800	1805	1809	rBV8	10260	18352	0.79%	0.152%
29	13.745	1809	1812	1820	rVB10	5870	13030	0.56%	0.108%
30	13.863	1827	1832	1838	rBV	31794	52346	2.24%	0.434%
31	14.134	1873	1878	1882	rBV	35065	53130	2.28%	0.441%
32	14.251	1896	1898	1903	rBV5	6749	8517	0.36%	0.071%
33	14.334	1909	1912	1916	rVB5	9360	11952	0.51%	0.099%
34	14.445	1924	1931	1947	rBV	810246	1259438	53.93%	10.449%
35	15.051	2031	2034	2035	rBV3	15019	14471	0.62%	0.120%
36	15.081	2036	2039	2048	rVB3	37838	57800	2.47%	0.480%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019265.D
Acq On : 04 Jan 2024 15:58
Operator : MA/JU
Sample : 05951-09DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF73DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	15.439	2096	2100	2106	rVB	51553	70200	3.01%	0.582%
38	16.175	2219	2225	2230	rBV7	26122	58106	2.49%	0.482%
39	16.857	2335	2341	2354	rBV	1460770	2335379	100.00%	19.376%
40	17.198	2394	2399	2410	rBV	1069087	1574719	67.43%	13.065%
41	17.298	2413	2416	2420	rVB	51370	69155	2.96%	0.574%
42	20.404	2941	2944	2946	rBV	163769	174574	7.48%	1.448%
43	21.304	3093	3097	3106	rVB	1679662	2099968	89.92%	17.423%
44	23.674	3495	3500	3507	rVB	1093800	2132642	91.32%	17.694%




Sum of corrected areas: 12052803

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019265.D
Acq On : 04 Jan 2024 15:58
Operator : MA/JU
Sample : 05951-09DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF73DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

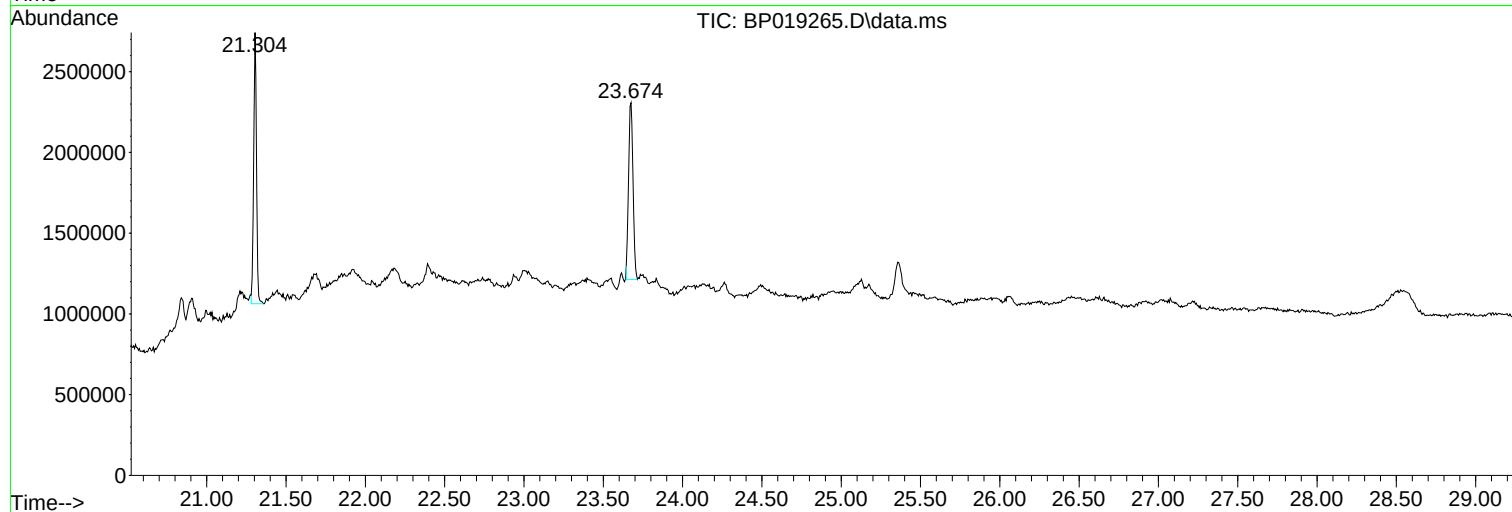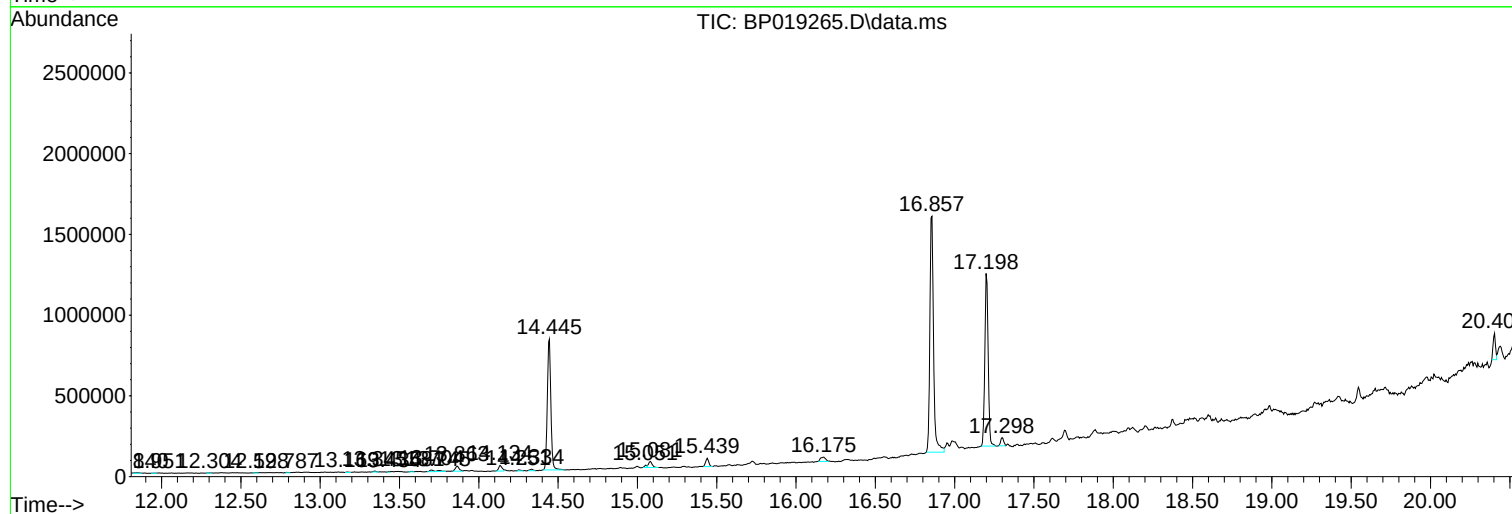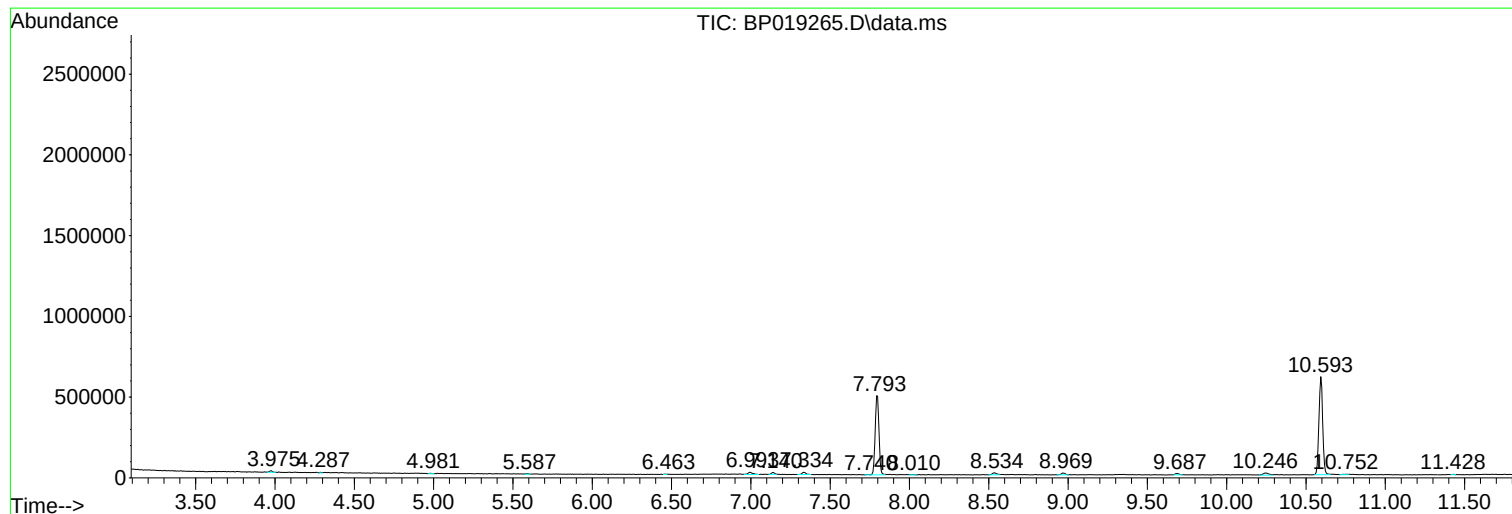

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019265.D
Acq On : 04 Jan 2024 15:58
Operator : MA/JU
Sample : 05951-09DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF73DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010424\
Data File : BP019265.D
Acq On : 04 Jan 2024 15:58
Operator : MA/JU
Sample : 05951-09DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCF73DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc