
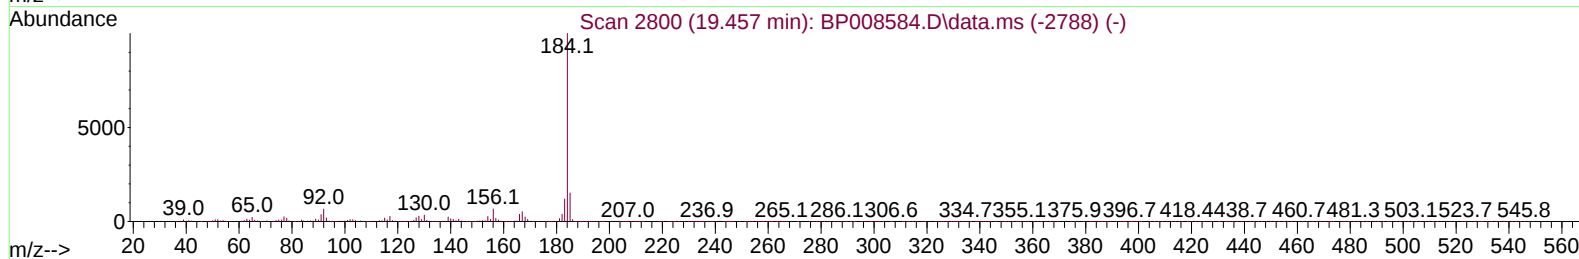
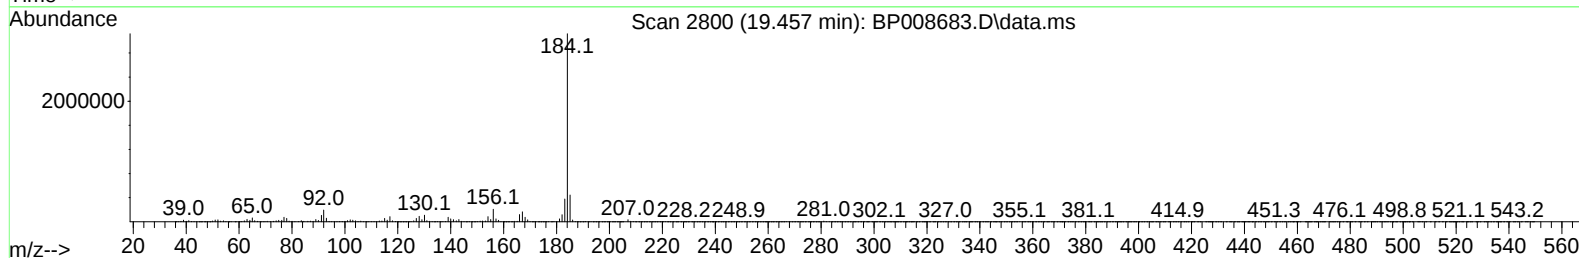


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
 Data File : BP008683.D
 Acq On : 05 Jan 2022 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 04:15:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

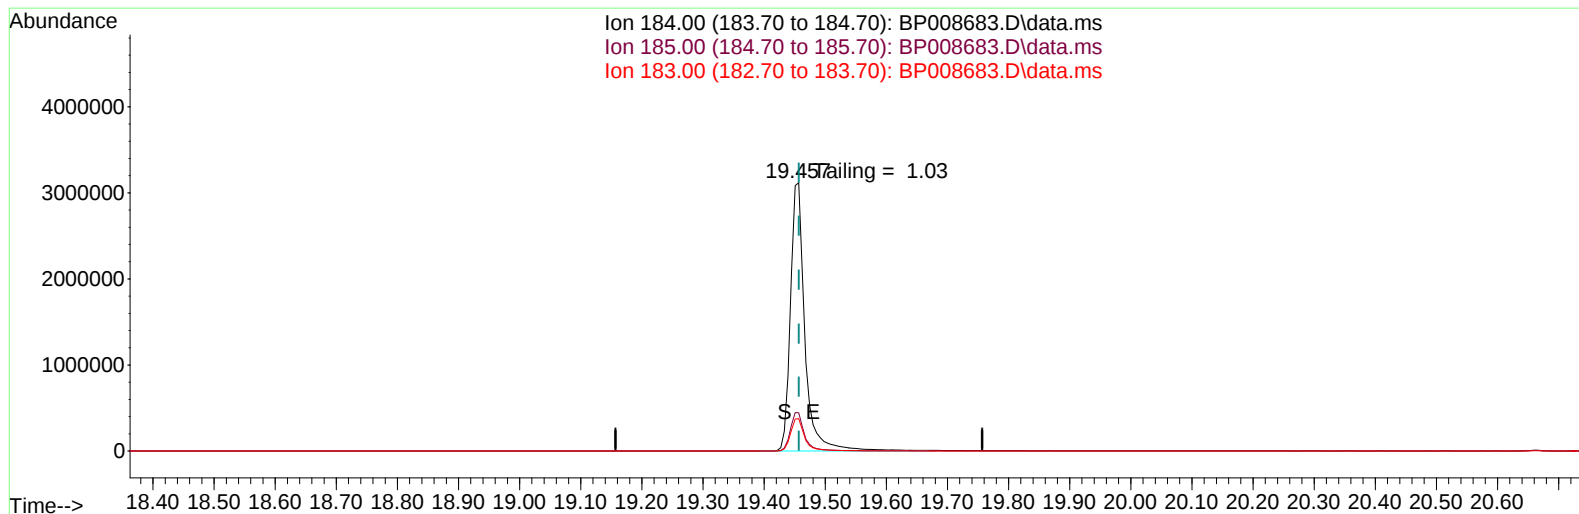




TIC: BP008683.D\data.ms

(77) Benzidine**19.457min (-0.000) 435361.78 ng****response 5179592**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.24
183.00	11.90	12.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
Data File : BP008683.D
Acq On : 05 Jan 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 04:15:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

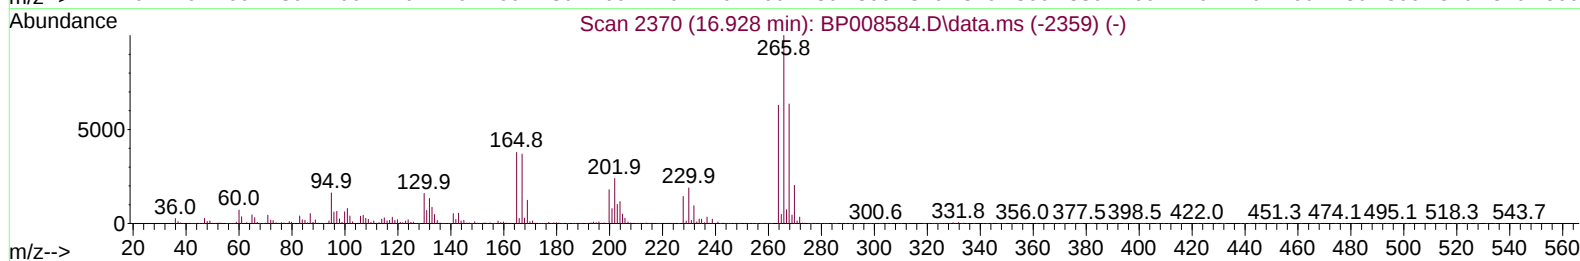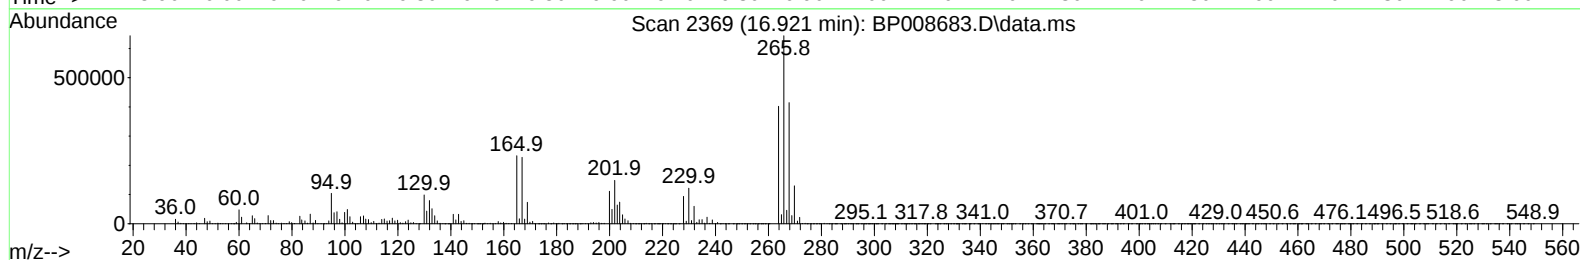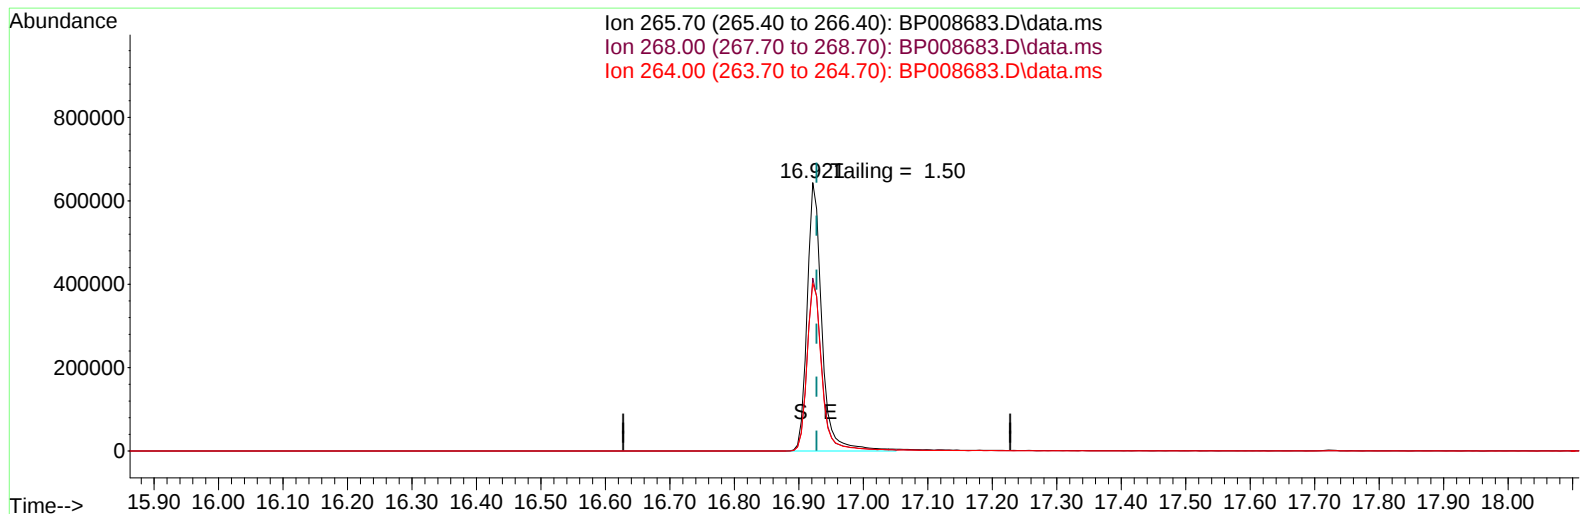

TIC: BP008683.D\data.ms

(70) Pentachlorophenol (C)

16.921min (-0.006) 622579.65 ng

response 1033905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.39
264.00	62.90	62.46
0.00	0.00	0.00