

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
 Data File : BP008699.D
 Acq On : 05 Jan 2022 20:16
 Operator : CG/JU
 Sample : M5342-05 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-8-(0-2)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	415	421	429	rBV	1175545	1781803	3.87%	1.892%
2	7.057	684	692	707	rBV	935780	1651426	3.58%	1.753%
3	7.881	825	832	841	rBV	2383774	3847984	8.35%	4.085%
4	9.040	1019	1029	1038	rBV	690531	1188641	2.58%	1.262%
5	10.687	1298	1309	1323	rBV	2702130	4728415	10.26%	5.020%
6	13.145	1719	1727	1741	rBV	1495717	2556532	5.55%	2.714%
7	14.516	1953	1960	1982	rBV	3022957	5292427	11.48%	5.619%
8	16.004	2207	2213	2223	rBV	948655	1543827	3.35%	1.639%
9	17.269	2421	2428	2434	rBV	3973407	6194012	13.44%	6.576%
10	19.274	2765	2769	2777	rBV	341091	488801	1.06%	0.519%
11	19.822	2858	2862	2869	rBV	2779389	3389002	7.35%	3.598%
12	21.351	3117	3122	3127	rBV	5569350	7474792	16.22%	7.936%
13	21.474	3137	3143	3167	rBV	28242141	46084620	100.00%	48.929%
14	23.774	3529	3534	3543	rVB2	4003958	7964785	17.28%	8.456%




Sum of corrected areas: 94187067

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
Data File : BP008699.D
Acq On : 05 Jan 2022 20:16
Operator : CG/JU
Sample : M5342-05 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-8-(0-2)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

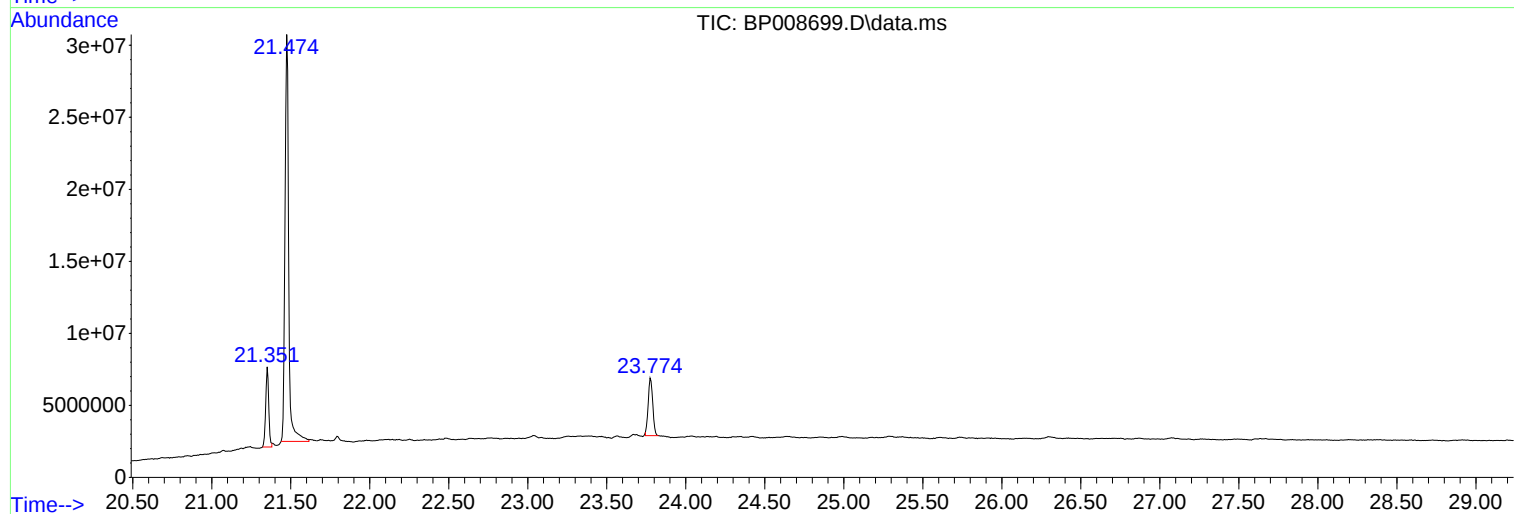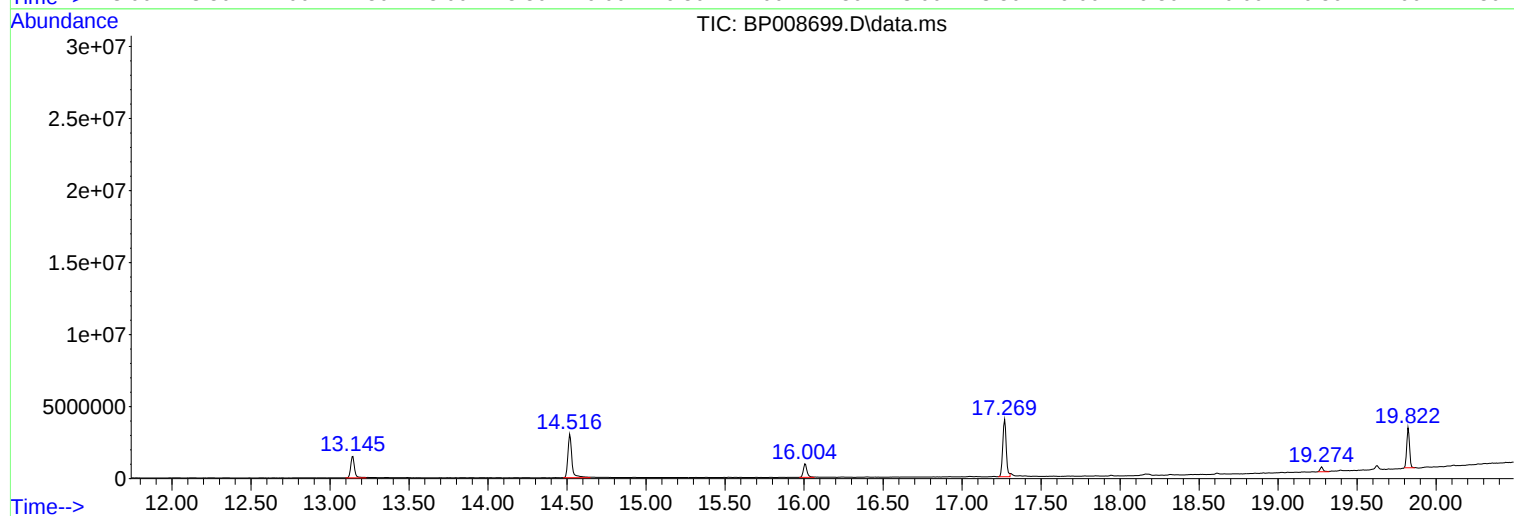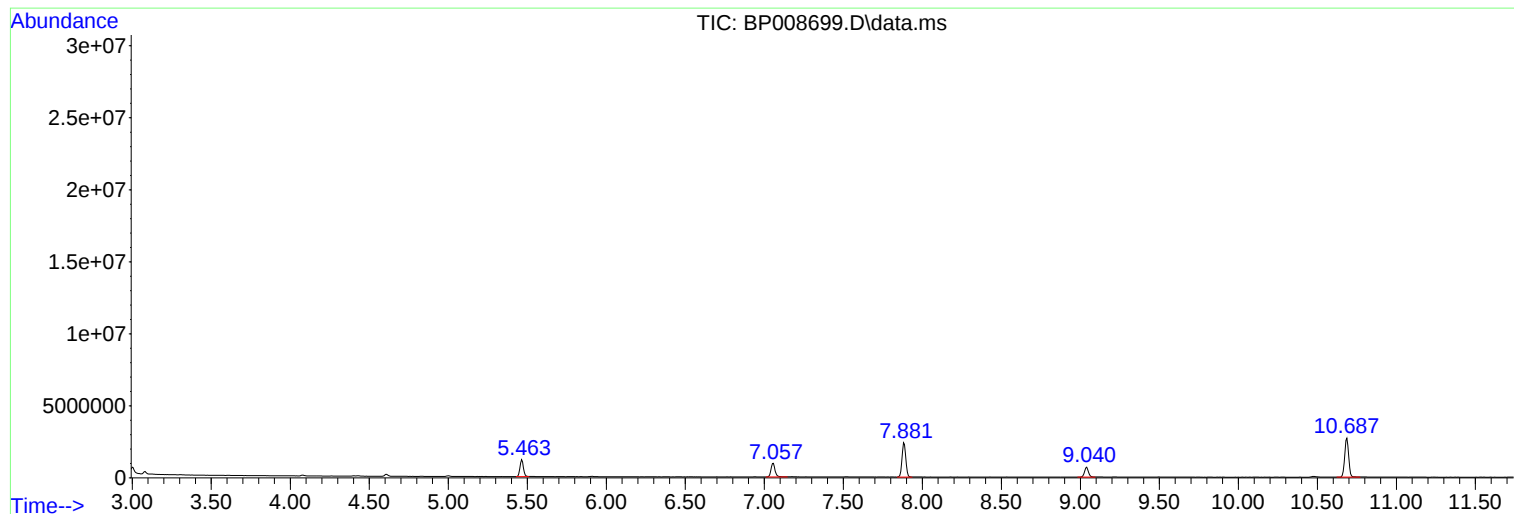

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
Data File : BP008699.D
Acq On : 05 Jan 2022 20:16
Operator : CG/JU
Sample : M5342-05 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-8-(0-2)










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.474	123.31 ng	46084600	Chrysene-d12	21.351

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	80
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	40
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	17
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	9

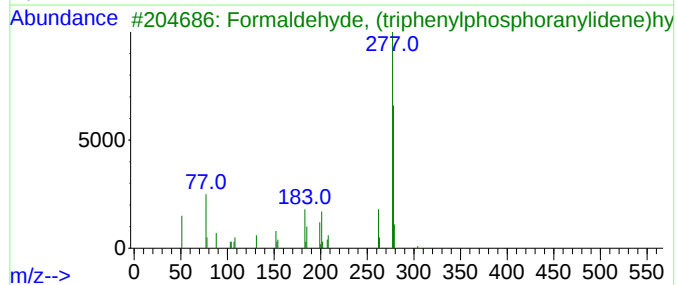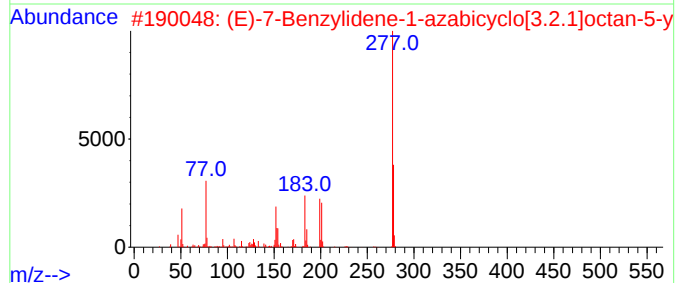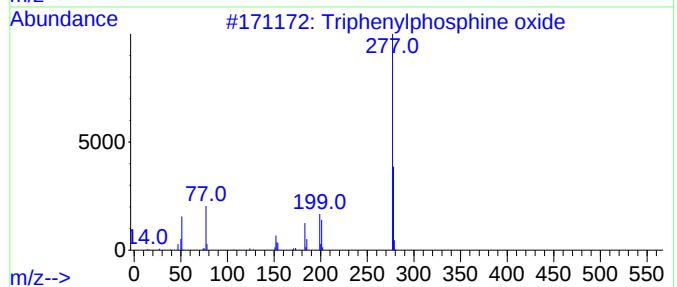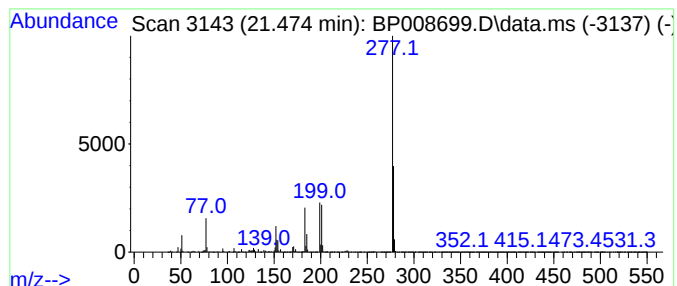

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
Data File : BP008699.D
Acq On : 05 Jan 2022 20:16
Operator : CG/JU
Sample : M5342-05 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-8-(0-2)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.474	123.3	ng	46084600	5	21.351	7474790	20.0