
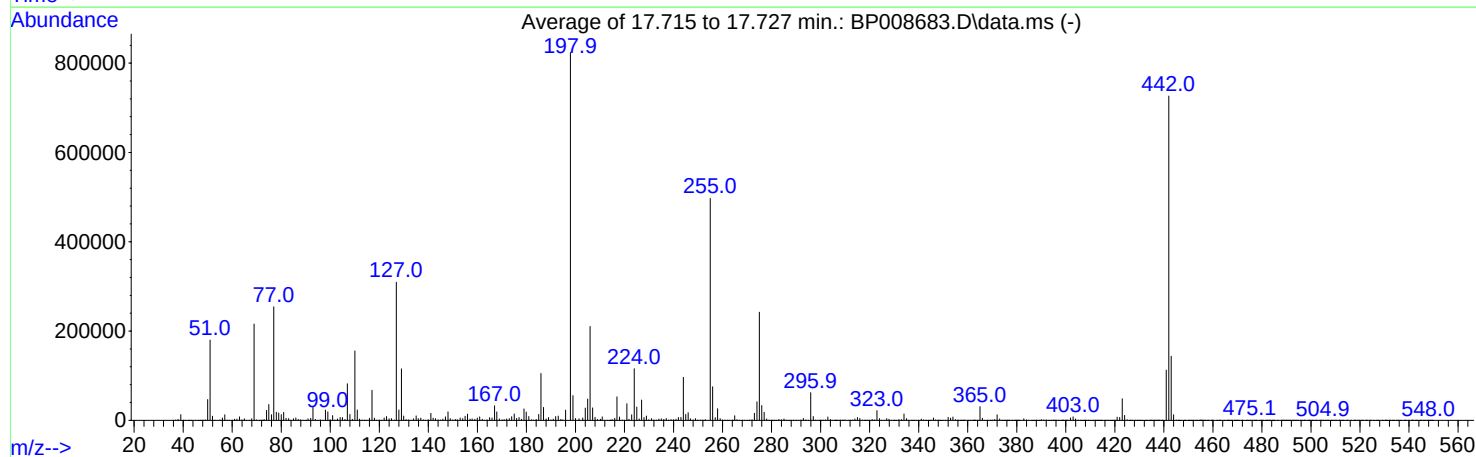


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
 Data File : BP008683.D
 Acq On : 05 Jan 2022 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 08:44:33 2021

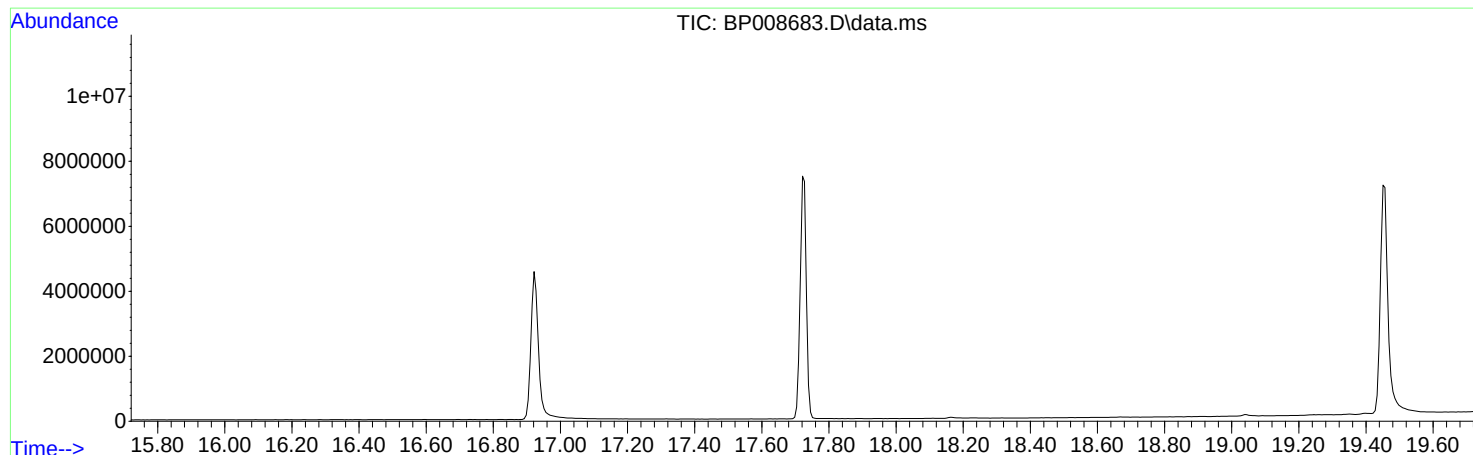




AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	179927	PASS
68	69	0.00	2	1.7	3600	PASS
69	198	0.00	100	26.2	215587	PASS
70	69	0.00	2	0.5	1054	PASS
127	198	10	80	37.6	309374	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	823813	PASS
199	198	5	9	6.8	55634	PASS
275	198	10	60	29.4	242376	PASS
365	198	1	100	3.7	30814	PASS
441	198	0.01	100	13.6	112403	PASS
442	442	100	100	100.0	726507	PASS
443	442	15	24	19.8	143883	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
Data File : BP008683.D
Acq On : 05 Jan 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 06 04:15:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 08:44:33 2021
Response via : Initial Calibration

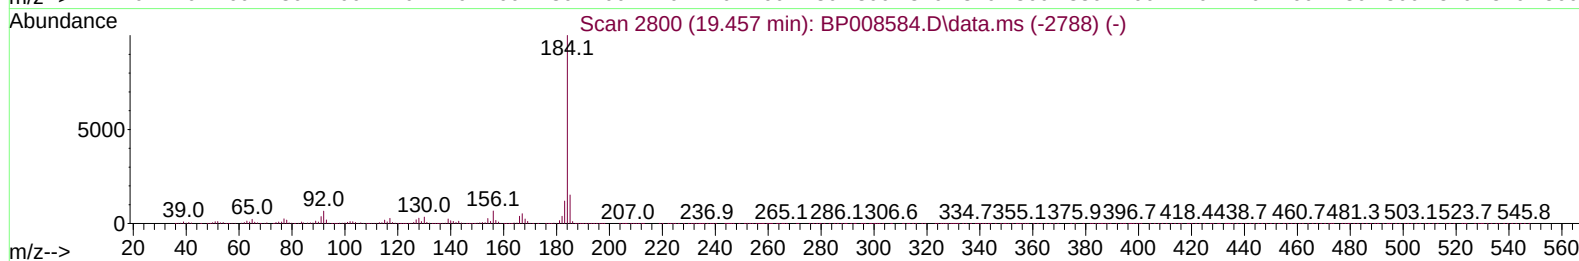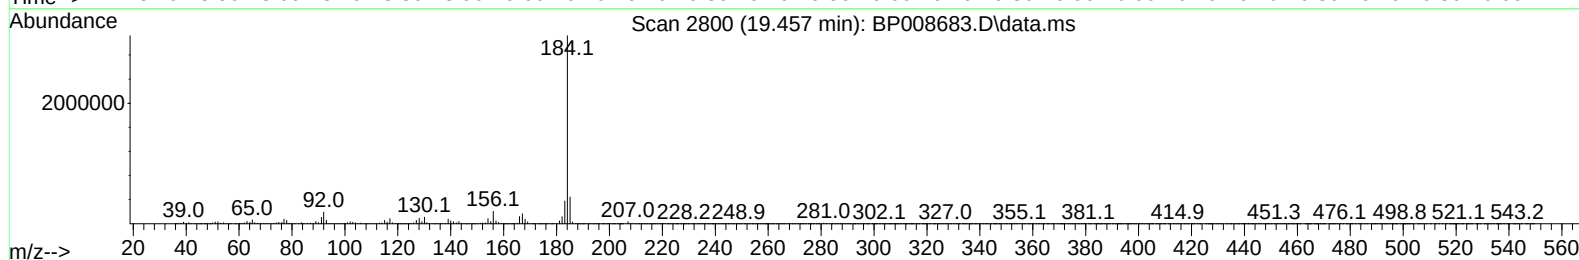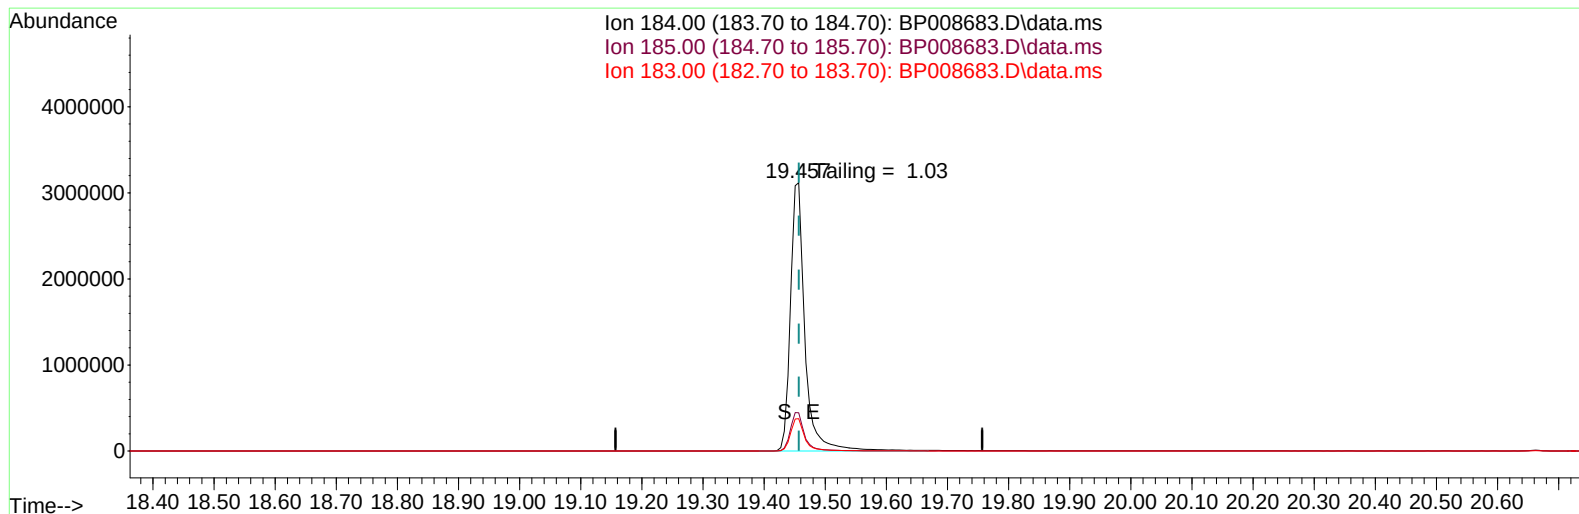

TIC: BP008683.D\data.ms

(77) Benzidine

19.457min (-0.000) 435361.78 ng


response 5179592

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.24
183.00	11.90	12.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010522\
 Data File : BP008683.D
 Acq On : 05 Jan 2022 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 06 04:15:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP122821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 08:44:33 2021
 Response via : Initial Calibration

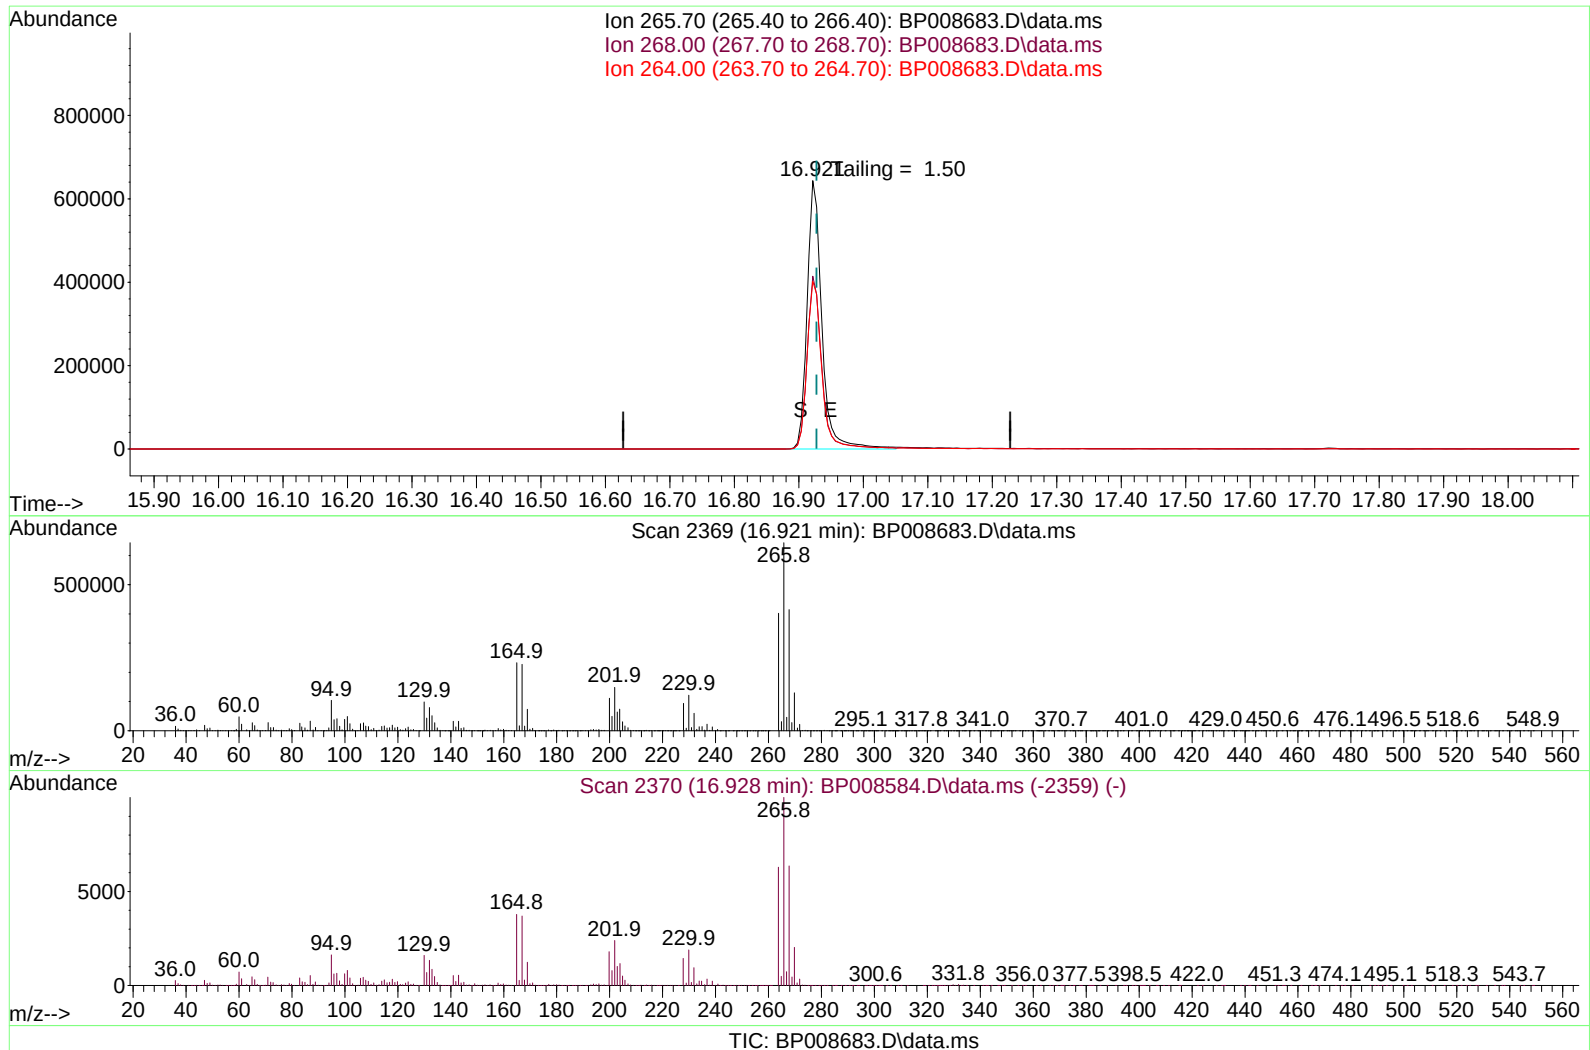

TIC: BP008683.D\data.ms

(70) Pentachlorophenol (C)

16.921min (-0.006) 622579.65 ng

response 1033905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.39
264.00	62.90	62.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/5/2022	BNA_P	<u>BP008683.D</u>
Compound Name	Response	Retention Time
DDT	2939012	20.662
DDD	84681	20.233
DDE	4381	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
89062	3028074	2.94