

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010523\
 Data File : BP013394.D
 Acq On : 05 Jan 2023 13:09
 Operator : CG/JU
 Sample : SST00517
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST005645

Quant Time: Jan 06 00:20:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 06 00:16:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	307045	20.000	ng/u1	0.00
20) Naphthalene-d8	10.734	136	1162480	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.569	164	706665	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	1592600	20.000	ng/u1	0.00
79) Chrysene-d12	21.416	240	1653036	20.000	ng/u1	0.00
88) Perylene-d12	23.880	264	1871568	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	15482	2.156	ng/uL	0.00
4) Pyridine-d5	3.752	84	94166	4.616	ng/u1	0.01
7) Phenol-d5	7.081	99	101293	4.050	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.252	67	72136	4.781	ng/u1	0.00
11) 2-Chlorophenol-d4	7.452	132	82613	4.196	ng/u1	0.00
15) 4-Methylphenol-d8	8.634	113	74589	3.640	ng/u1	0.00
21) Nitrobenzene-d5	9.093	128	33315	3.901	ng/u1	0.00
24) 2-Nitrophenol-d4	9.816	143	34195	3.556	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	74092	3.967	ng/u1	0.00
31) 4-Chloroaniline-d4	10.881	131	102750	3.897	ng/u1	0.00
46) Dimethylphthalate-d6	13.975	166	235914	4.344	ng/u1	0.00
49) Acenaphthylene-d8	14.263	160	238745	4.001	ng/u1	0.00
54) 4-Nitrophenol-d4	14.775	143	24952	2.554	ng/u1	0.00
60) Fluorene-d10	15.563	176	212158	4.617	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	25501	2.488	ng/u1	0.00
73) Anthracene-d10	17.428	188	317668	4.421	ng/u1	0.00
81) Pyrene-d10	19.663	212	396961	4.184	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	1567586	16.804	ng/u1	0.17
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	18020	2.404	ng/uL#	84
5) Pyridine	3.770	79	95328	4.702	ng/u1	89
6) Benzaldehyde	7.063	77	44007	4.494	ng/u1	95
8) Phenol	7.111	94	109685	4.338	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.346	93	96052	4.628	ng/u1	99
12) 2-Chlorophenol	7.481	128	88400	4.379	ng/u1	97
13) 2-Methylphenol	8.369	108	74198	3.764	ng/u1	93
14) 2,2'-oxybis(1-Chloropr...	8.452	45	151506	5.320	ng/u1	97
16) Acetophenone	8.752	105	133104	4.236	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.734	70	64528	4.084	ng/u1	97
18) 4-Methylphenol	8.699	108	83464	3.822	ng/u1	100
19) Hexachloroethane	9.005	117	37590	4.659	ng/u1	91
22) Nitrobenzene	9.134	77	93318	4.656	ng/u1	97
23) Isophorone	9.663	82	163320	4.030	ng/u1	96
25) 2-Nitrophenol	9.852	139	36891	3.541	ng/u1	96
26) 2,4-Dimethylphenol	9.904	107	91167	4.485	ng/u1	96
27) Bis(2-Chloroethoxy)met...	10.140	93	115542	4.459	ng/u1	99
29) 2,4-Dichlorophenol	10.381	162	76989	4.208	ng/u1	97
30) Naphthalene	10.787	128	296378	4.875	ng/u1	100
32) 4-Chloroaniline	10.899	127	104520	4.006	ng/u1	98
33) Hexachlorobutadiene	11.063	225	64559	5.139	ng/u1	95
34) Caprolactam	11.687	113	17413	2.791	ng/u1	89
35) 4-Chloro-3-methylphenol	12.022	107	71441	3.826	ng/u1	99
36) 2-Methylnaphthalene	12.393	142	180881	4.337	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010523\
 Data File : BP013394.D
 Acq On : 05 Jan 2023 13:09
 Operator : CG/JU
 Sample : SST00517
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST005645

Quant Time: Jan 06 00:20:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 06 00:16:51 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.610	142	194009	4.523	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.757	216	114900	5.050	ng/ul	98
40) Hexachlorocyclopentadiene	12.734	237	49423	3.338	ng/ul	98
41) 2,4,6-Trichlorophenol	12.998	196	57186	3.910	ng/ul	99
42) 2,4,5-Trichlorophenol	13.075	196	64926	4.133	ng/ul	97
43) 1,1'-Biphenyl	13.404	154	257151	4.845	ng/ul	99
44) 2-Chloronaphthalene	13.445	162	206201	4.936	ng/ul	98
45) 2-Nitroaniline	13.657	65	35753	3.530	ng/ul	99
47) Dimethylphthalate	14.022	163	237680	4.415	ng/ul	98
48) 2,6-Dinitrotoluene	14.145	165	30944	3.093	ng/ul#	91
50) Acenaphthylene	14.292	152	272477	4.247	ng/ul	100
51) 3-Nitroaniline	14.475	138	25131	2.660	ng/ul	93
52) Acenaphthene	14.634	153	216138	4.861	ng/ul	98
53) 2,4-Dinitrophenol	14.692	184	15295	2.237	ng/ul#	90
55) 4-Nitrophenol	14.787	109	19295	2.895	ng/ul	95
56) Dibenzofuran	14.969	168	308551	4.881	ng/ul	99
57) 2,4-Dinitrotoluene	14.940	165	44246	3.045	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.192	232	55930	3.902	ng/ul	97
59) Diethylphthalate	15.387	149	222564	4.253	ng/ul	99
61) Fluorene	15.616	166	245041	4.833	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.610	204	130068	4.852	ng/ul	98
63) 4-Nitroaniline	15.639	138	20062	2.414	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.698	198	27323	2.728	ng/ul#	83
67) N-Nitrosodiphenylamine	15.828	169	194266	4.400	ng/ul	98
68) 4-Bromophenyl-phenylether	16.510	248	76095	4.400	ng/ul	98
69) Hexachlorobenzene	16.628	284	94586	4.606	ng/ul	98
70) Atrazine	16.781	200	62626	3.640	ng/ul	94
71) Pentachlorophenol	16.975	266	37932	3.050	ng/ul	97
72) Phenanthrene	17.369	178	405643	4.890	ng/ul	99
74) Anthracene	17.463	178	385891	4.659	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.369	216	113604	5.000	ng/uL	99
76) Pentachlorobenzene	14.887	250	112609	4.861	ng/uL	98
77) Carbazole	17.733	167	308800	4.427	ng/ul	100
78) Di-n-butylphthalate	18.275	149	289984	3.414	ng/ul	99
80) Fluoranthene	19.333	202	460248	4.274	ng/ul	98
82) Pyrene	19.686	202	506343	4.558	ng/ul	98
83) Butylbenzylphthalate	20.551	149	124103	2.892	ng/ul	94
84) 3,3'-Dichlorobenzidine	21.333	252	115504	3.093	ng/ul#	97
85) Benzo(a)anthracene	21.398	228	510437	4.651	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.310	149	191972	3.171	ng/ul#	99
87) Chrysene	21.451	228	509918	4.914	ng/ul	98
89) Di-n-octyl phthalate	22.257	149	293770	2.802	ng/ul	100
90) Benzo(b)fluoranthene	23.127	252	545716	4.573	ng/ul	98
91) Benzo(k)fluoranthene	23.174	252	512647	4.332	ng/ul	99
93) Benzo(a)pyrene	23.768	252	465017	4.475	ng/ul	95
94) Indeno(1,2,3-cd)pyrene	26.451	276	653013	5.045	ng/ul	99
95) Dibenzo(a,h)anthracene	26.468	278	548041	5.114	ng/ul	97
96) Benzo(g,h,i)perylene	27.245	276	539702	5.194	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010523\
 Data File : BP013394.D
 Acq On : 05 Jan 2023 13:09
 Operator : CG/JU
 Sample : SSTD00517
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005645

Quant Time: Jan 06 00:20:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 06 00:16:51 2023
 Response via : Initial Calibration




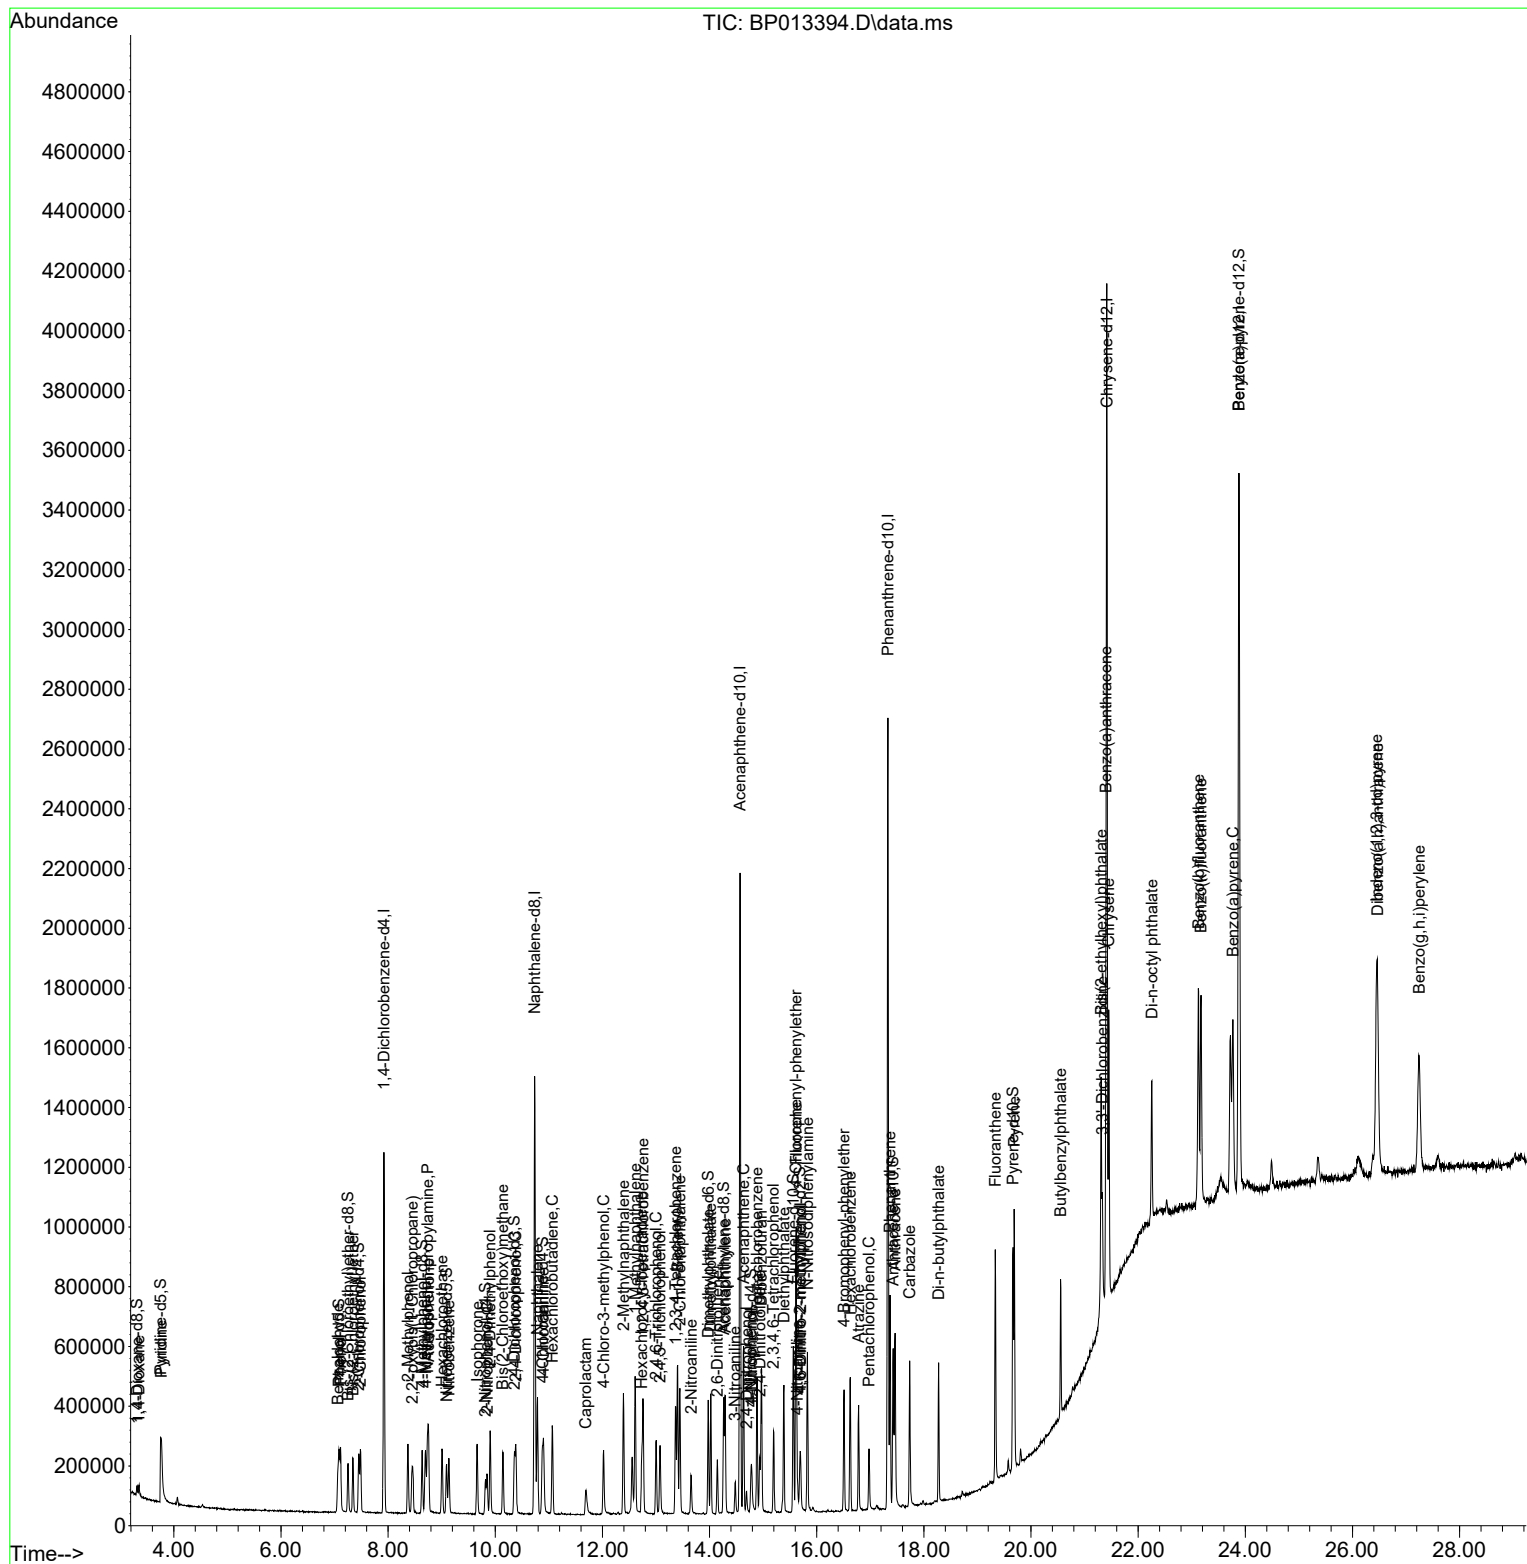


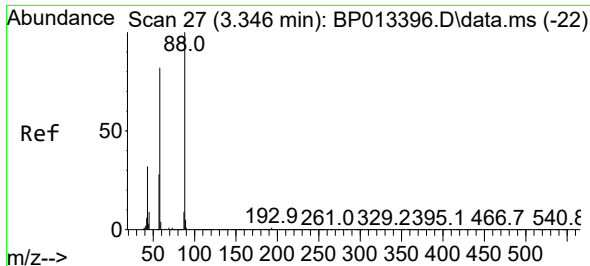

#2
1,4-Dioxane
Concen: 2.404 ng/uL
RT: 3.352 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion: 88 Resp: 18020
Ion Ratio Lower Upper
88 100
43 34.1 26.6 40.0
58 61.7 64.7 97.1#

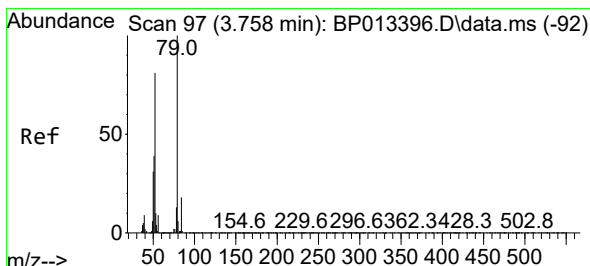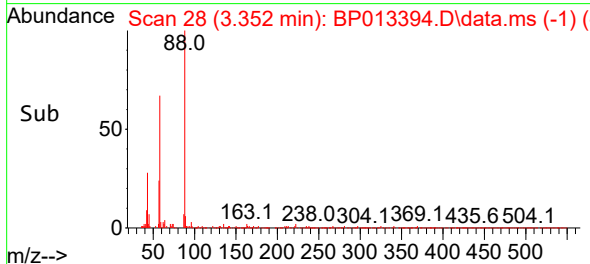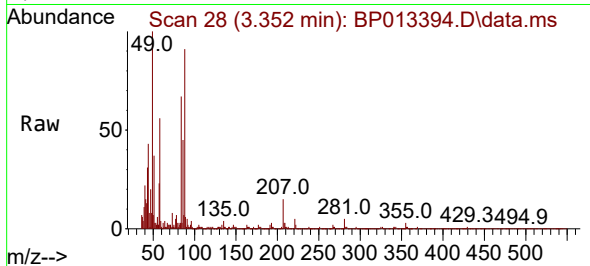

#5
Pyridine
Concen: 4.702 ng/uL
RT: 3.770 min Scan# 99
Delta R.T. 0.012 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion: 79 Resp: 95328
Ion Ratio Lower Upper
79 100
52 93.4 67.7 101.5
51 48.2 32.3 48.5


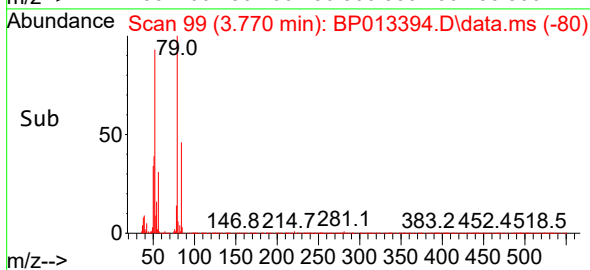

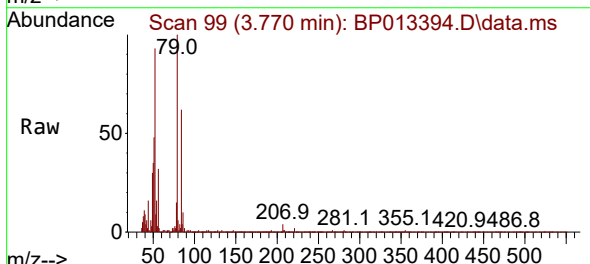




#6
Benzaldehyde
Concen: 4.494 ng/ul
RT: 7.063 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion: 77 Resp: 44007
Ion Ratio Lower Upper
77 100
105 101.3 75.4 113.0
106 90.1 69.8 104.8

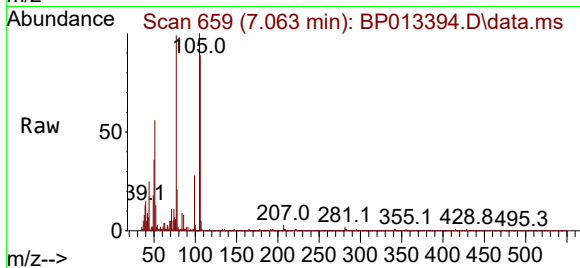

#8
Phenol
Concen: 4.338 ng/ul
RT: 7.111 min Scan# 667
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion: 94 Resp: 109685
Ion Ratio Lower Upper
94 100
65 29.5 22.8 34.2
66 37.9 28.6 42.8


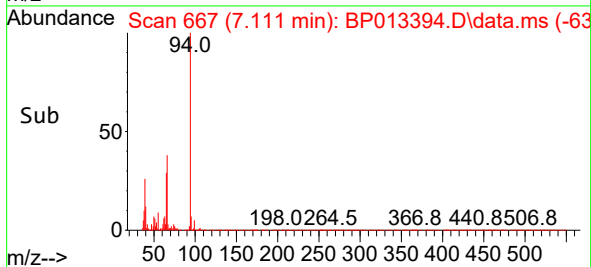

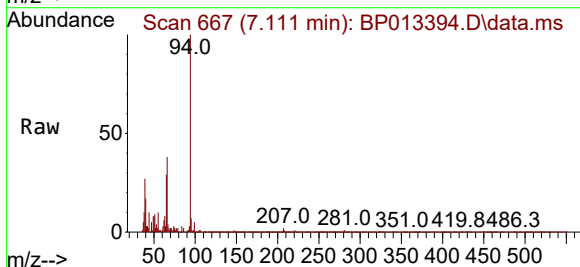




#10
Bis(2-Chloroethyl)ether
Concen: 4.628 ng/ul
RT: 7.346 min Scan# 706
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion: 93 Resp: 96052
Ion Ratio Lower Upper
93 100
63 79.9 64.7 97.1
95 32.7 25.7 38.5



#12
2-Chlorophenol
Concen: 4.379 ng/ul
RT: 7.481 min Scan# 730
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:128 Resp: 88400
Ion Ratio Lower Upper
128 100
64 49.6 41.4 62.2
130 32.7 24.9 37.3









#13
2-Methylphenol
Concen: 3.764 ng/ul
RT: 8.369 min Scan# 880
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:108 Resp: 74198
Ion Ratio Lower Upper
108 100
107 92.9 69.4 104.0



#14
2,2'-oxybis(1-Chloropropane)
Concen: 5.320 ng/ul
RT: 8.452 min Scan# 895
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion: 45 Resp: 151506
Ion Ratio Lower Upper
45 100
77 13.5 10.1 15.1
79 10.0 7.0 10.4









#16
Acetophenone
Concen: 4.236 ng/ul
RT: 8.752 min Scan# 946
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:105 Resp: 133104
Ion Ratio Lower Upper
105 100
77 80.9 62.5 93.7
51 32.4 24.7 37.1



#17
N-Nitroso-di-n-propylamine
Concen: 4.084 ng/ul
RT: 8.734 min Scan# 943
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion: 70 Resp: 64528
Ion Ratio Lower Upper
70 100
42 69.6 53.6 80.4
101 9.2 8.0 12.0
130 19.2 15.9 23.9









#18
4-Methylphenol
Concen: 3.822 ng/ul
RT: 8.699 min Scan# 911
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:108 Resp: 83464
Ion Ratio Lower Upper
108 100
107 112.3 89.5 134.3



#19
Hexachloroethane
Concen: 4.659 ng/ul
RT: 9.005 min Scan# 989
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:117 Resp: 37590
Ion Ratio Lower Upper
117 100
201 103.6 90.6 136.0
199 65.0 58.7 88.1









#22
Nitrobenzene
Concen: 4.656 ng/ul
RT: 9.134 min Scan# 1101
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion: 77 Resp: 93318
Ion Ratio Lower Upper
77 100
123 40.1 33.7 50.5
65 15.0 11.0 16.4



#23
Isophorone
Concen: 4.030 ng/ul
RT: 9.663 min Scan# 1101
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion: 82 Resp: 163320
Ion Ratio Lower Upper
82 100
95 6.5 5.4 8.0
138 19.7 13.8 20.6









#25
2-Nitrophenol
Concen: 3.541 ng/ul
RT: 9.852 min Scan# 1132
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:139 Resp: 36891
Ion Ratio Lower Upper
139 100
65 57.4 43.0 64.6
109 28.2 23.4 35.2



#26
2,4-Dimethylphenol
Concen: 4.485 ng/ul
RT: 9.904 min Scan# 1142
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:107 Resp: 91167
Ion Ratio Lower Upper
107 100
121 56.6 39.9 59.9
122 85.4 68.3 102.5

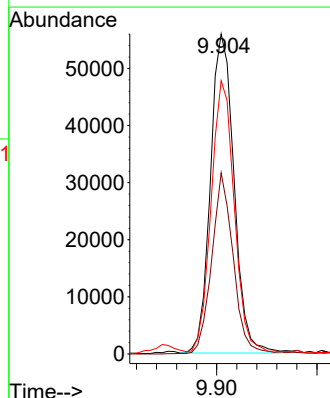



#27

Bis(2-Chloroethoxy)methane

Concen: 4.459 ng/ul

RT: 10.140 min Scan# 1182

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion: 93 Resp: 115542

Ion Ratio Lower Upper

93 100

95 32.5 25.3 37.9

123 10.9 8.4 12.6



#29

2,4-Dichlorophenol

Concen: 4.208 ng/ul

RT: 10.381 min Scan# 1223

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:162 Resp: 76989


Ion Ratio Lower Upper

162 100

164 62.0 51.9 77.9

98 32.9 27.1 40.7

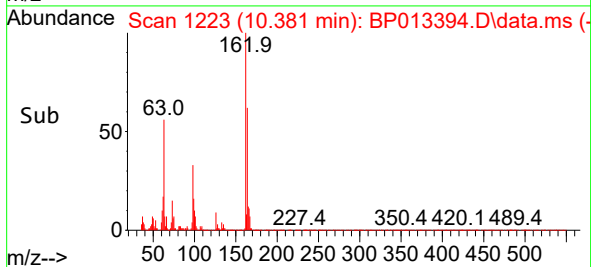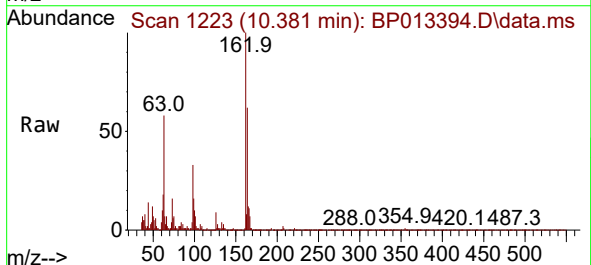



#30

Naphthalene

Concen: 4.875 ng/ul

RT: 10.787 min Scan# 1291

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:128 Resp: 296378

Ion Ratio Lower Upper

128 100

129 10.9 8.7 13.1

127 12.9 10.1 15.1

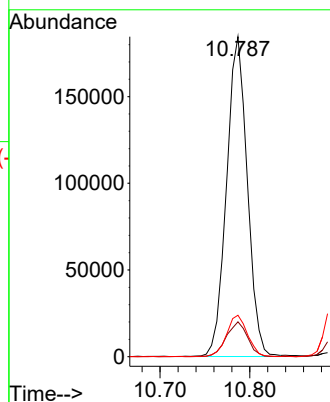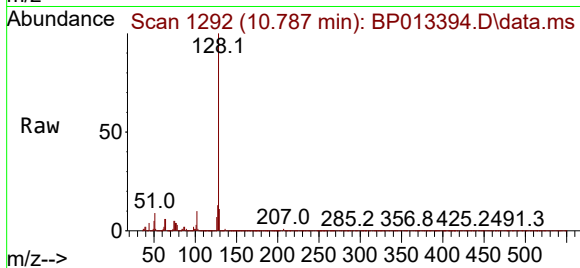

#32

4-Chloroaniline

Concen: 4.006 ng/ul

RT: 10.899 min Scan# 1311

Delta R.T. -0.000 min

Lab File: BP013394.D




Acq: 05 Jan 2023 13:09


Tgt Ion:127 Resp: 104520

Ion Ratio Lower Upper

127 100

129 31.3 26.1 39.1









#33
Hexachlorobutadiene
Concen: 5.139 ng/ul
RT: 11.063 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:225 Resp: 64559
Ion Ratio Lower Upper
225 100
223 68.2 48.8 73.2
227 63.4 50.6 76.0



#34
Caprolactam
Concen: 2.791 ng/ul
RT: 11.687 min Scan# 1445
Delta R.T. -0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:113 Resp: 17413
Ion Ratio Lower Upper
113 100
55 172.9 156.4 234.6
56 138.8 117.1 175.7




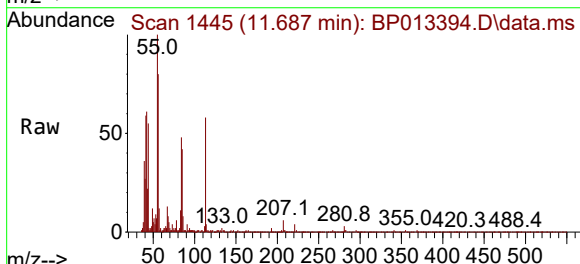




#35
4-Chloro-3-methylphenol
Concen: 3.826 ng/ul
RT: 12.022 min Scan# 1501
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:107 Resp: 71441
Ion Ratio Lower Upper
107 100
144 26.5 21.0 31.6
142 80.2 64.8 97.2

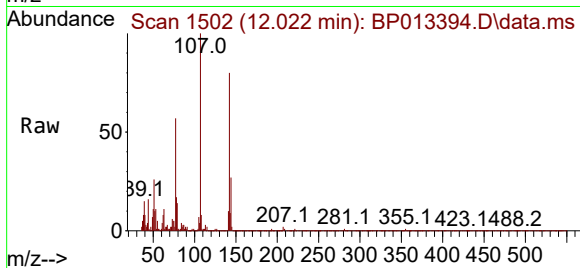

#36
2-Methylnaphthalene
Concen: 4.337 ng/ul
RT: 12.393 min Scan# 1565
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:142 Resp: 180881
Ion Ratio Lower Upper
142 100
141 88.7 69.7 104.5







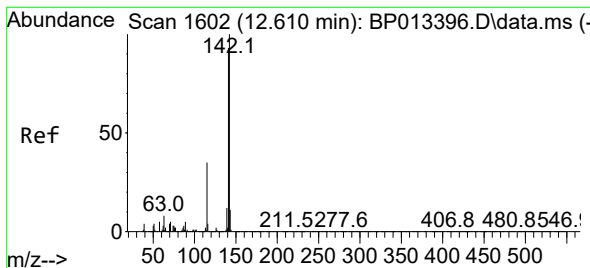

#37
1-Methylnaphthalene
Concen: 4.523 ng/ul
RT: 12.610 min Scan# 1602
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:142 Resp: 194009
Ion Ratio Lower Upper
142 100
141 90.7 74.2 111.4
116 4.1 3.0 4.4

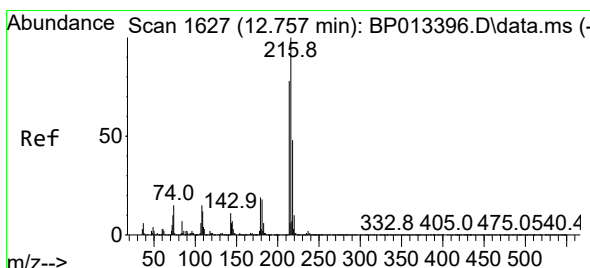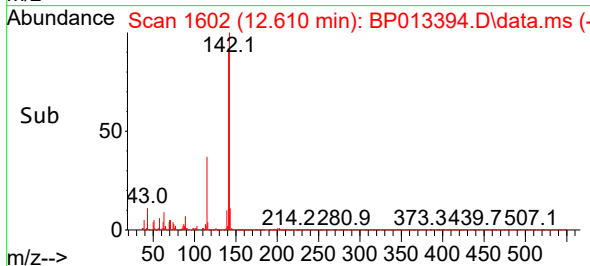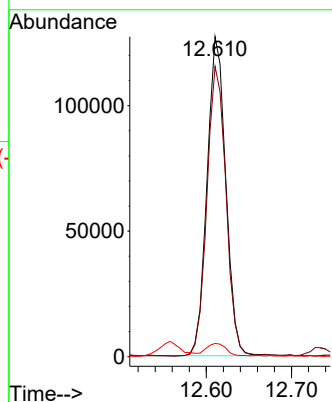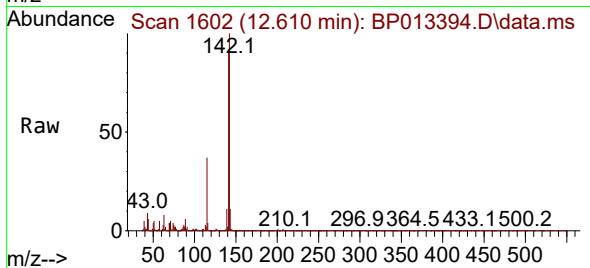

#39
1,2,4,5-Tetrachlorobenzene
Concen: 5.050 ng/ul
RT: 12.757 min Scan# 1627
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:216 Resp: 114900
Ion Ratio Lower Upper
216 100
214 80.6 62.8 94.2
179 19.1 15.1 22.7
108 15.9 12.2 18.2

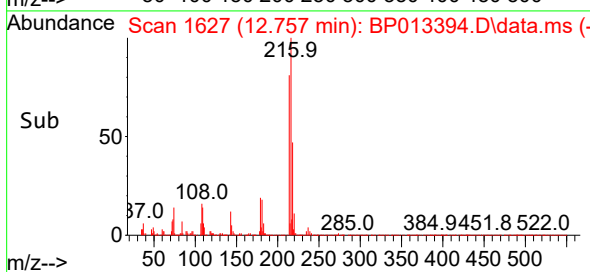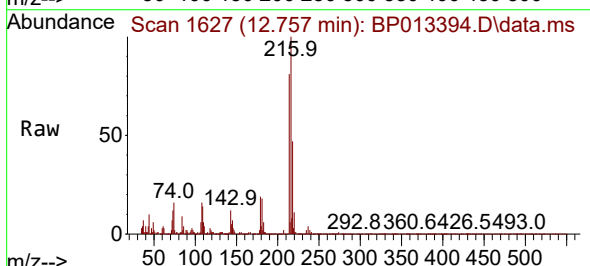



#40

Hexachlorocyclopentadiene

Concen: 3.338 ng/ul

RT: 12.734 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:237 Resp: 49423

Ion Ratio Lower Upper

237 100

235 64.3 50.8 76.2

272 12.5 11.5 17.3

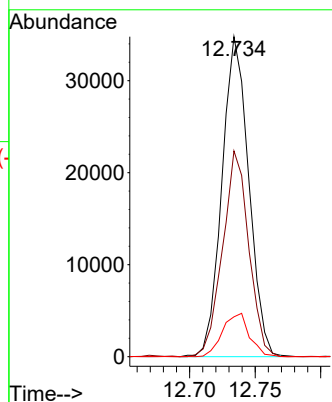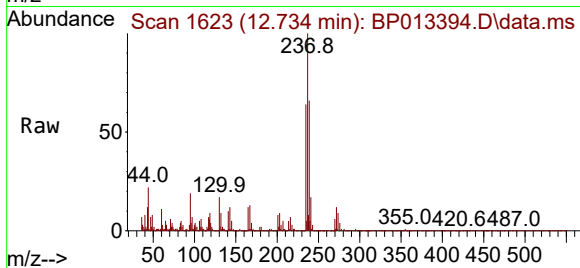

#41

2,4,6-Trichlorophenol

Concen: 3.910 ng/ul

RT: 12.998 min Scan# 1668

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:196 Resp: 57186


Ion Ratio Lower Upper

196 100

198 96.9 77.9 116.9

200 30.0 25.6 38.4





#42

2,4,5-Trichlorophenol

Concen: 4.133 ng/ul

RT: 13.075 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:196 Resp: 64926

Ion Ratio Lower Upper

196 100

198 92.2 76.0 114.0

200 31.4 24.4 36.6



#43

1,1'-Biphenyl

Concen: 4.845 ng/ul

RT: 13.404 min Scan# 1737

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:154 Resp: 257151


Ion Ratio Lower Upper

154 100

153 39.9 31.9 47.9

76 11.3 10.3 15.5





#44

2-Chloronaphthalene

Concen: 4.936 ng/ul

RT: 13.445 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:162 Resp: 206201

Ion Ratio Lower Upper

162 100

164 33.9 26.4 39.6

127 36.9 28.9 43.3



#45

2-Nitroaniline

Concen: 3.530 ng/ul

RT: 13.657 min Scan# 1780

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion: 65 Resp: 35753


Ion Ratio Lower Upper

65 100

92 65.6 53.5 80.3

138 99.7 79.4 119.0









#47
Dimethylphthalate
Concen: 4.415 ng/ul
RT: 14.022 min Scan# 1842
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:163 Resp: 237680
Ion Ratio Lower Upper
163 100
194 4.3 3.4 5.2
164 10.7 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 3.093 ng/ul
RT: 14.145 min Scan# 1863
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:165 Resp: 30944
Ion Ratio Lower Upper
165 100
89 65.3 47.1 70.7
121 26.6 17.3 25.9









#50
Acenaphthylene
Concen: 4.247 ng/ul
RT: 14.292 min Scan# 1888
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:152 Resp: 272477
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.8
153 12.9 10.3 15.5



#51
3-Nitroaniline
Concen: 2.660 ng/ul
RT: 14.475 min Scan# 1919
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:138 Resp: 25131
Ion Ratio Lower Upper
138 100
108 12.2 8.6 12.8
92 111.1 95.0 142.4




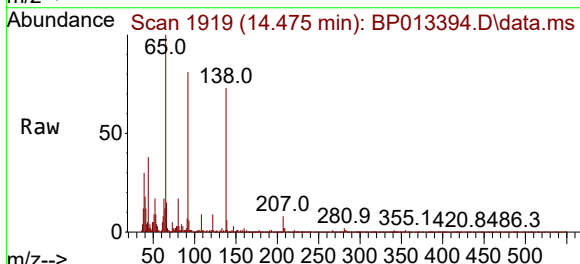




#52
Acenaphthene
Concen: 4.861 ng/ul
RT: 14.634 min Scan# 1946
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:153 Resp: 216138
Ion Ratio Lower Upper
153 100
152 49.2 38.4 57.6
154 86.2 70.6 106.0



#53
2,4-Dinitrophenol
Concen: 2.237 ng/ul
RT: 14.692 min Scan# 1956
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:184 Resp: 15295
Ion Ratio Lower Upper
184 100
63 82.5 54.3 81.5#
154 62.6 49.1 73.7



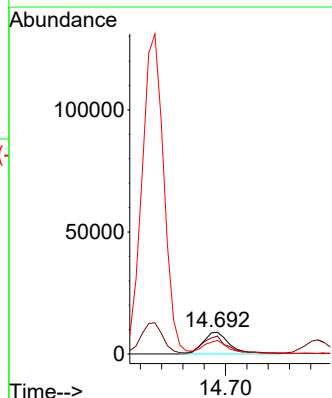
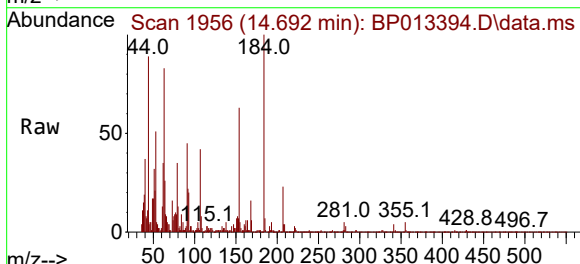




#55
4-Nitrophenol
Concen: 2.895 ng/ul
RT: 14.787 min Scan# 1971
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:109 Resp: 19295
Ion Ratio Lower Upper
109 100
139 129.5 109.2 163.8
65 150.2 116.6 174.8



#56
Dibenzofuran
Concen: 4.881 ng/ul
RT: 14.969 min Scan# 2003
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:168 Resp: 308551
Ion Ratio Lower Upper
168 100
139 34.0 27.4 41.2

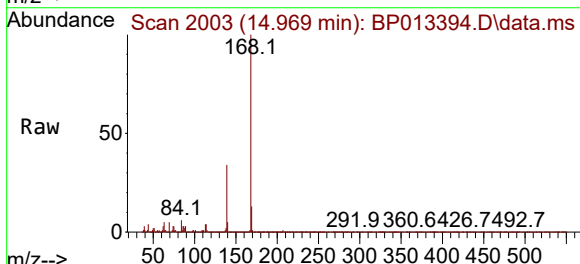



#57

2,4-Dinitrotoluene

Concen: 3.045 ng/ul

RT: 14.940 min Scan# 1997

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:165 Resp: 44246

Ion Ratio Lower Upper

165 100

63 52.3 37.3 55.9

182 2.7 2.0 3.0



#58

2,3,4,6-Tetrachlorophenol

Concen: 3.902 ng/ul

RT: 15.192 min Scan# 2041

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Tgt Ion:232 Resp: 55930




Ion Ratio Lower Upper


232 100

131 40.7 30.7 46.1

130 2.4 1.7 2.5

166 28.5 22.1 33.1


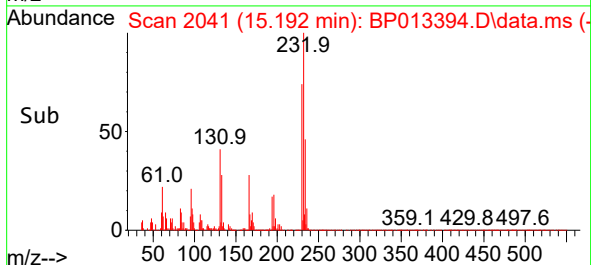
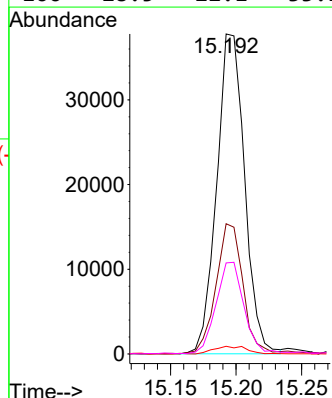
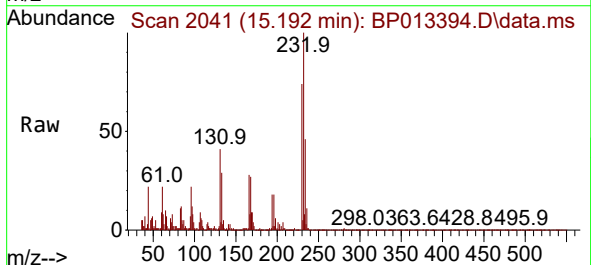




#59
Diethylphthalate
Concen: 4.253 ng/ul
RT: 15.387 min Scan# 2073
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:149 Resp: 222564
Ion Ratio Lower Upper
149 100
177 22.9 18.9 28.3
150 12.8 9.9 14.9



#61
Fluorene
Concen: 4.833 ng/ul
RT: 15.616 min Scan# 2113
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:166 Resp: 245041
Ion Ratio Lower Upper
166 100
165 95.0 78.0 117.0
167 13.2 10.8 16.2




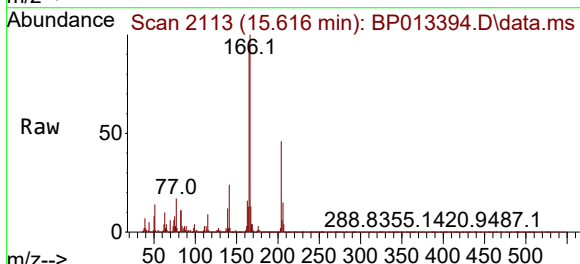




#62
4-Chlorophenyl-phenylether
Concen: 4.852 ng/ul
RT: 15.610 min Scan# 2112
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:204 Resp: 130068
Ion Ratio Lower Upper
204 100
206 32.6 26.2 39.2
141 50.8 39.3 58.9

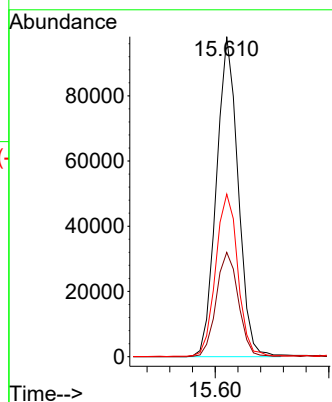

#63
4-Nitroaniline
Concen: 2.414 ng/ul
RT: 15.639 min Scan# 2117
Delta R.T. -0.000 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:138 Resp: 20062
Ion Ratio Lower Upper
138 100
92 49.5 43.1 64.7
108 74.7 63.6 95.4




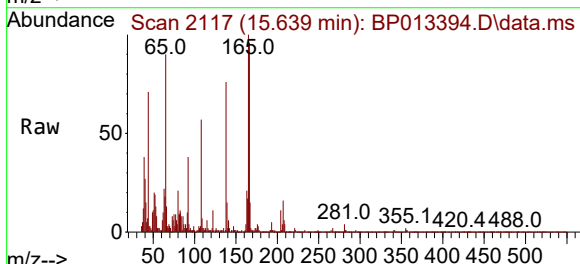




#66
 4,6-Dinitro-2-methylphenol
 Concen: 2.728 ng/ul
 RT: 15.698 min Scan# 2127
 Delta R.T. -0.000 min
 Lab File: BP013394.D
 Acq: 05 Jan 2023 13:09




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005645


Tgt Ion:198 Resp: 27323
 Ion Ratio Lower Upper
 198 100
 182 11.2 4.8 7.2#
 77 32.2 18.9 28.3#

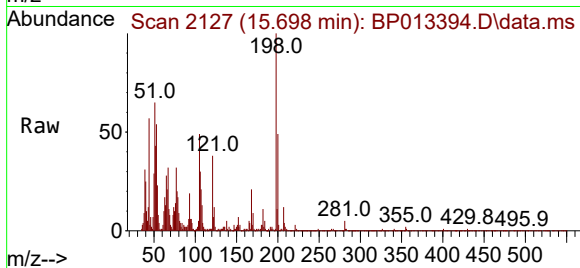

#67
 N-Nitrosodiphenylamine
 Concen: 4.400 ng/ul
 RT: 15.828 min Scan# 2149
 Delta R.T. 0.006 min
 Lab File: BP013394.D
 Acq: 05 Jan 2023 13:09

Tgt Ion:169 Resp: 194266
 Ion Ratio Lower Upper
 169 100
 168 64.6 52.9 79.3
 167 36.0 29.3 43.9









#68
4-Bromophenyl-phenylether
Concen: 4.400 ng/ul
RT: 16.510 min Scan# 2265
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09




Instrument :
BNA_P
ClientSampleId :
SSTD005645


Tgt Ion:	248	Resp:	76095
Ion Ratio	Lower	Upper	
248	100		
250	99.3	78.5	117.7
141	63.5	53.0	79.4

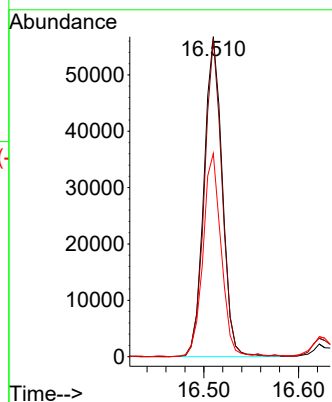

#69
Hexachlorobenzene
Concen: 4.606 ng/ul
RT: 16.628 min Scan# 2285
Delta R.T. 0.006 min
Lab File: BP013394.D
Acq: 05 Jan 2023 13:09

Tgt Ion:	284	Resp:	94586
Ion Ratio	Lower	Upper	
284	100		
142	29.1	24.8	37.2
249	29.8	24.1	36.1





#70

Atrazine

Concen: 3.640 ng/ul

RT: 16.781 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:200 Resp: 62626

Ion Ratio Lower Upper

200 100

173 27.5 19.2 28.8

215 52.3 39.0 58.4

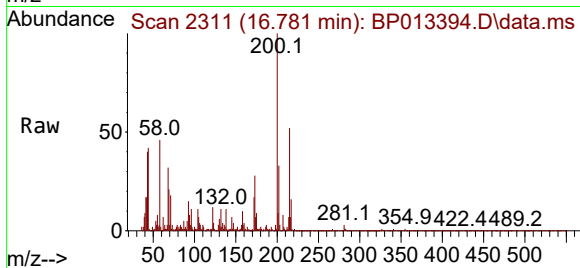

#71

Pentachlorophenol

Concen: 3.050 ng/ul

RT: 16.975 min Scan# 2344

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:266 Resp: 37932


Ion Ratio Lower Upper

266 100

264 57.0 49.7 74.5

268 61.7 49.4 74.0

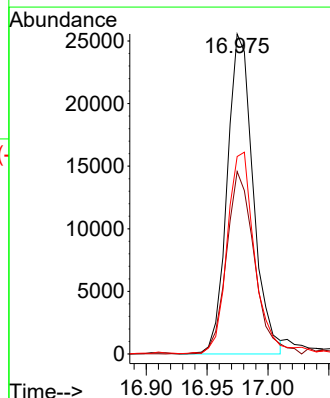



#72

Phenanthrene

Concen: 4.890 ng/ul

RT: 17.369 min Scan# 2411

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:178 Resp: 405643

Ion Ratio Lower Upper

178 100

179 14.8 12.1 18.1

176 18.3 15.4 23.0

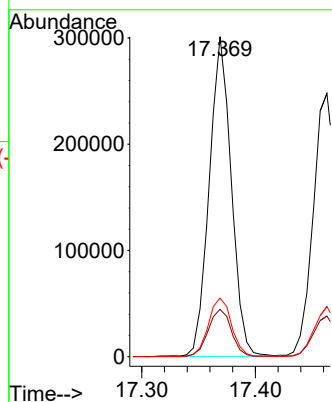

#74

Anthracene

Concen: 4.659 ng/ul

RT: 17.463 min Scan# 2427

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:178 Resp: 385891


Ion Ratio Lower Upper

178 100

179 15.4 12.5 18.7

176 19.1 14.7 22.1





#75

1,2,3,4-Tetrachlorobenzene

Concen: 5.000 ng/uL

RT: 13.369 min Scan# 1731

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:216 Resp: 113604

Ion Ratio Lower Upper

216 100

214 78.1 61.7 92.5

218 48.6 38.1 57.1



#76

Pentachlorobenzene

Concen: 4.861 ng/uL

RT: 14.887 min Scan# 1989

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:250 Resp: 112609


Ion Ratio Lower Upper

250 100

248 60.5 50.0 75.0

252 62.7 51.1 76.7









#77
 Carbazole
 Concen: 4.427 ng/ul
 RT: 17.733 min Scan# 2473
 Delta R.T. 0.006 min
 Lab File: BP013394.D
 Acq: 05 Jan 2023 13:09




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005645


Tgt Ion:167 Resp: 308800
 Ion Ratio Lower Upper
 167 100
 166 21.9 17.5 26.3
 139 12.0 9.8 14.6



#78
 Di-n-butylphthalate
 Concen: 3.414 ng/ul
 RT: 18.275 min Scan# 2565
 Delta R.T. 0.006 min
 Lab File: BP013394.D
 Acq: 05 Jan 2023 13:09

Tgt Ion:149 Resp: 289984
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.1 10.7
 104 5.8 4.3 6.5





#80

Fluoranthene

Concen: 4.274 ng/ul

RT: 19.333 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:202 Resp: 460248

Ion Ratio Lower Upper

202 100

101 9.6 8.3 12.5

100 8.8 6.8 10.2

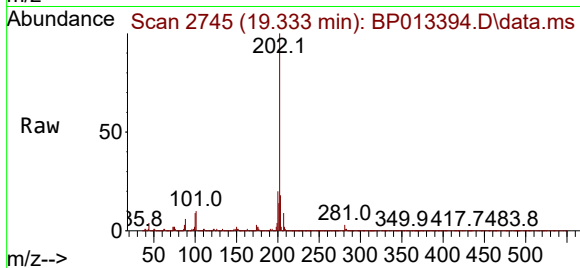

#82

Pyrene

Concen: 4.558 ng/ul

RT: 19.686 min Scan# 2805

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:202 Resp: 506343


Ion Ratio Lower Upper

202 100

101 11.8 8.8 13.2

100 10.1 7.4 11.2





#83

Butylbenzylphthalate

Concen: 2.892 ng/ul

RT: 20.551 min Scan# 2952

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:149 Resp: 124103

Ion Ratio Lower Upper

149 100

91 75.6 55.8 83.6

206 21.7 18.5 27.7

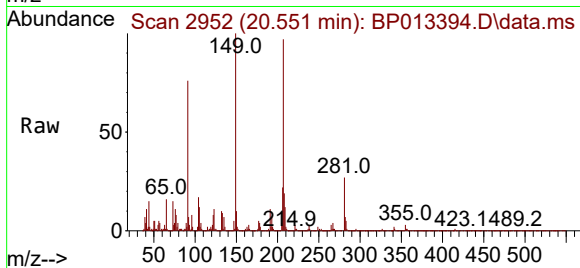

#84

3,3'-Dichlorobenzidine

Concen: 3.093 ng/ul

RT: 21.333 min Scan# 3085

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:252 Resp: 115504


Ion Ratio Lower Upper

252 100

254 65.5 51.0 76.4

126 10.5 7.0 10.4#





#85

Benzo(a)anthracene

Concen: 4.651 ng/ul

RT: 21.398 min Scan# 3095

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:228 Resp: 510437

Ion Ratio Lower Upper

228 100

229 19.8 15.9 23.9

226 26.4 21.2 31.8

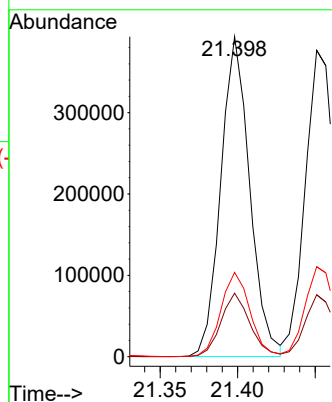

#86

Bis(2-ethylhexyl)phthalate

Concen: 3.171 ng/ul

RT: 21.310 min Scan# 3081

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:149 Resp: 191972


Ion Ratio Lower Upper

149 100

167 28.4 22.2 33.4

279 5.4 3.5 5.3#





#87

Chrysene

Concen: 4.914 ng/ul

RT: 21.451 min Scan# 3105

Delta R.T. -0.000 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:228 Resp: 509918

Ion Ratio Lower Upper

228 100

226 29.4 24.2 36.2

229 20.2 15.6 23.4

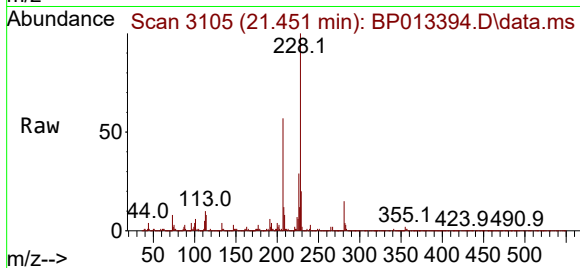

#89

Di-n-octyl phthalate

Concen: 2.802 ng/ul




RT: 22.257 min Scan# 3242


Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Tgt Ion:149 Resp: 293770

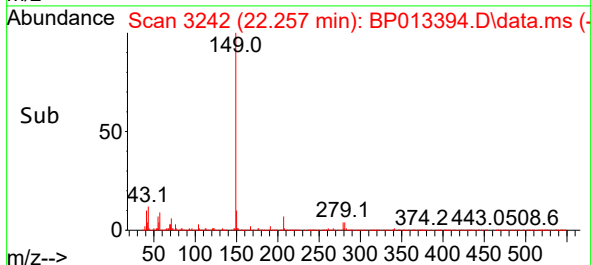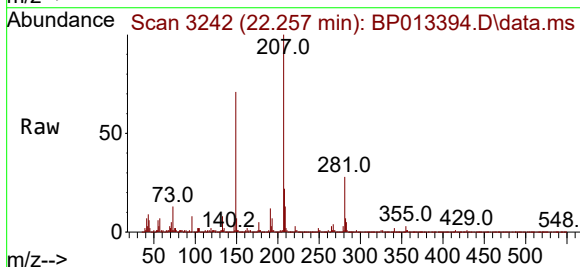



#90

Benzo(b)fluoranthene

Concen: 4.573 ng/ul

RT: 23.127 min Scan# 3388

Delta R.T. 0.012 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:252 Resp: 545716

Ion Ratio Lower Upper

252 100

253 23.0 17.7 26.5

125 9.5 7.1 10.7

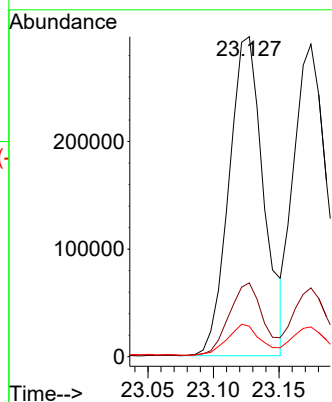

#91

Benzo(k)fluoranthene

Concen: 4.332 ng/ul

RT: 23.174 min Scan# 3398

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:252 Resp: 512647


Ion Ratio Lower Upper

252 100

253 22.0 17.6 26.4

125 9.5 6.9 10.3





#93

Benzo(a)pyrene

Concen: 4.475 ng/ul

RT: 23.768 min Scan# 34

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:252 Resp: 465017

Ion Ratio Lower Upper

252 100

253 24.5 17.4 26.0

125 11.0 7.6 11.4

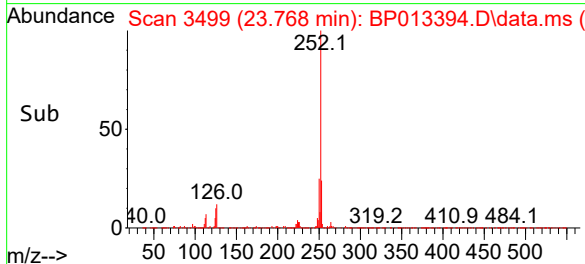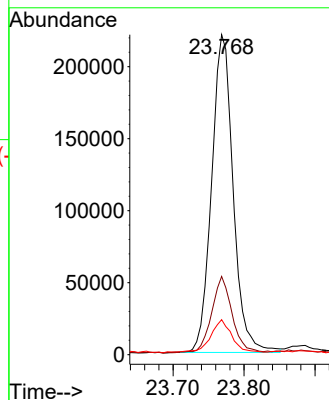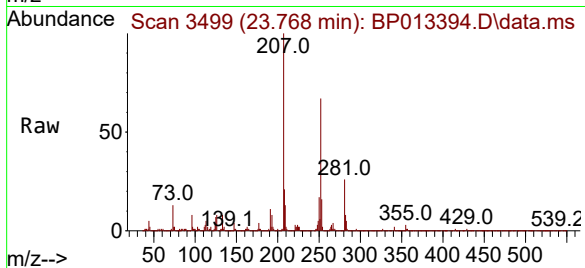

#94

Indeno(1,2,3-cd)pyrene

Concen: 5.045 ng/ul

RT: 26.451 min Scan# 3955

Delta R.T. 0.006 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09




Tgt Ion:276 Resp: 653013


Ion Ratio Lower Upper

276 100

138 21.9 17.3 25.9

277 25.6 20.1 30.1

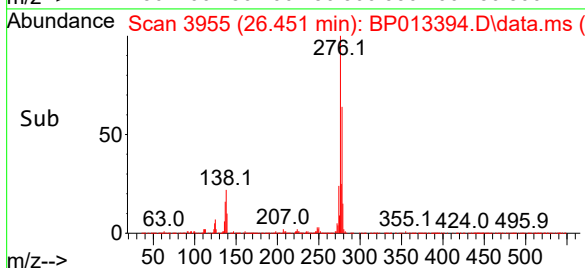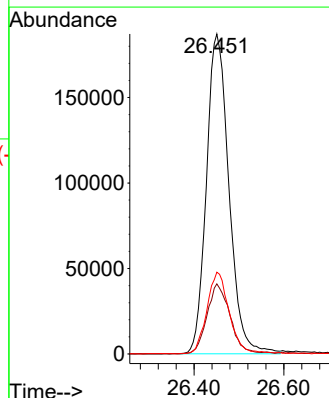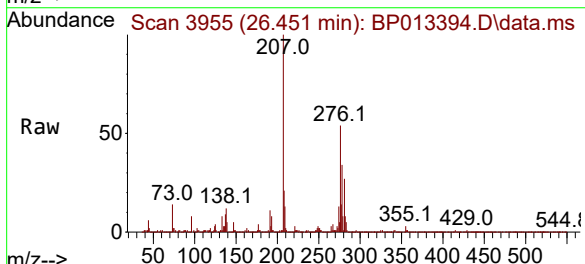



#95

Dibenzo(a,h)anthracene

Concen: 5.114 ng/ul

RT: 26.468 min Scan# 3958

Delta R.T. 0.012 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Instrument :

BNA_P

ClientSampleId :

SSTD005645





Tgt Ion:278 Resp: 548041

Ion Ratio Lower Upper

278 100

139 13.2 11.3 16.9

279 22.5 19.2 28.8



#96

Benzo(g,h,i)perylene

Concen: 5.194 ng/ul

RT: 27.245 min Scan# 4090

Delta R.T. 0.012 min

Lab File: BP013394.D

Acq: 05 Jan 2023 13:09

Tgt Ion:276 Resp: 539702

Ion Ratio Lower Upper

276 100

138 18.1 14.5 21.7

277 24.1 18.8 28.2

