
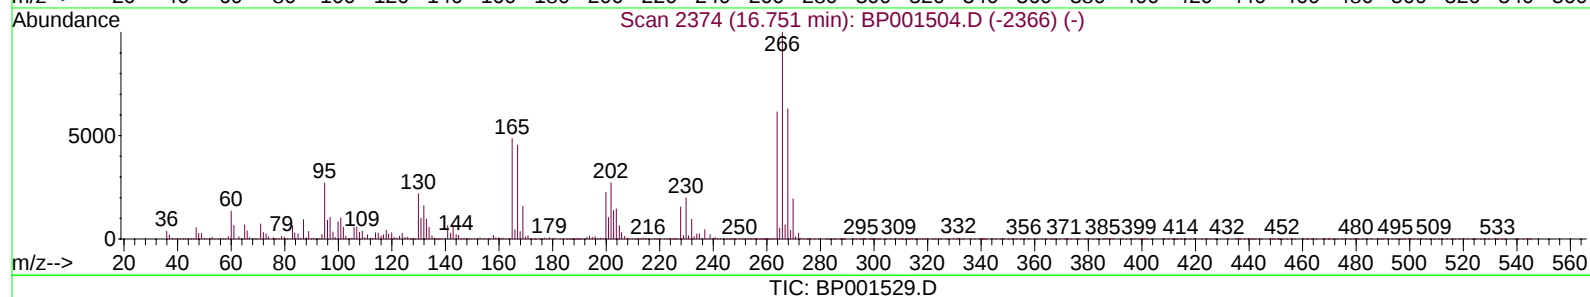
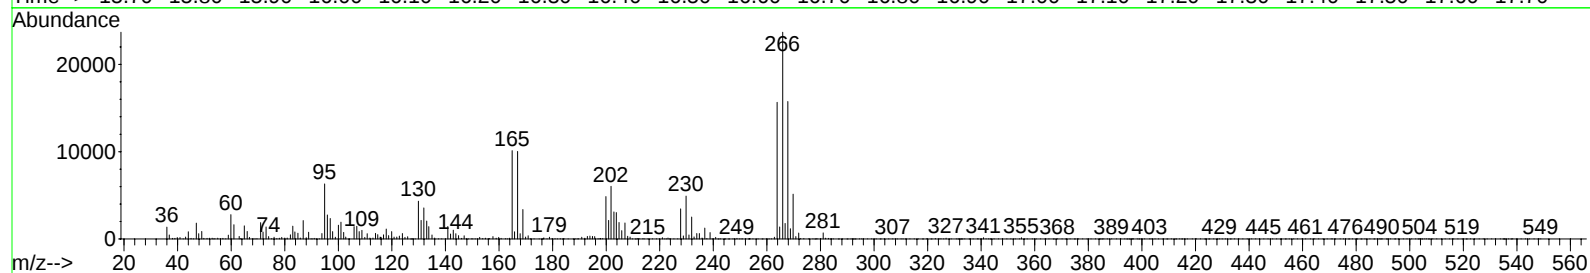


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP010620\
Data File : BP001529.D
Acq On : 06 Jan 2020 14:08
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 17:54:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 06 16:38:29 2020
Response via : Initial Calibration

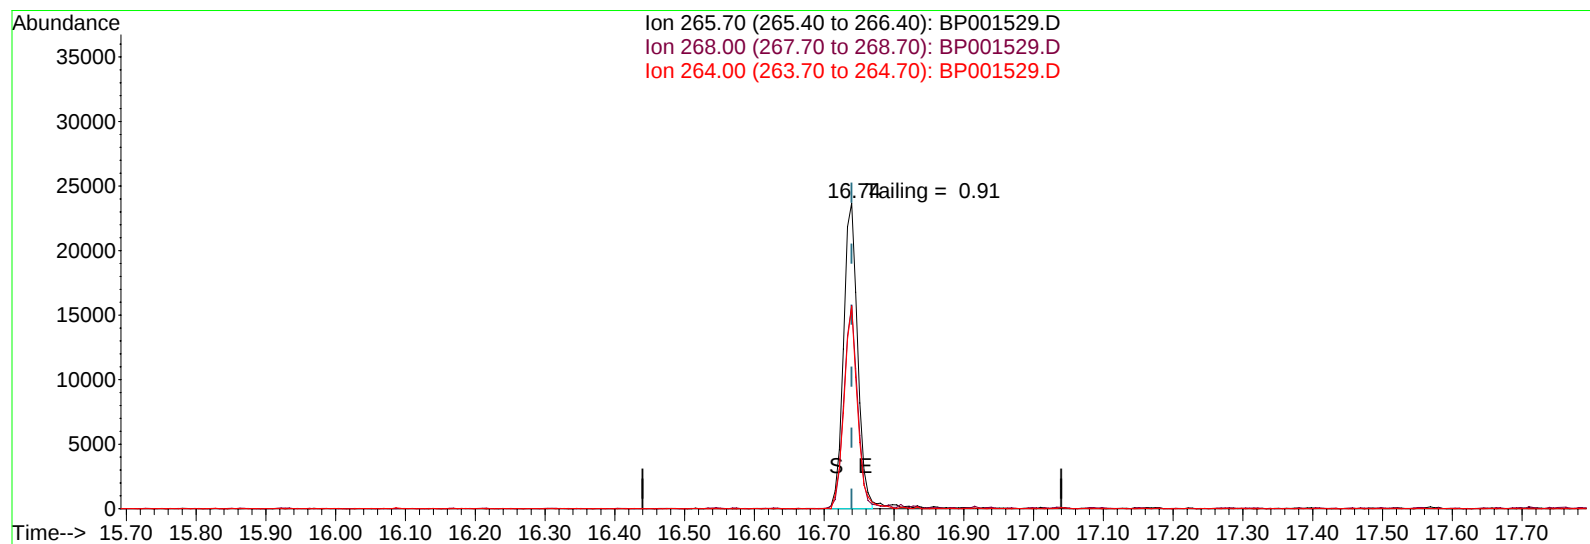

(70) Pentachlorophenol (C)




16.739min (-0.000) 435611.95ng

response 33507

Ion	Exp%	Act%
265.70	100	100
268.00	59.80	66.52
264.00	62.60	66.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP010620\
 Data File : BP001529.D
 Acq On : 06 Jan 2020 14:08
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 17:54:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 06 16:38:29 2020
 Response via : Initial Calibration

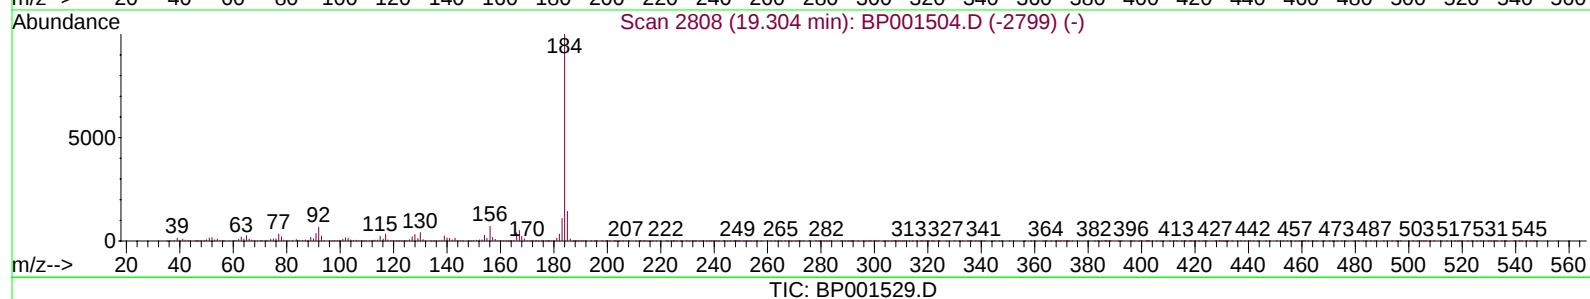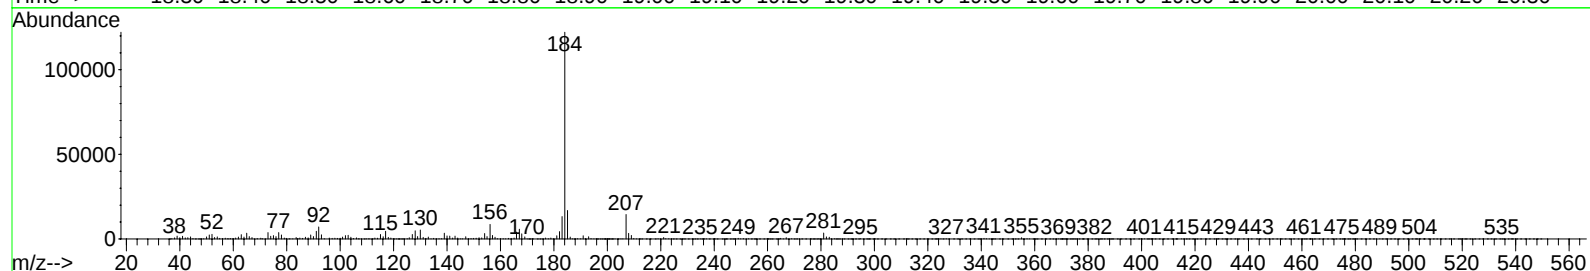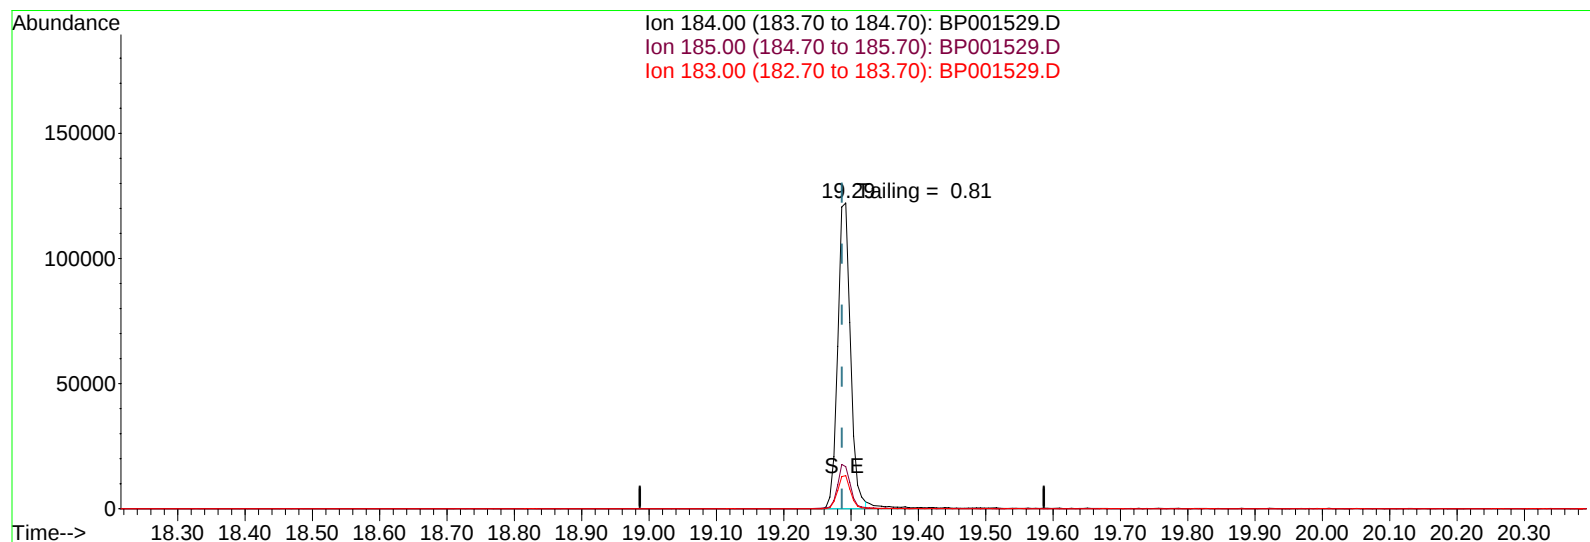

(77) Benzidine

19.292min (+0.006) 247244.53ng

response 163948

Ion	Exp%	Act%
184.00	100	100
185.00	13.40	13.75
183.00	11.40	10.81
0.00	0.00	0.00