


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP010620\
 Data File : BP001529.D
 Acq On : 06 Jan 2020 14:08
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 06 16:38:29 2020

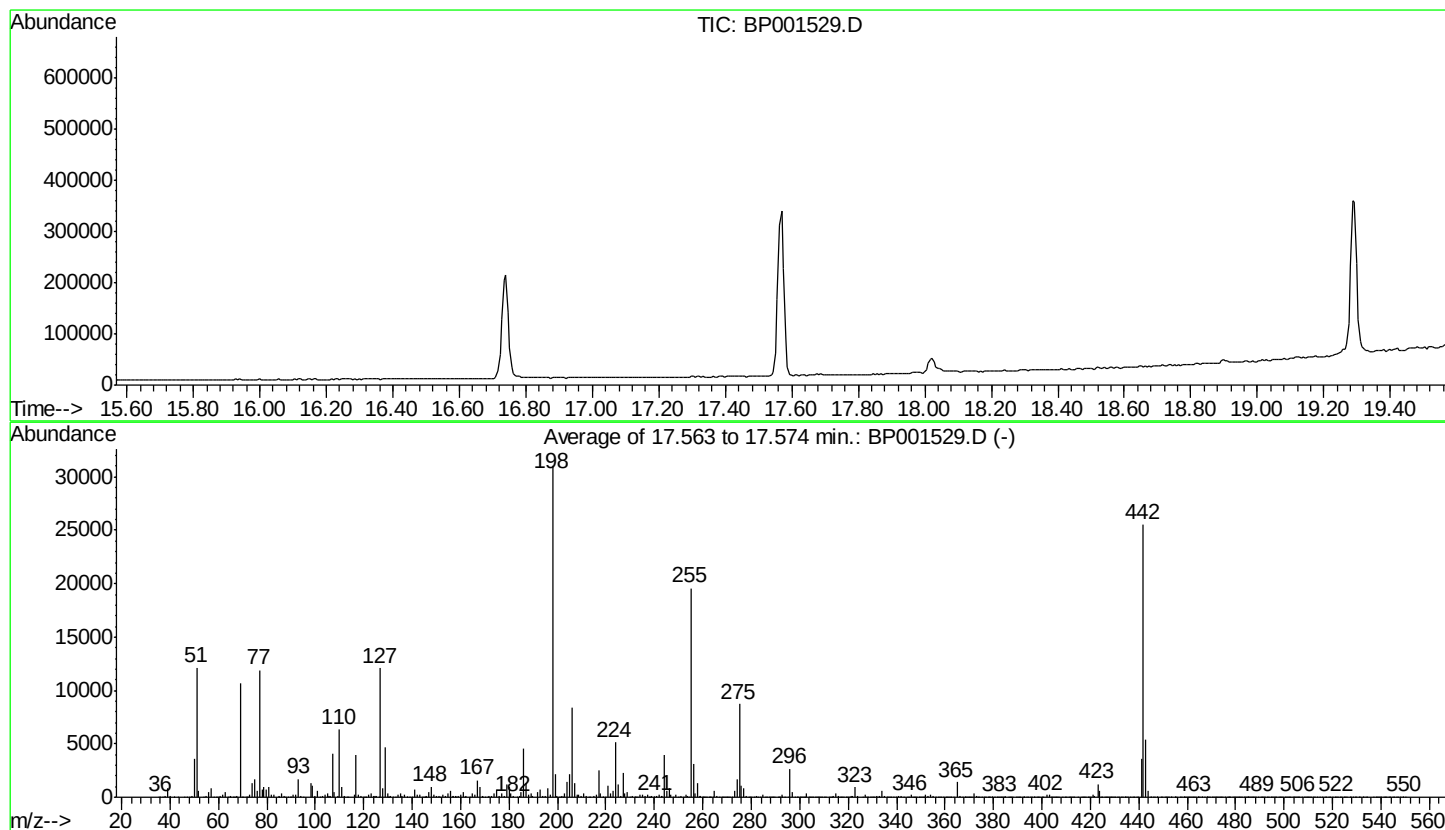

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	12147	PASS
68	69	0.00	2	1.7	180	PASS
69	198	0.00	100	34.2	10623	PASS
70	69	0.00	2	0.5	48	PASS
127	198	10	80	38.9	12069	PASS
197	198	0.00	2	0.7	219	PASS
198	198	100	100	100.0	31054	PASS
199	198	5	9	7.0	2186	PASS
275	198	10	60	28.2	8750	PASS
365	198	1	100	4.5	1387	PASS
441	198	0.01	100	11.5	3585	PASS
442	198	50	100	82.2	25527	PASS
443	442	15	24	21.2	5414	PASS