
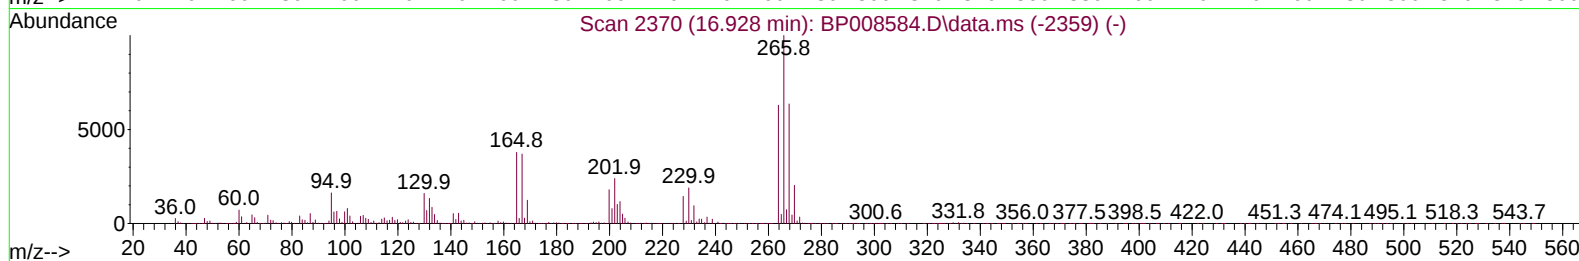
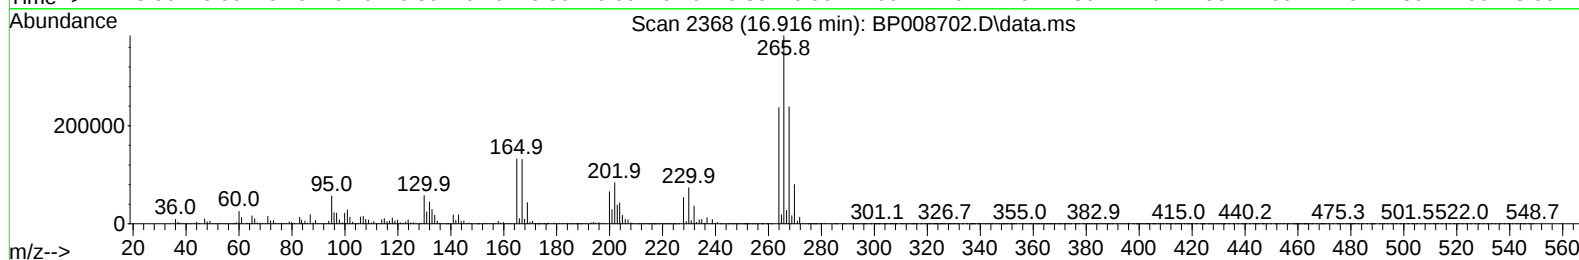


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
 Data File : BP008702.D
 Acq On : 06 Jan 2022 10:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 16:10:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 06 16:06:12 2022
 Response via : Initial Calibration

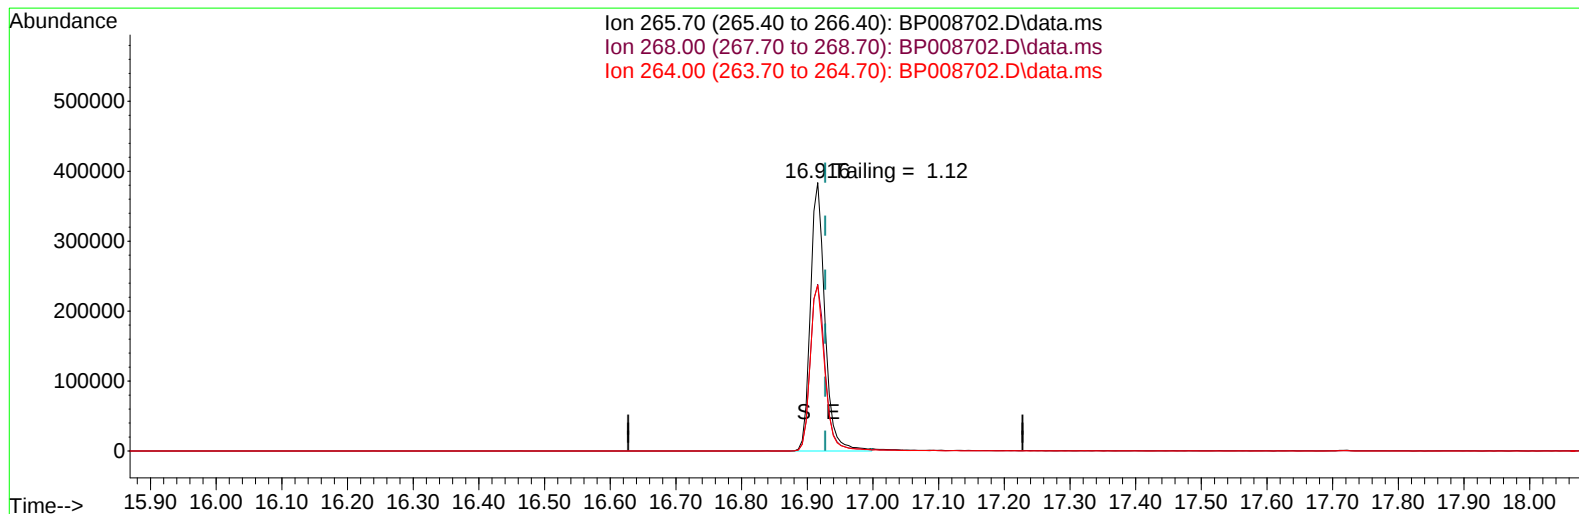

TIC: BP008702.D\data.ms

(70) Pentachlorophenol (C)




16.916min (-0.012) 146072.11 ng

response 594158

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.09
264.00	62.90	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
Data File : BP008702.D
Acq On : 06 Jan 2022 10:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 16:10:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 06 16:06:12 2022
Response via : Initial Calibration

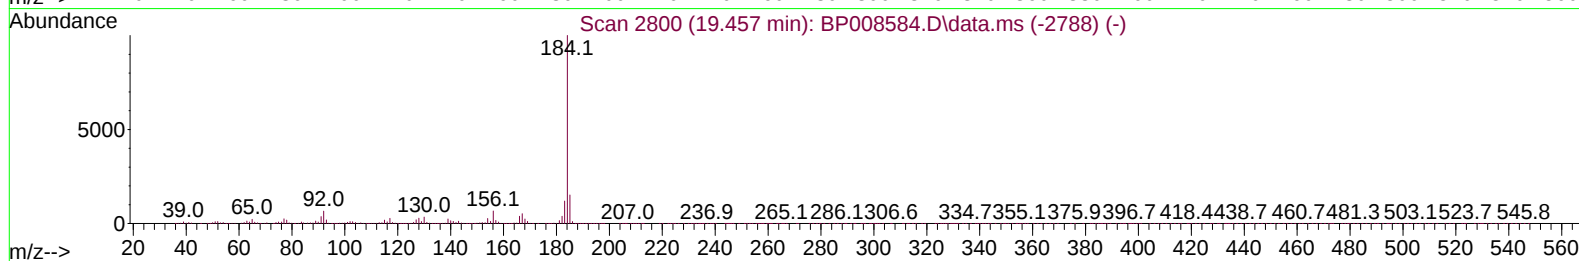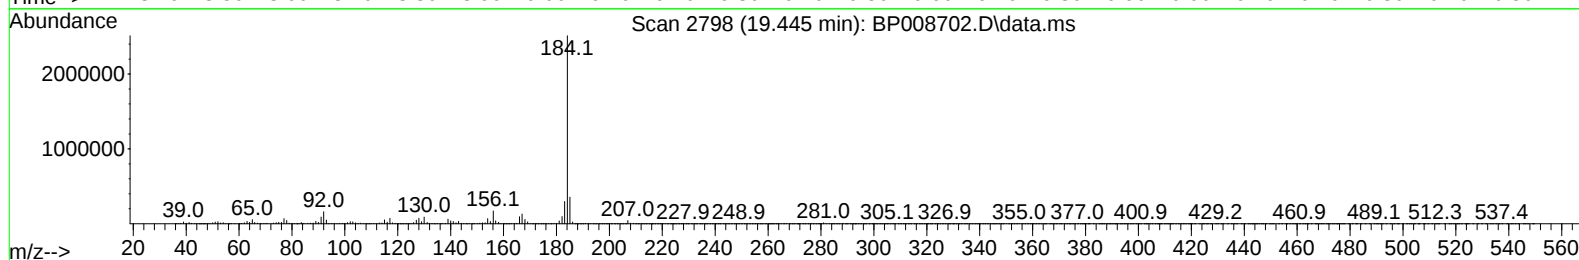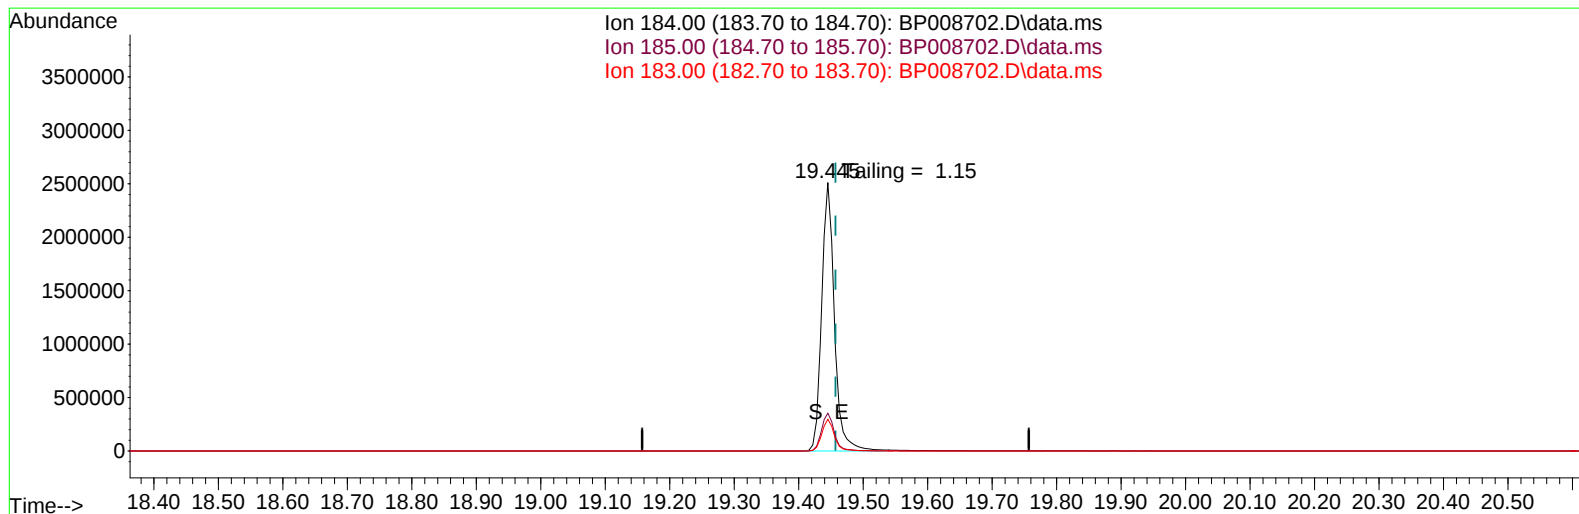

TIC: BP008702.D\data.ms

(77) Benzidine**19.445min (-0.012) 37369.52 ng****response 3471419**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.12
183.00	11.90	11.86
0.00	0.00	0.00