

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
 Data File : BP008712.D
 Acq On : 06 Jan 2022 16:53
 Operator : CG/JU
 Sample : PB141691BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141691BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	415	421	441	rVB	7149746	11121548	30.46%	8.031%
2	7.057	684	692	708	rBV	6947922	11483806	31.46%	8.292%
3	7.887	826	833	845	rBV	1376777	2258724	6.19%	1.631%
4	9.046	1021	1030	1046	rBV	4290103	7303492	20.01%	5.274%
5	10.687	1301	1309	1324	rBV	1830193	3286732	9.00%	2.373%
6	13.151	1720	1728	1743	rBV	13774166	20642890	56.55%	14.906%
7	14.522	1953	1961	1975	rBV	3415896	5010511	13.73%	3.618%
8	15.533	2125	2133	2147	rBV	249489	535452	1.47%	0.387%
9	16.016	2207	2215	2239	rBV	12193976	17602157	48.22%	12.710%
10	17.275	2422	2429	2441	rBV	4557501	6513656	17.84%	4.703%
11	19.839	2859	2865	2870	rBV	29243155	36506351	100.00%	26.361%
12	21.363	3119	3124	3134	rBV	5981521	7775529	21.30%	5.615%
13	23.798	3531	3538	3549	rVB2	4064052	8445471	23.13%	6.098%


Sum of corrected areas: 138486319

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
Data File : BP008712.D
Acq On : 06 Jan 2022 16:53
Operator : CG/JU
Sample : PB141691BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141691BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

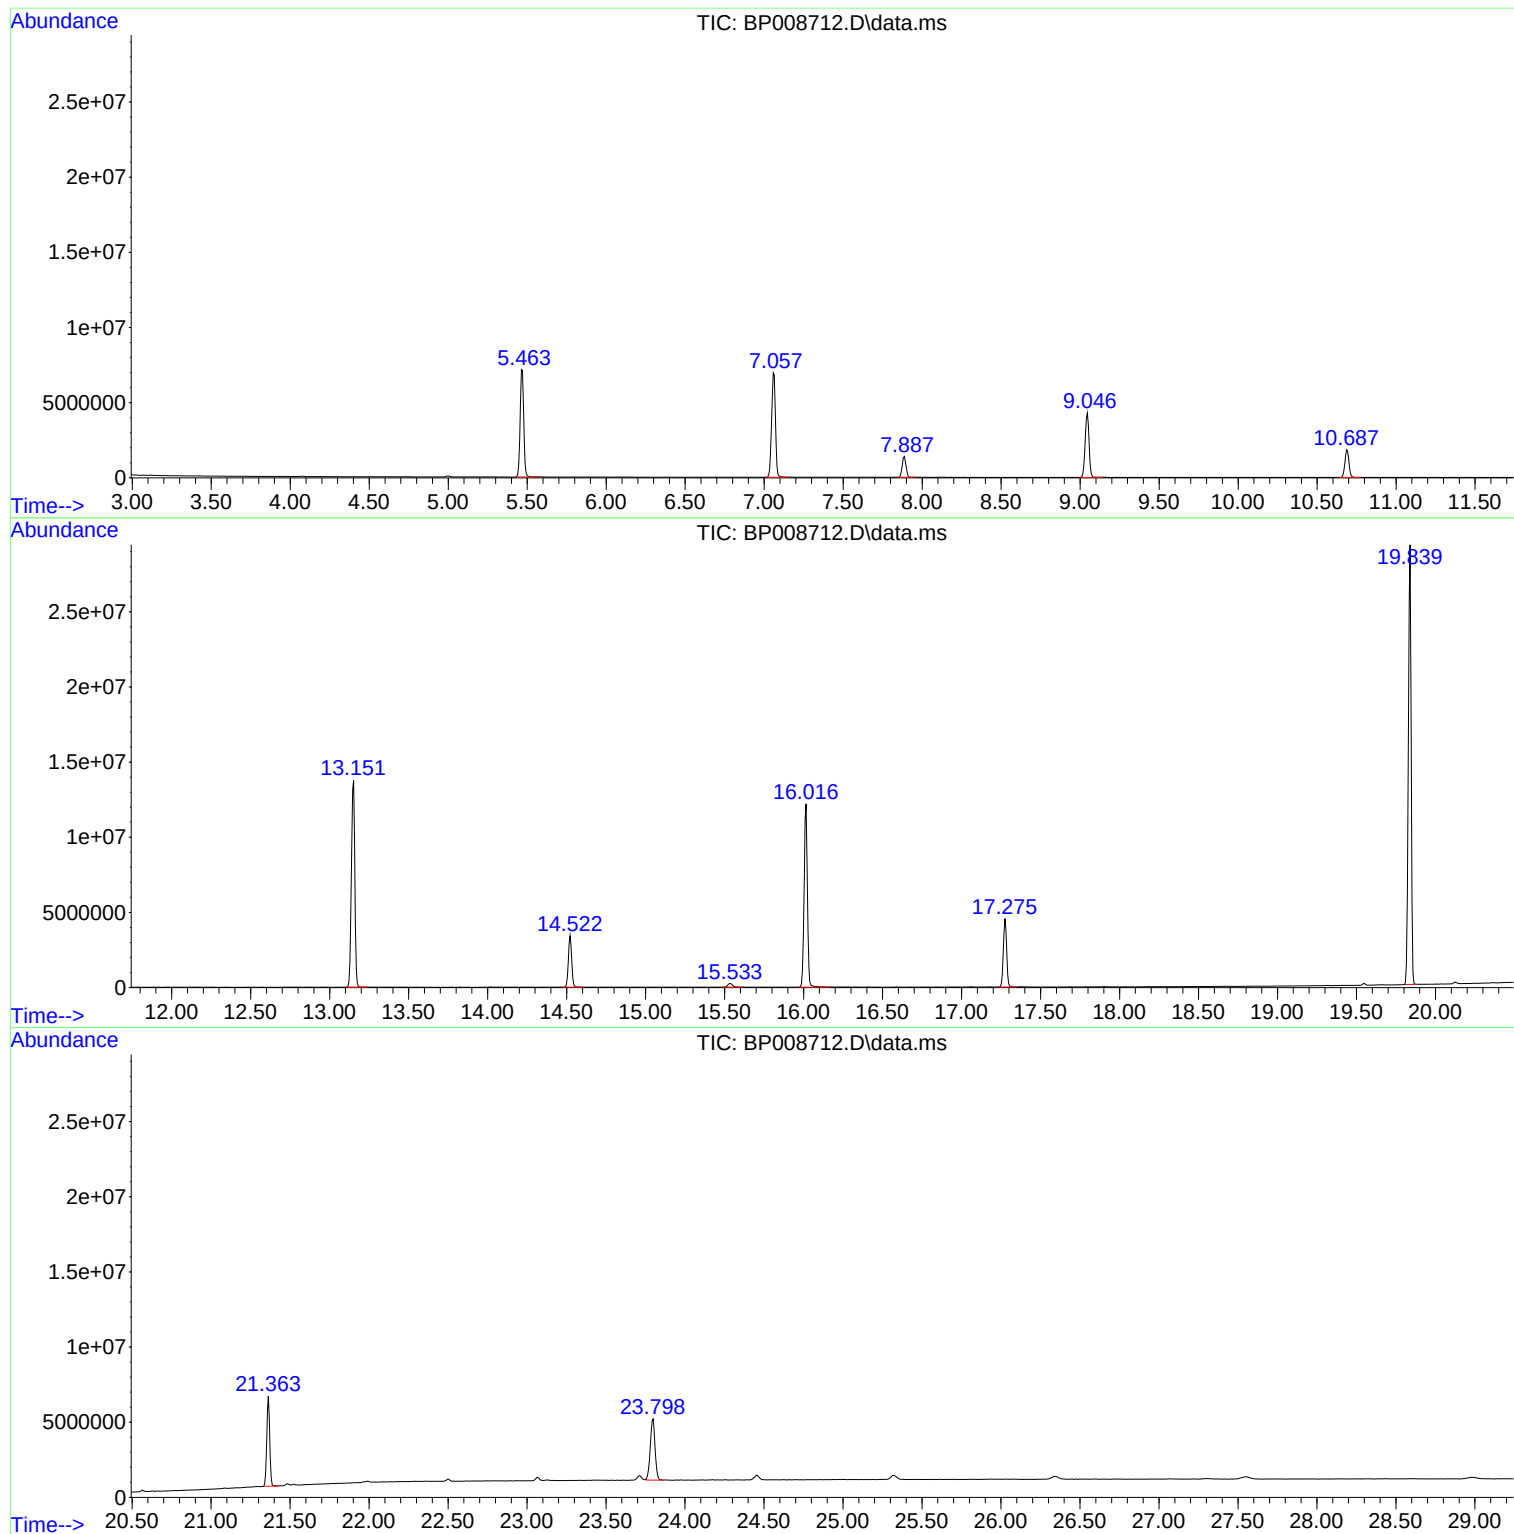

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
Data File : BP008712.D
Acq On : 06 Jan 2022 16:53
Operator : CG/JU
Sample : PB141691BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141691BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diphenyl sulfide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.534	2.14 ng	535452	Acenaphthene-d10	14.522

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diphenyl sulfide	186	C12H10S	000139-66-2	96
2			Imidazole, 5-phenyl-1,2,4-trimet...	186	C12H14N2	062576-15-2	64
3			1H-Benzo[d]pyrrolo[1,2-a]imidazo...	186	C12H14N2	1000304-47-4	64
4			6,8-Diazatricyclo[7.5.0.0(2,7)]t...	186	C12H14N2	1000459-82-3	59
5			1-Naphthalenecarboxaldehyde, 4-m...	186	C12H10O2	015971-29-6	59

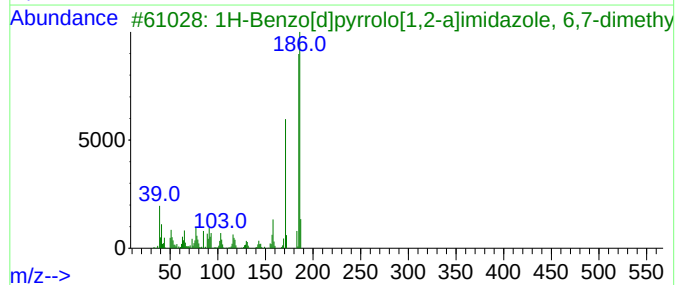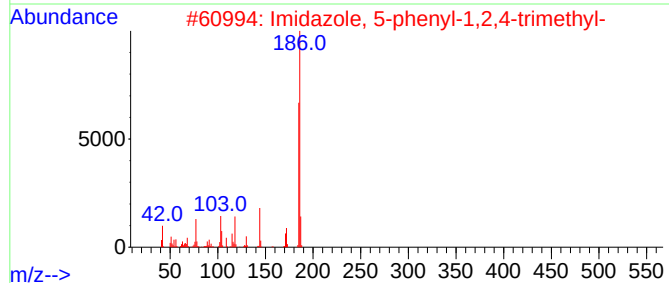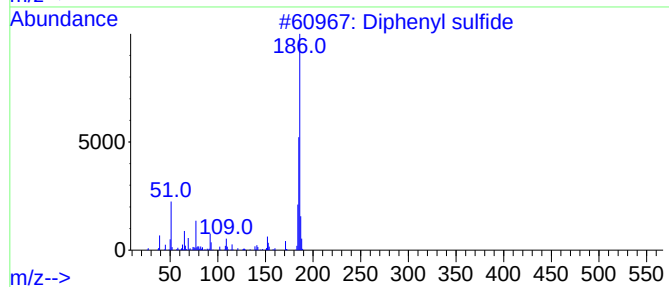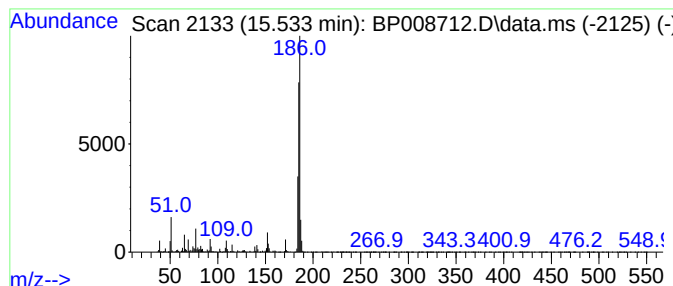

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
Data File : BP008712.D
Acq On : 06 Jan 2022 16:53
Operator : CG/JU
Sample : PB141691BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141691BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diphenyl sulfide	15.534	2.1	ng	535452	3	14.522	5010510	20.0