
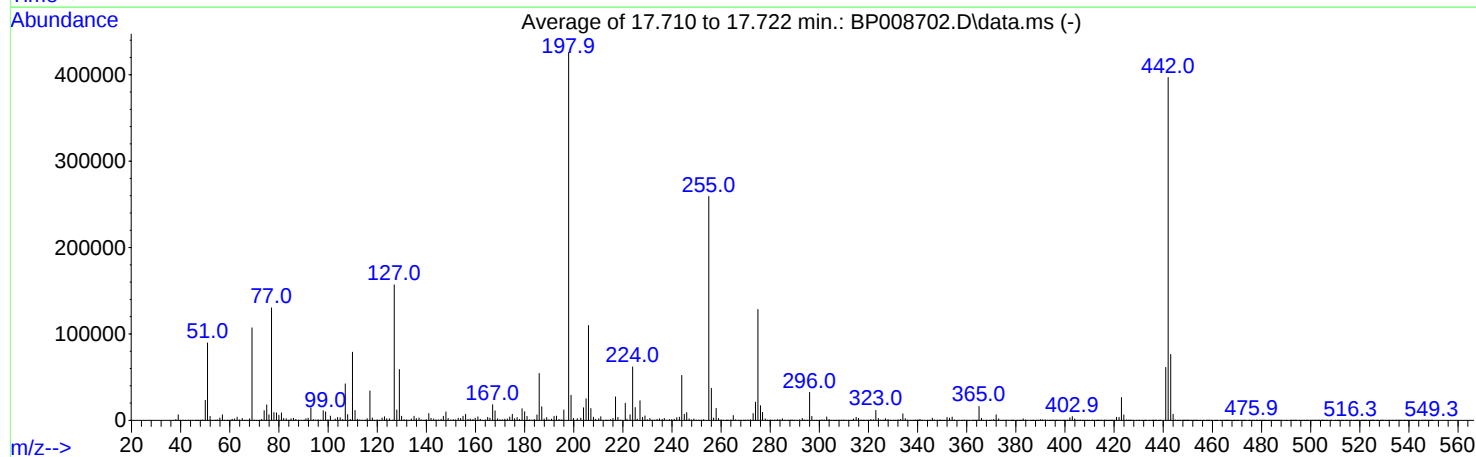


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
 Data File : BP008702.D
 Acq On : 06 Jan 2022 10:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 07 07:45:52 2022

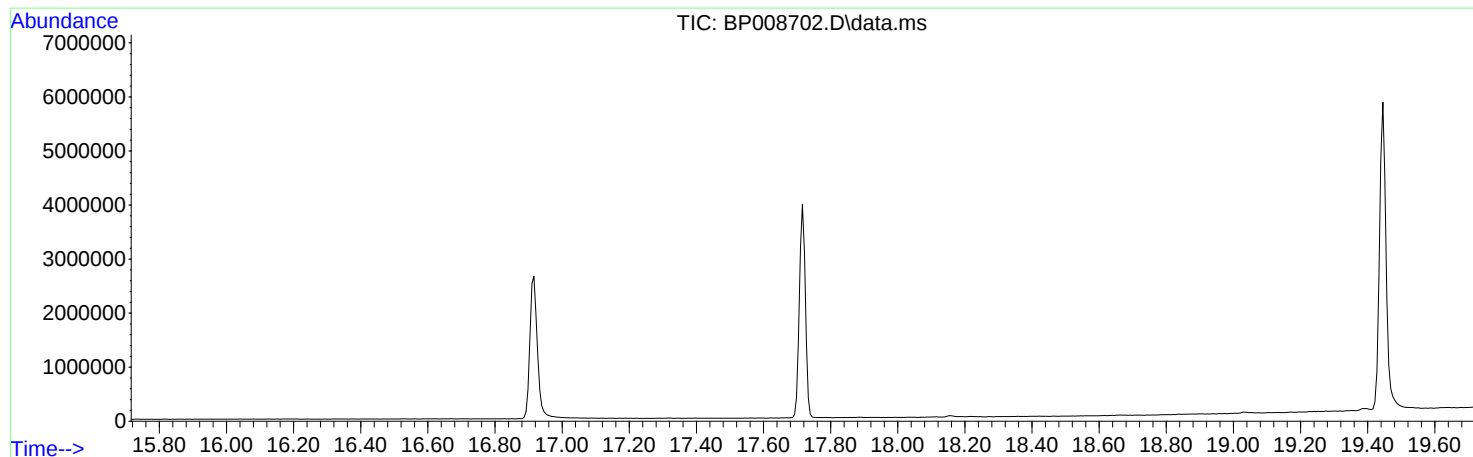




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.1	89705	PASS
68	69	0.00	2	1.8	1908	PASS
69	198	0.00	100	25.1	106952	PASS
70	69	0.00	2	0.4	457	PASS
127	198	10	80	36.9	156873	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	425664	PASS
199	198	5	9	6.8	29035	PASS
275	198	10	60	30.2	128360	PASS
365	198	1	100	3.8	16151	PASS
441	198	0.01	100	14.4	61386	PASS
442	442	100	100	100.0	396738	PASS
443	442	15	24	19.2	76349	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
 Data File : BP008702.D
 Acq On : 06 Jan 2022 10:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 06 16:10:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 06 16:06:12 2022
 Response via : Initial Calibration

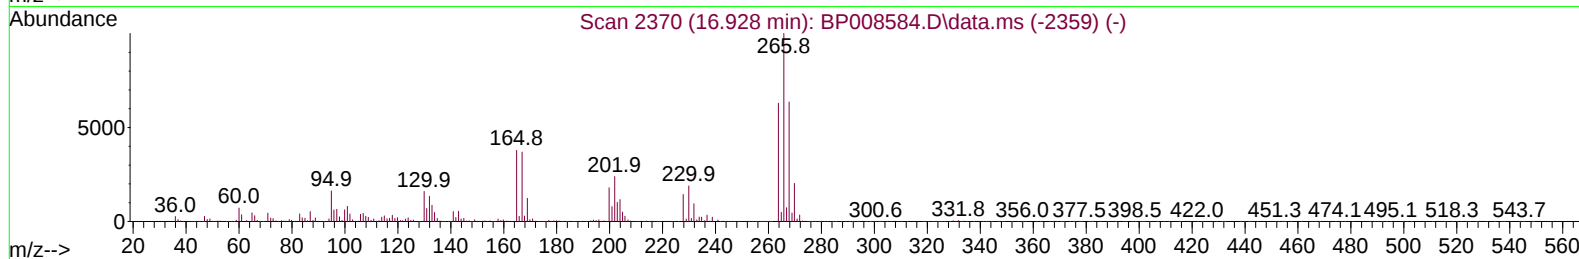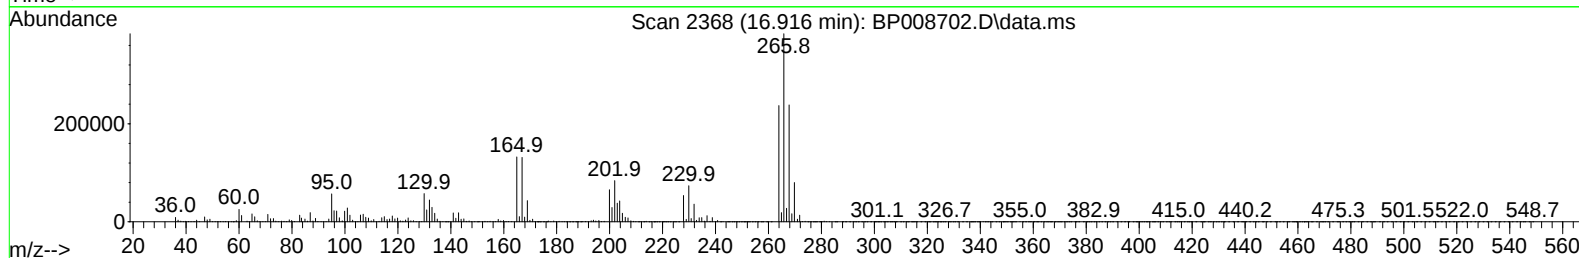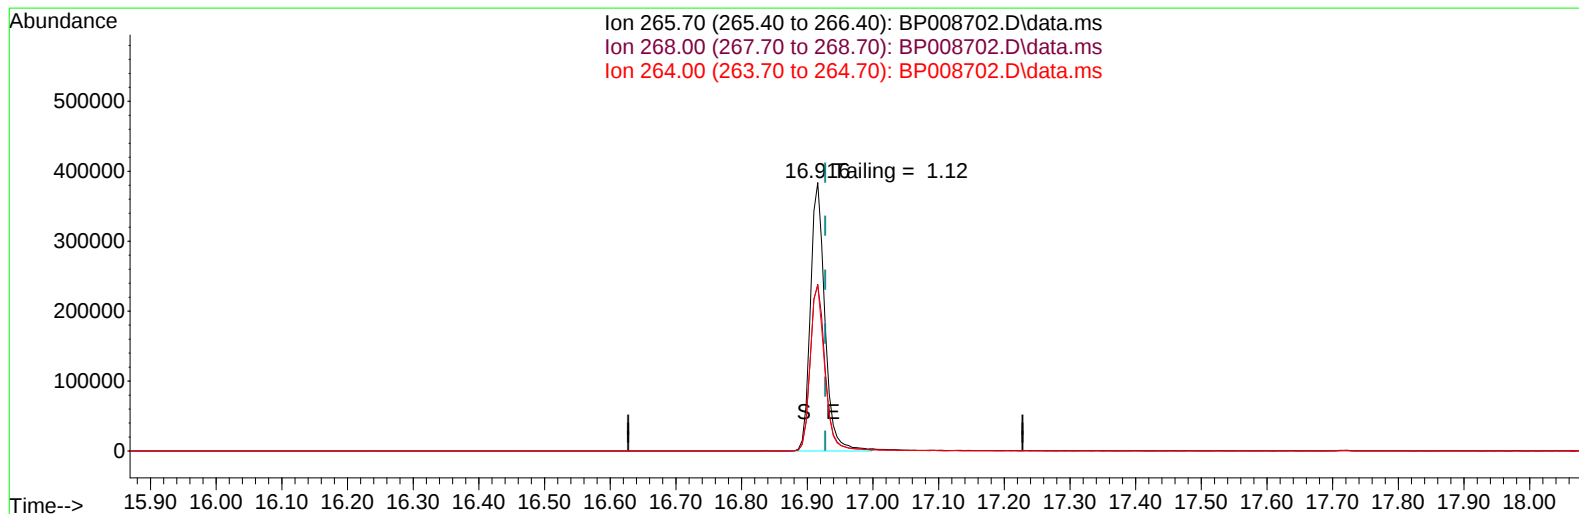

TIC: BP008702.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.012) 146072.11 ng




response 594158

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.09
264.00	62.90	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010622\
 Data File : BP008702.D
 Acq On : 06 Jan 2022 10:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 06 16:10:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 06 16:06:12 2022
 Response via : Initial Calibration

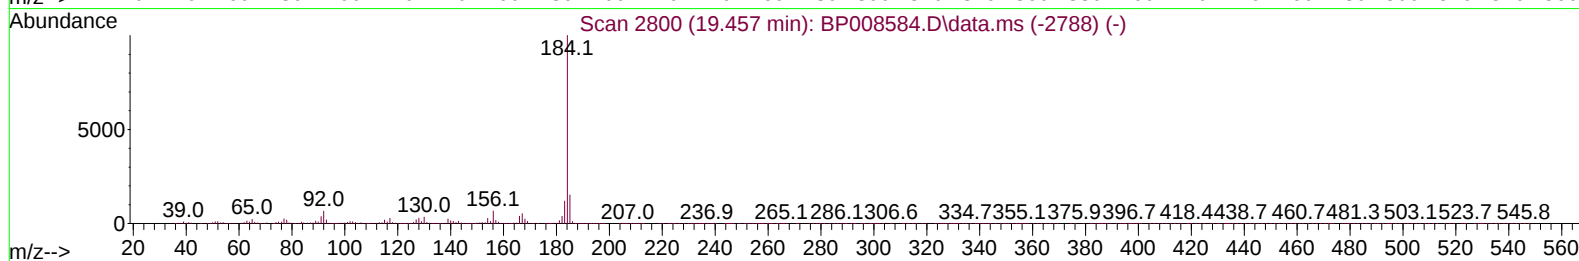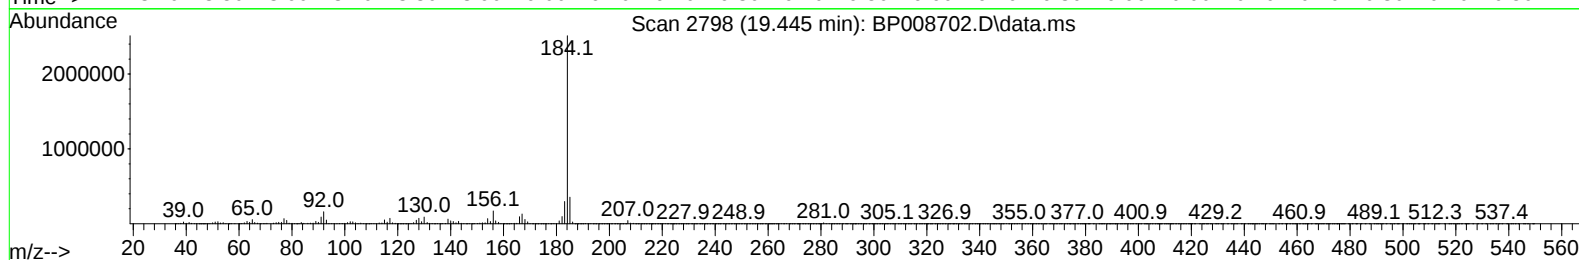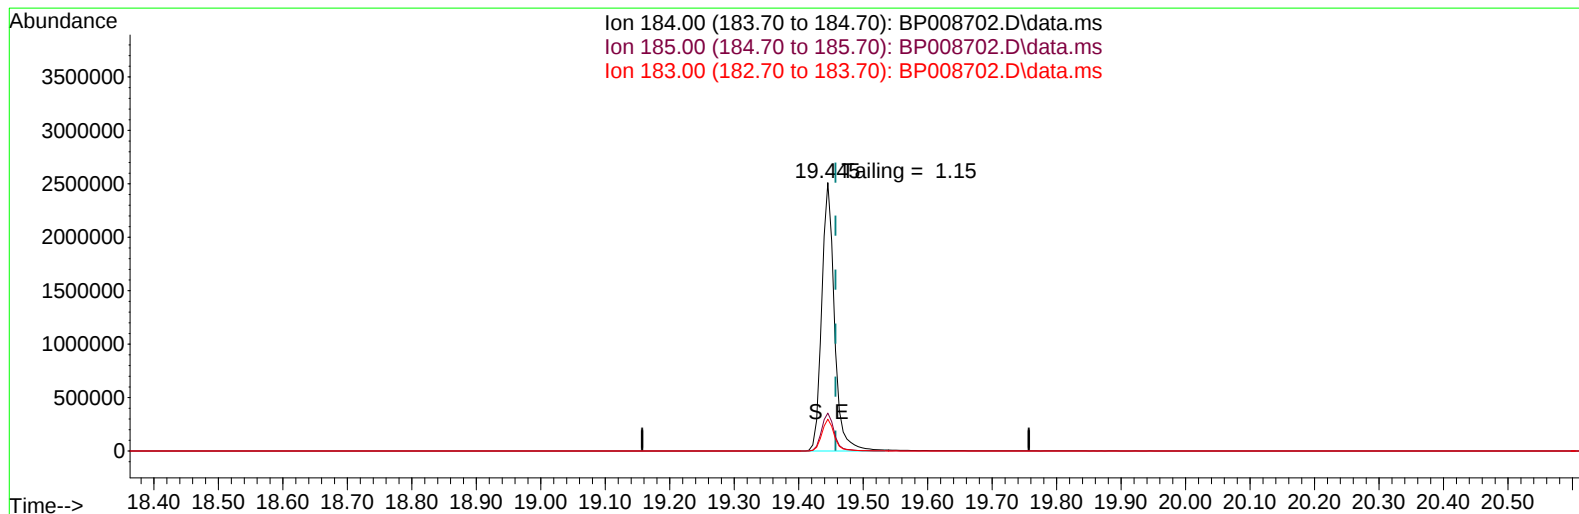

TIC: BP008702.D\data.ms

(77) Benzidine

19.445min (-0.012) 37369.52 ng

response 3471419

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.12
183.00	11.90	11.86
0.00	0.00	0.00

Instrument :

BNA_P

ClientSampleId :

DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/6/2022	BNA_P	<u>BP008702.D</u>
Compound Name	Response	Retention Time
DDT	1651899	20.65
DDD	29267	20.22
DDE	2619	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31886	1683785	1.89