

Data File : BP001574.D

Acq On : 09 Jan 2020 10:58

Operator : JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1



Quant Time: Jan 10 06:33:41 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jan 08 15:02:19 2020

Response via : Initial Calibration

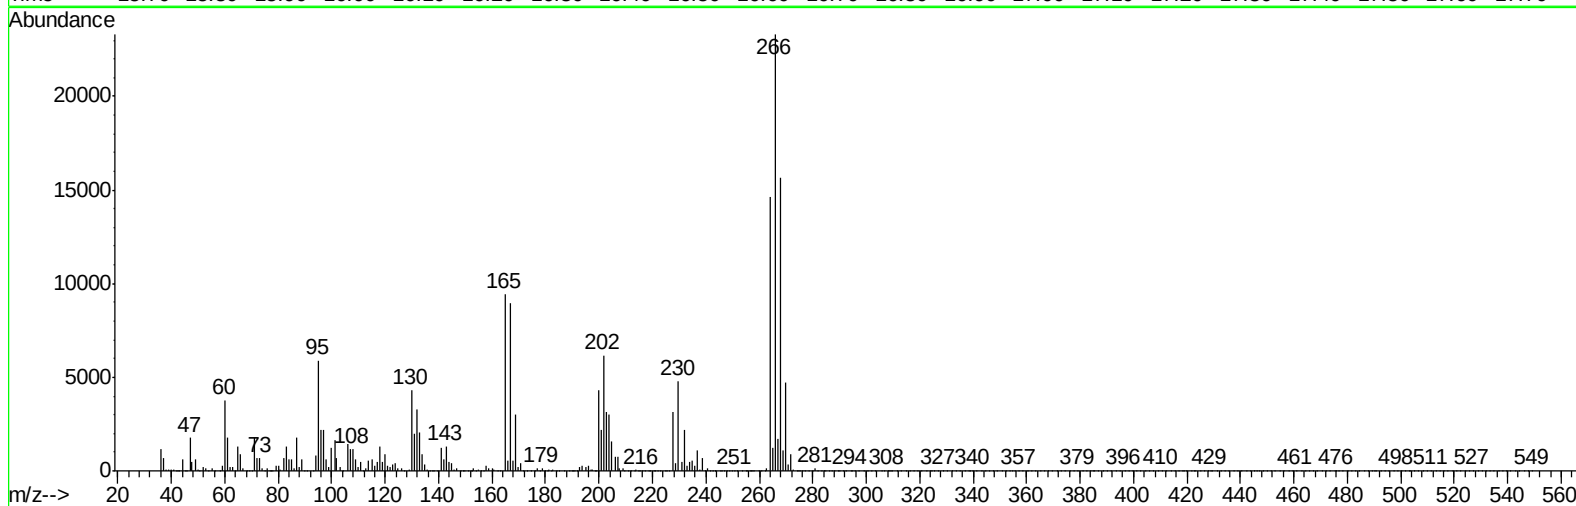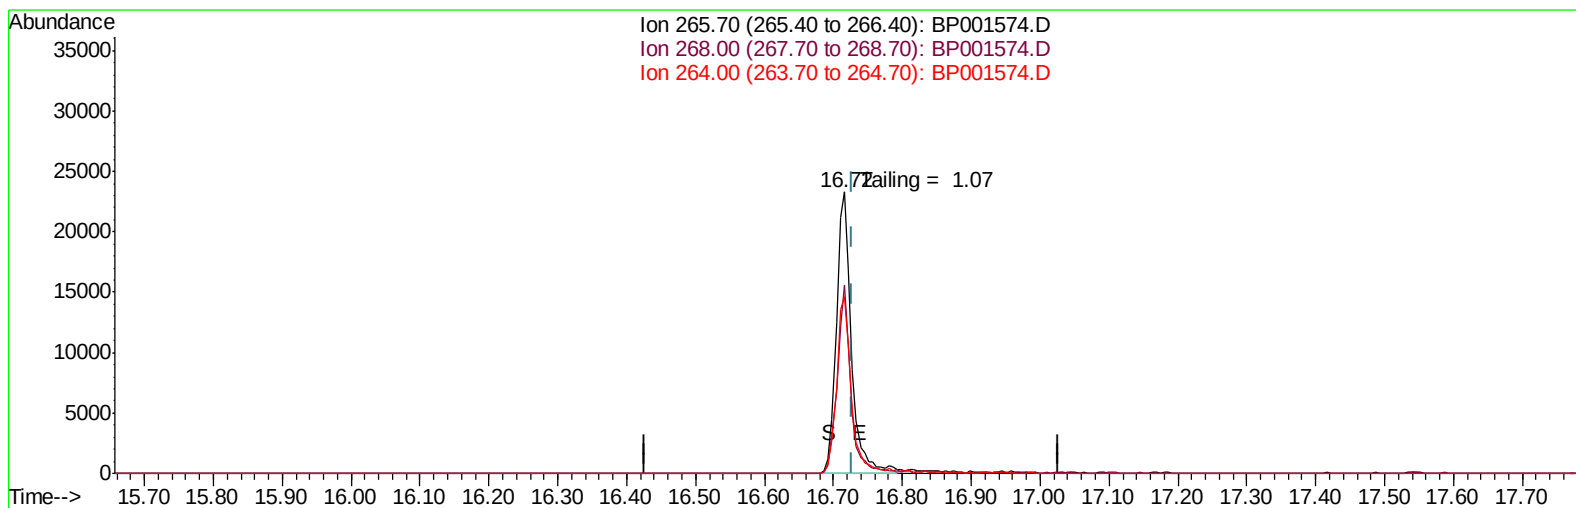

TIC: BP001574.D

(70) Pentachlorophenol (C)



16.716min (-0.012) 174150.27ng

response 35296

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	67.02
264.00	63.60	62.85
0.00	0.00	0.00

Data File : BP001574.D
Acq On : 09 Jan 2020 10:58
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 06:33:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 15:02:19 2020
Response via : Initial Calibration

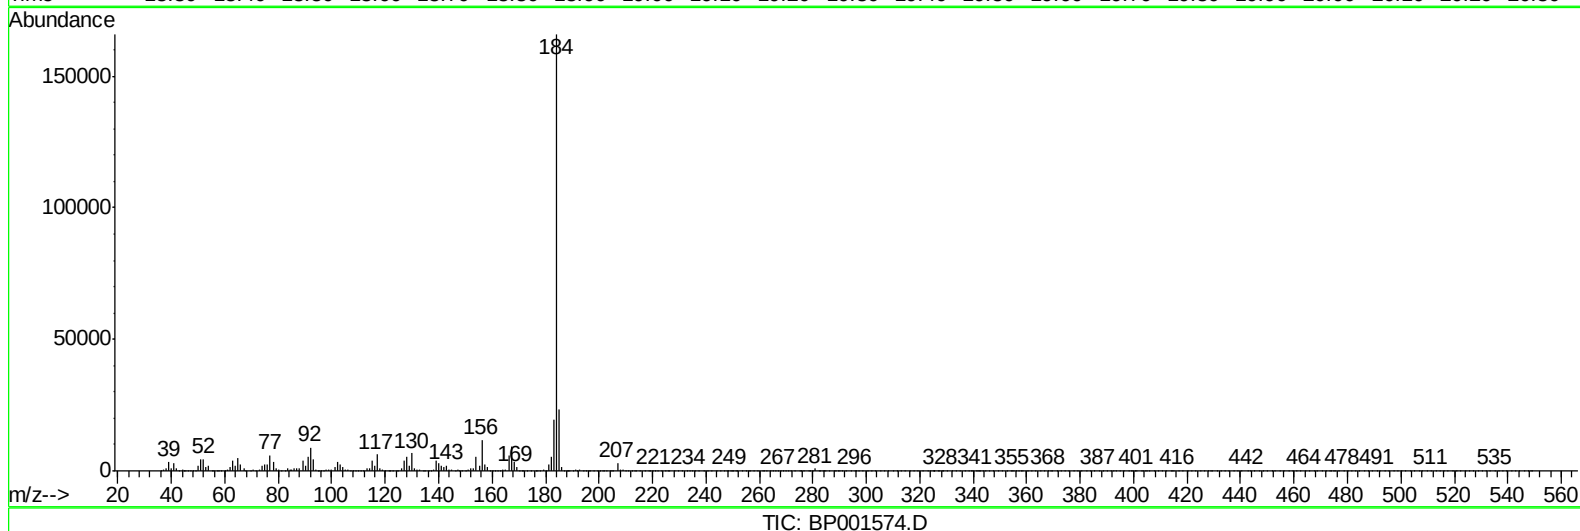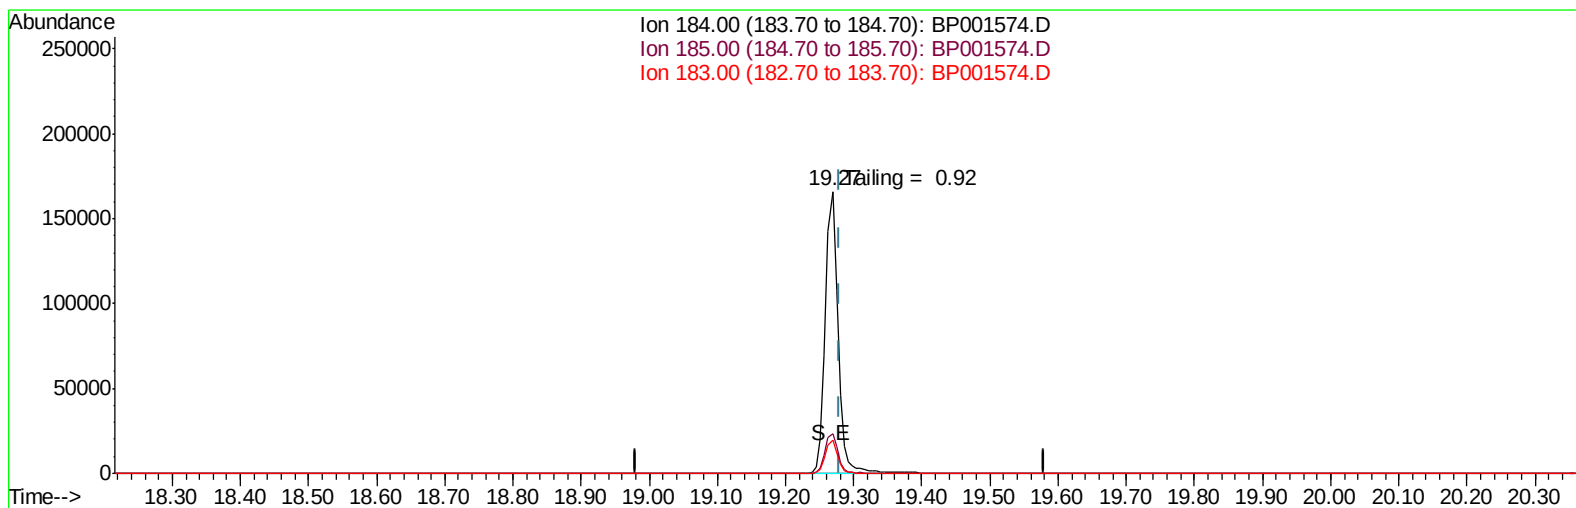

TIC: BP001574.D

(77) Benzidine

19.269min (-0.012) 18051.88ng

response 211865

Ion	Exp%	Act%
184.00	100	100
185.00	13.30	14.18
183.00	11.70	11.84
0.00	0.00	0.00