


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP010920\
 Data File : BP001574.D
 Acq On : 09 Jan 2020 10:58
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 15:02:19 2020

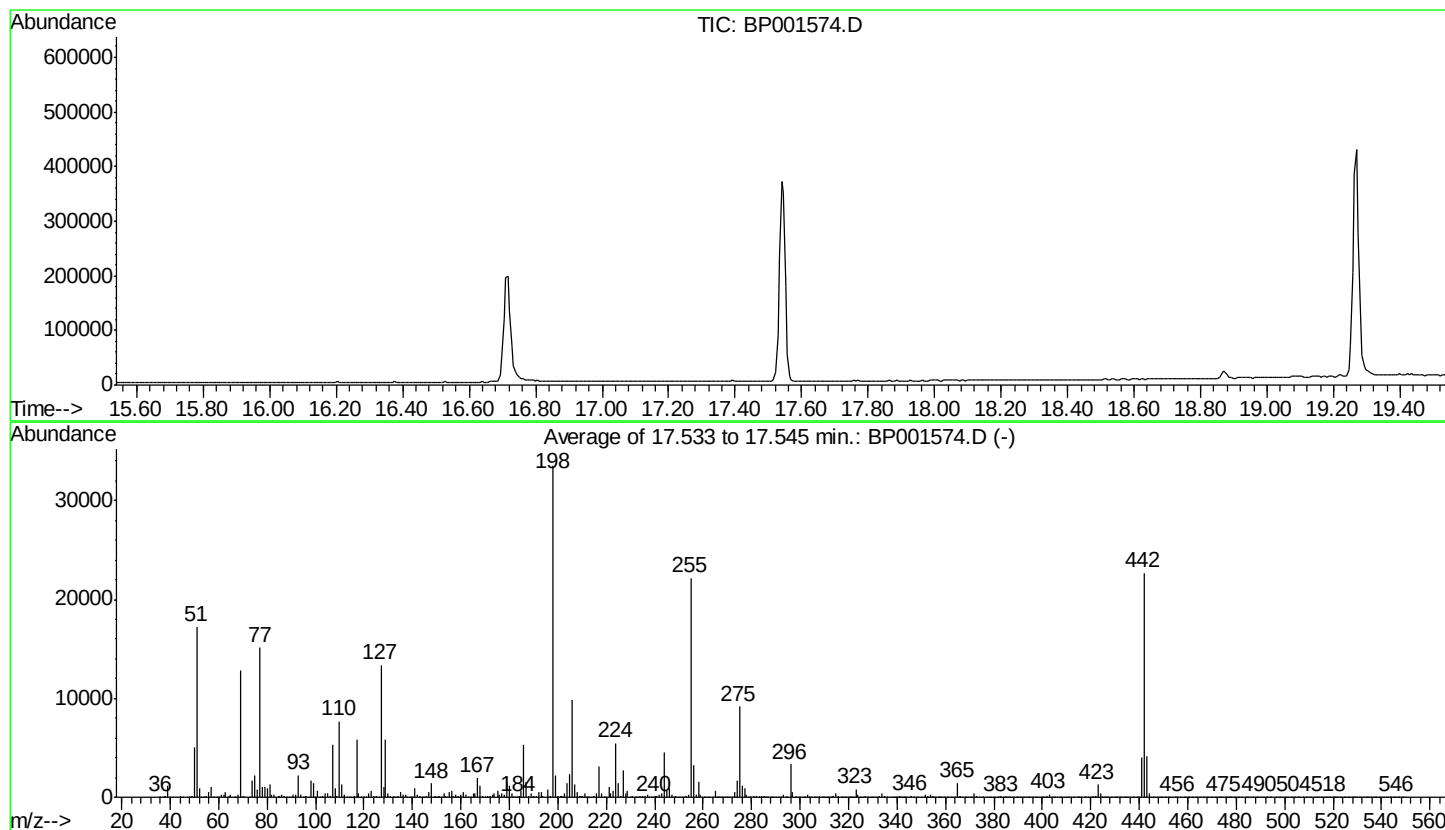

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	17262	PASS
68	69	0.00	2	1.8	236	PASS
69	198	0.00	100	38.3	12856	PASS
70	69	0.00	2	0.8	105	PASS
127	198	10	80	39.8	13350	PASS
197	198	0.00	2	0.4	142	PASS
198	198	100	100	100.0	33531	PASS
199	198	5	9	6.7	2241	PASS
275	198	10	60	27.4	9182	PASS
365	198	1	100	4.3	1437	PASS
441	198	0.01	100	11.9	3976	PASS
442	198	50	100	67.7	22707	PASS
443	442	15	24	18.5	4198	PASS