
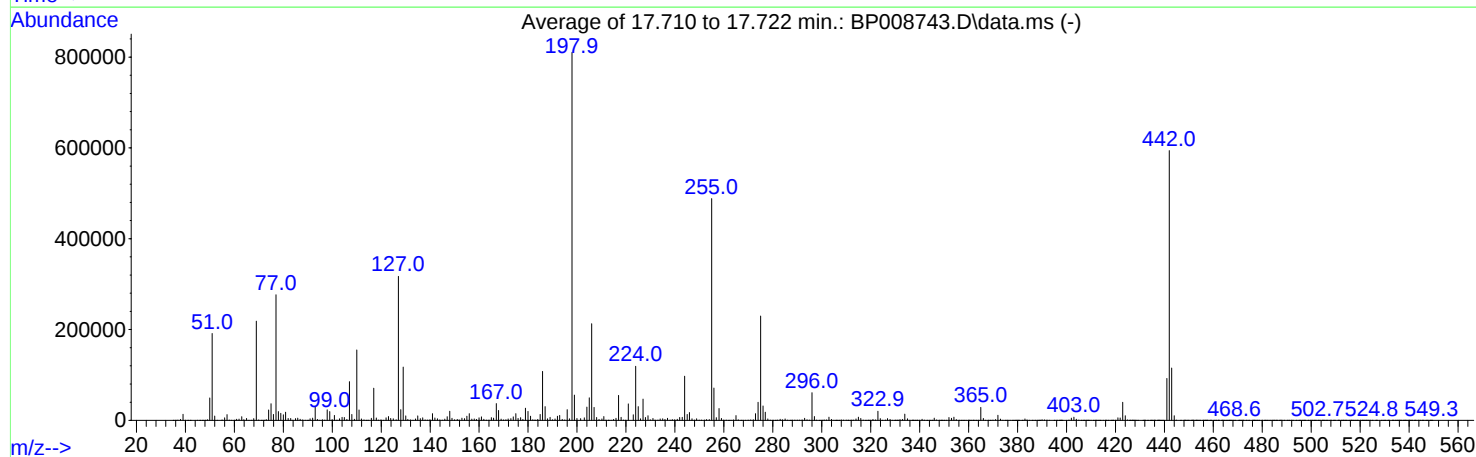


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011022\
 Data File : BP008743.D
 Acq On : 10 Jan 2022 10:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 07 07:45:52 2022

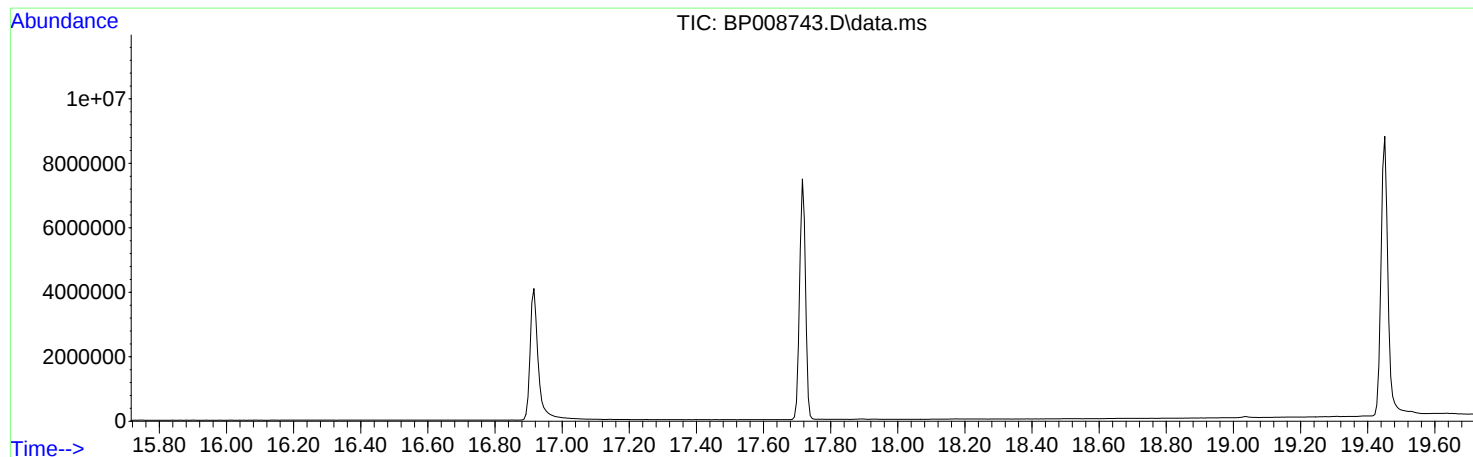




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.6	191395	PASS
68	69	0.00	2	1.7	3744	PASS
69	198	0.00	100	26.9	218306	PASS
70	69	0.00	2	0.5	1188	PASS
127	198	10	80	39.2	317239	PASS
197	198	0.00	2	0.4	3470	PASS
198	198	100	100	100.0	810075	PASS
199	198	5	9	6.9	55552	PASS
275	198	10	60	28.4	229739	PASS
365	198	1	100	3.5	28683	PASS
441	198	0.01	100	11.4	92244	PASS
442	442	100	100	100.0	593956	PASS
443	442	15	24	19.4	115112	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011022\
 Data File : BP008743.D
 Acq On : 10 Jan 2022 10:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 10 16:49:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 07 07:45:52 2022
 Response via : Initial Calibration

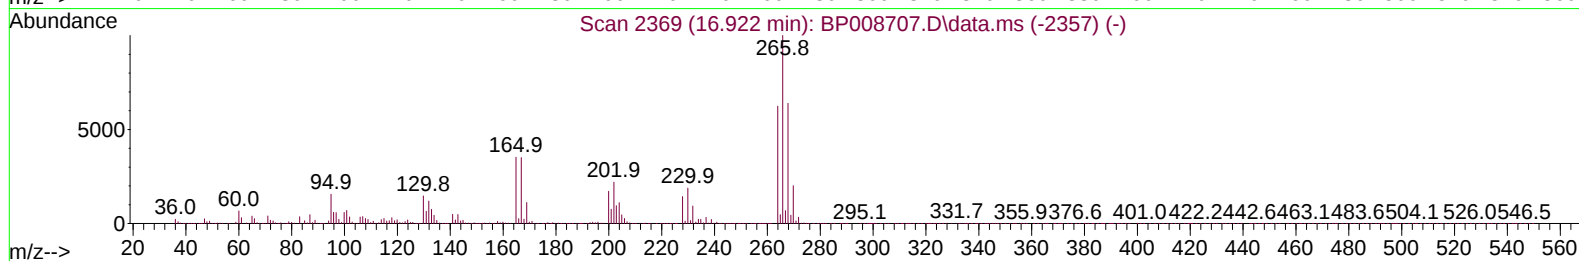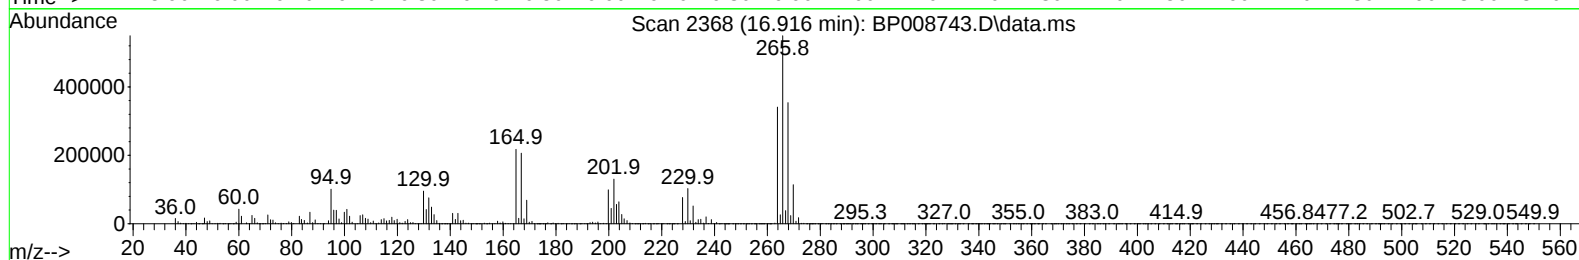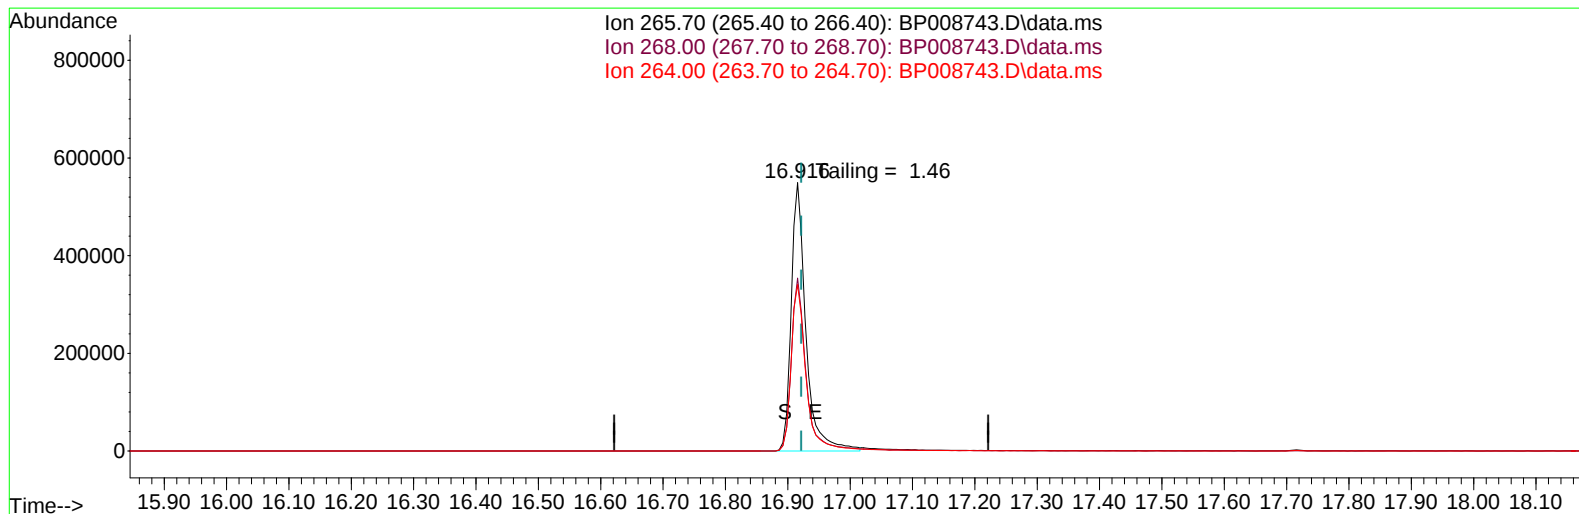

TIC: BP008743.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.006) 176016.36 ng




response 927250

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.45
264.00	62.90	62.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011022\
Data File : BP008743.D
Acq On : 10 Jan 2022 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 10 16:49:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 07 07:45:52 2022
Response via : Initial Calibration

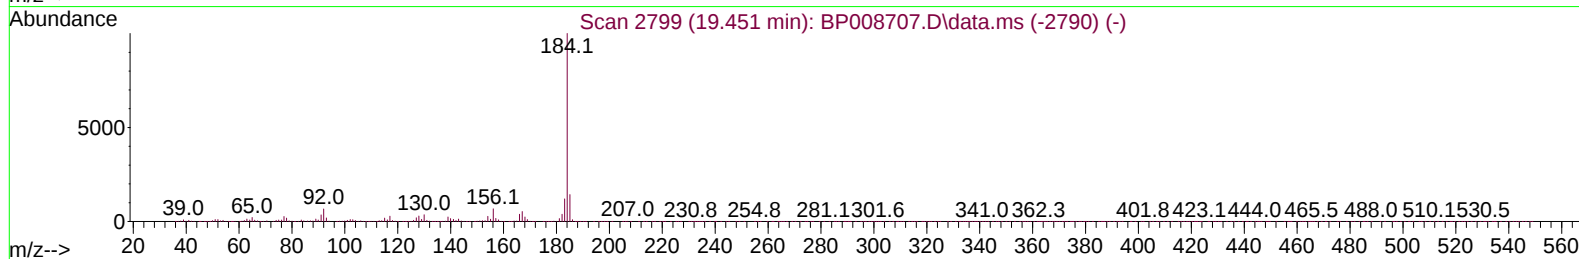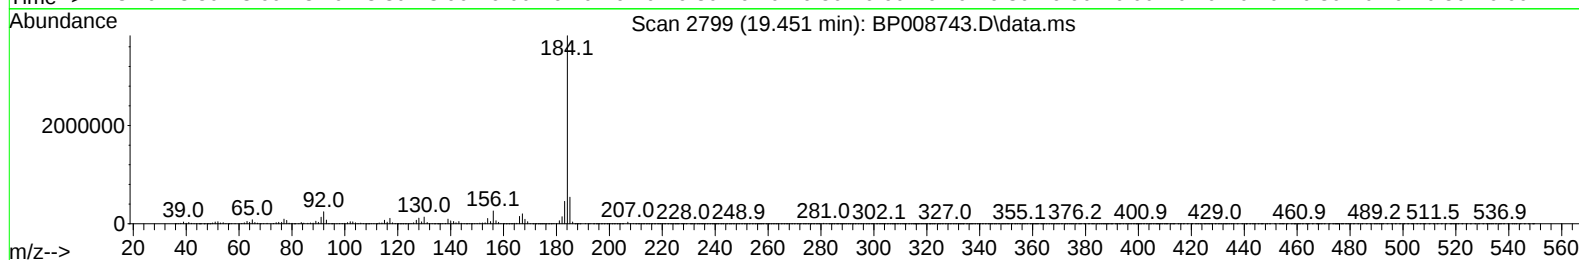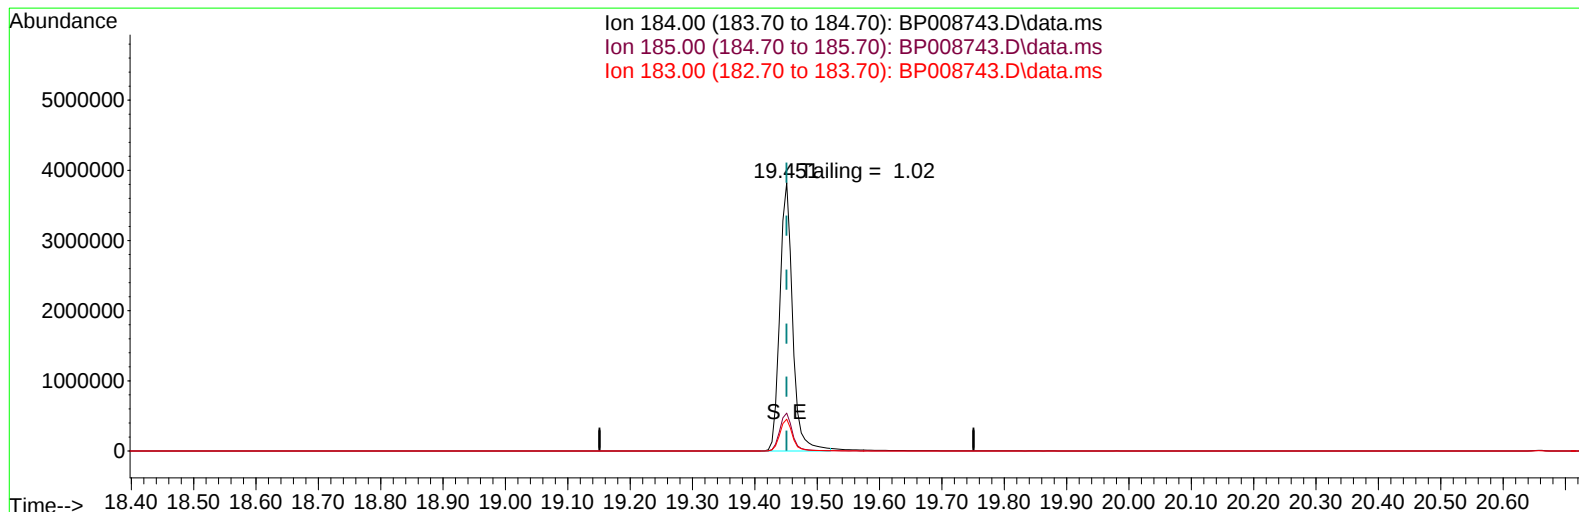

TIC: BP008743.D\data.ms

(77) Benzidine

19.451min (-0.000) 61214.45 ng

response 5542409

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.14
183.00	11.90	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/10/2022	BNA_P	BP008743.D
Compound Name	Response	Retention Time
DDT	2847304	20.65
DDD	26114	20.22
DDE	5021	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31135	2878439	1.08

Instrument :
BNA_P
ClientSampleId :
DFTPP