

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
 Data File : BP013422.D
 Acq On : 10 Jan 2023 11:22
 Operator : CG/JU
 Sample : 01050-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4493

Quant Time: Jan 10 11:47:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 06 01:03:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	370533	20.000	ng/u1	0.00
20) Naphthalene-d8	10.734	136	1519012	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.569	164	939770	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.328	188	2088976	20.000	ng/u1	0.00
79) Chrysene-d12	21.422	240	2092135	20.000	ng/u1	0.01
88) Perylene-d12	23.880	264	2308910	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	30540	3.204	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.081	99	599959	19.513	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.246	67	391700	20.194	ng/u1	0.00
11) 2-Chlorophenol-d4	7.452	132	475609	20.743	ng/u1	0.00
15) 4-Methylphenol-d8	8.634	113	434003	18.528	ng/u1	0.00
21) Nitrobenzene-d5	9.093	128	210401	19.453	ng/u1	0.00
24) 2-Nitrophenol-d4	9.816	143	235310	19.875	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.352	165	460694	19.525	ng/u1	0.00
31) 4-Chloroaniline-d4	10.875	131	469653	14.129	ng/u1	0.00
46) Dimethylphthalate-d6	13.975	166	1666384	24.338	ng/u1	0.00
49) Acenaphthylene-d8	14.263	160	1693622	22.346	ng/u1	0.00
54) 4-Nitrophenol-d4	14.769	143	216038	17.238	ng/u1	0.00
60) Fluorene-d10	15.563	176	1522830	25.180	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	205079	15.483	ng/u1	0.00
73) Anthracene-d10	17.428	188	2716705	29.423	ng/u1	0.00
81) Pyrene-d10	19.663	212	3368423	29.592	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.727	264	3369722	29.711	ng/u1	0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.310	149	3698004	63.378	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
Data File : BP013422.D
Acq On : 10 Jan 2023 11:22
Operator : CG/JU
Sample : 01050-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4493

Quant Time: Jan 10 11:47:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 06 01:03:32 2023
Response via : Initial Calibration

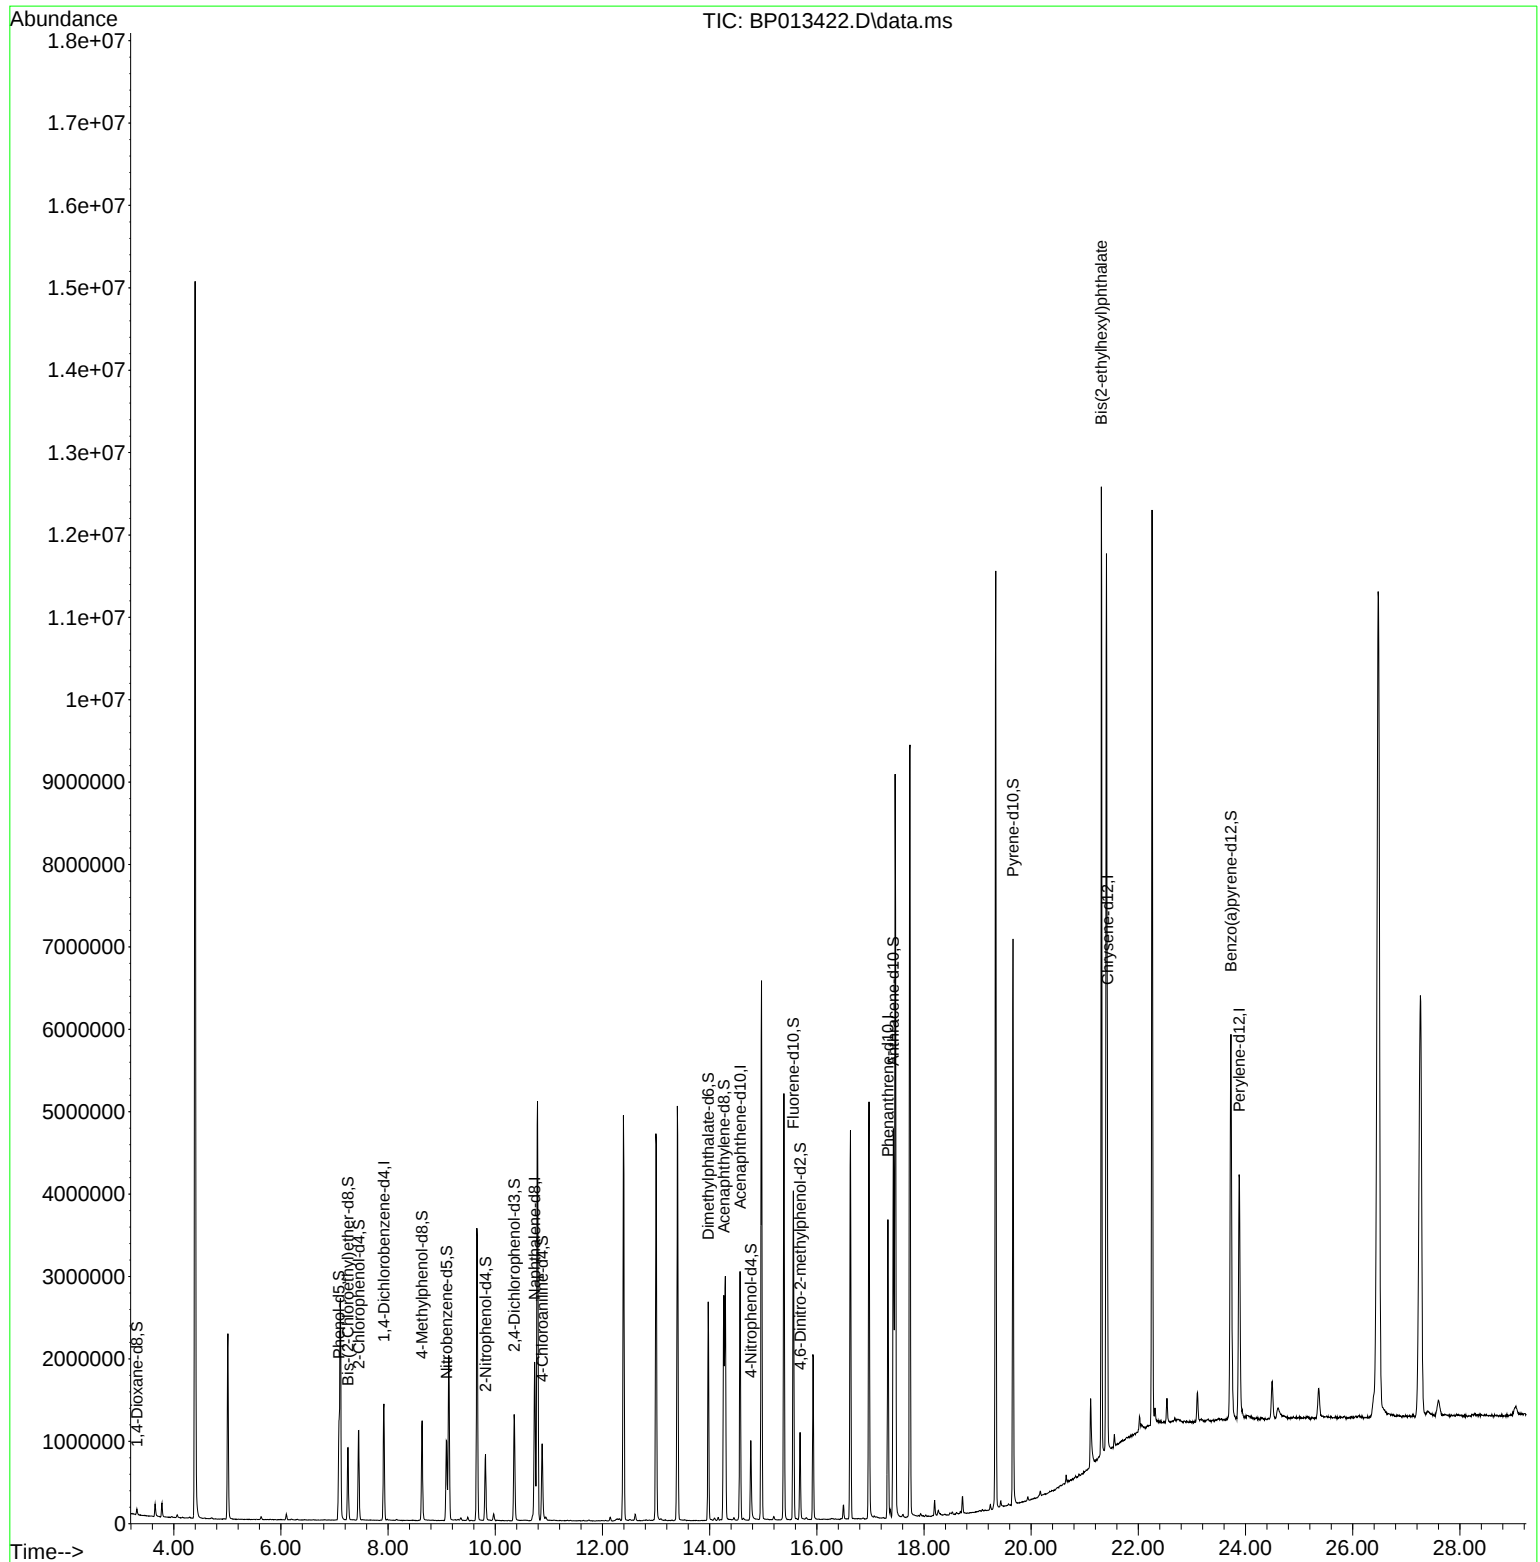

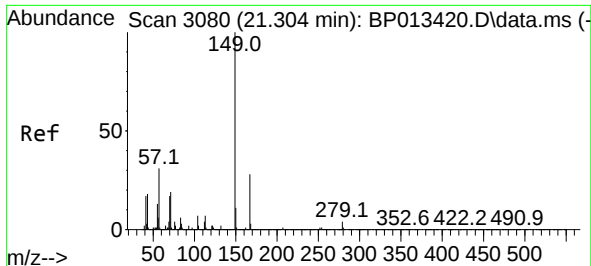

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 63.378 ng/ul
 RT: 21.310 min Scan# 3081
 Delta R.T. 0.006 min
 Lab File: BP013422.D
 Acq: 10 Jan 2023 11:22

Instrument :
 BNA_P
 ClientSampleId :
 A4493

Tgt Ion:149 Resp: 3698004
 Ion Ratio Lower Upper
 149 100
 167 27.8 22.2 33.4
 279 4.2 3.5 5.3

