

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
 Data File : BP013431.D
 Acq On : 10 Jan 2023 16:59
 Operator : CG/JU
 Sample : PB150112BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.310	17	21	29	rVB	136010	195413	1.65%	0.158%
2	3.734	90	93	116	rBV	1760889	2558237	21.60%	2.063%
3	4.063	145	149	155	rVB	39185	52442	0.44%	0.042%
4	7.075	654	661	673	rBV	1976420	3021263	25.51%	2.437%
5	7.245	683	690	701	rVB	1621257	2543984	21.48%	2.052%
6	7.445	717	724	731	rBV	1978922	3108120	26.25%	2.507%
7	7.916	797	804	812	rBV	2098555	3230601	27.28%	2.606%
8	8.622	917	924	938	rBV	2290212	3678566	31.07%	2.967%
9	9.081	993	1002	1015	rBV	1830106	3002901	25.36%	2.422%
10	9.810	1116	1126	1137	rBV	1498381	2512806	21.22%	2.027%
11	10.345	1209	1217	1227	rBV	2322481	3841416	32.44%	3.098%
12	10.728	1274	1282	1290	rBV	2846660	4628081	39.08%	3.733%
13	10.869	1298	1306	1320	rBV	2152380	3790509	32.01%	3.057%
14	11.392	1390	1395	1403	rVB	7237	17422	0.15%	0.014%
15	12.316	1546	1552	1559	rBV3	38304	66093	0.56%	0.053%
16	13.527	1755	1758	1763	rBV7	7958	13086	0.11%	0.011%
17	13.969	1825	1833	1848	rBV	4327901	5788599	48.89%	4.669%
18	14.080	1848	1852	1857	rVB8	8294	13648	0.12%	0.011%
19	14.257	1874	1882	1899	rBV	4505783	6616279	55.88%	5.337%
20	14.563	1925	1934	1941	rBV	4188849	6160194	52.02%	4.969%
21	14.763	1960	1968	1982	rBV	1494761	2409268	20.35%	1.943%
22	14.969	2001	2003	2011	rVB8	11630	22266	0.19%	0.018%
23	15.557	2096	2103	2116	rBV	5950911	8459896	71.44%	6.824%
24	15.680	2117	2124	2138	rVV	2018285	2739733	23.14%	2.210%
25	15.798	2140	2144	2150	rVB2	27782	44910	0.38%	0.036%
26	16.339	2231	2236	2239	rBV7	8402	12455	0.11%	0.010%
27	16.998	2344	2348	2352	rVB7	10002	14499	0.12%	0.012%
28	17.098	2363	2365	2370	rVB3	8563	14163	0.12%	0.011%
29	17.321	2396	2403	2410	rBV	5032824	7238605	61.13%	5.839%
30	17.421	2413	2420	2434	rBV	6417648	9124905	77.06%	7.360%
31	19.233	2724	2728	2733	rVB2	79882	106915	0.90%	0.086%
32	19.298	2735	2739	2743	rBV	76653	103167	0.87%	0.083%
33	19.657	2794	2800	2811	rBV	8090709	10967191	92.62%	8.846%
34	21.409	3093	3098	3110	rBV	6079513	7834639	66.16%	6.319%
35	23.709	3482	3489	3505	rVB	5605222	11841205	100.00%	9.551%
36	23.868	3510	3516	3532	rVB2	3970473	8204452	69.29%	6.618%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
Data File : BP013431.D
Acq On : 10 Jan 2023 16:59
Operator : CG/JU
Sample : PB150112BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK112

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Title : SVOA CALIBRATION




Sum of corrected areas: 123977929

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
Data File : BP013431.D
Acq On : 10 Jan 2023 16:59
Operator : CG/JU
Sample : PB150112BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

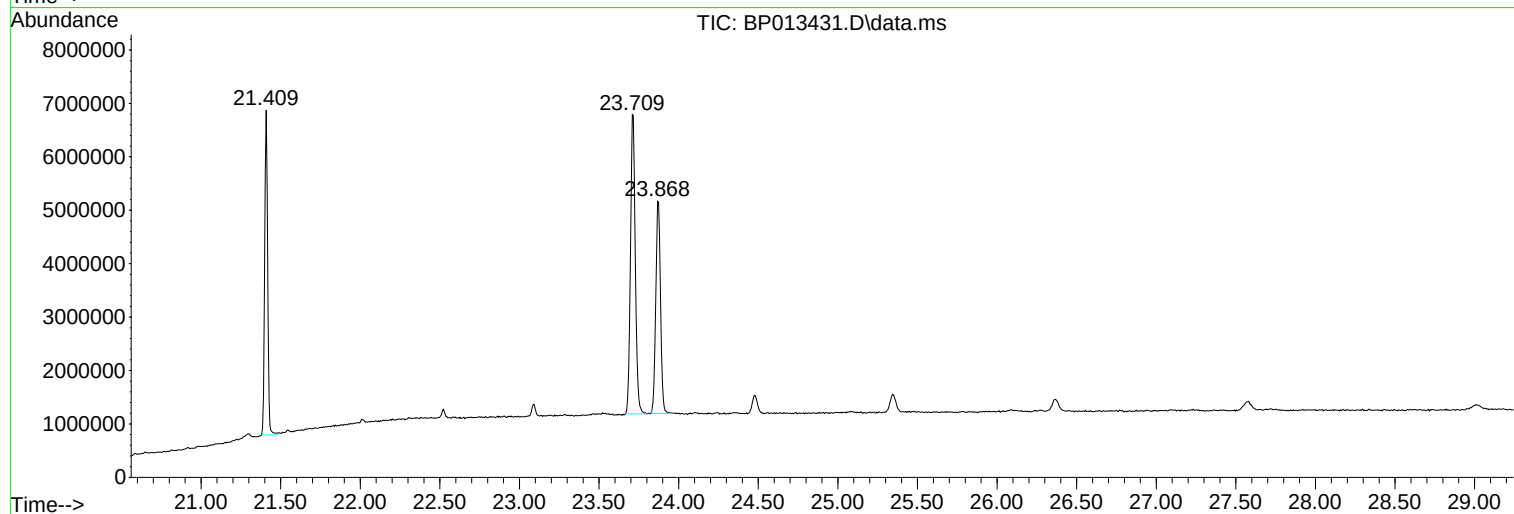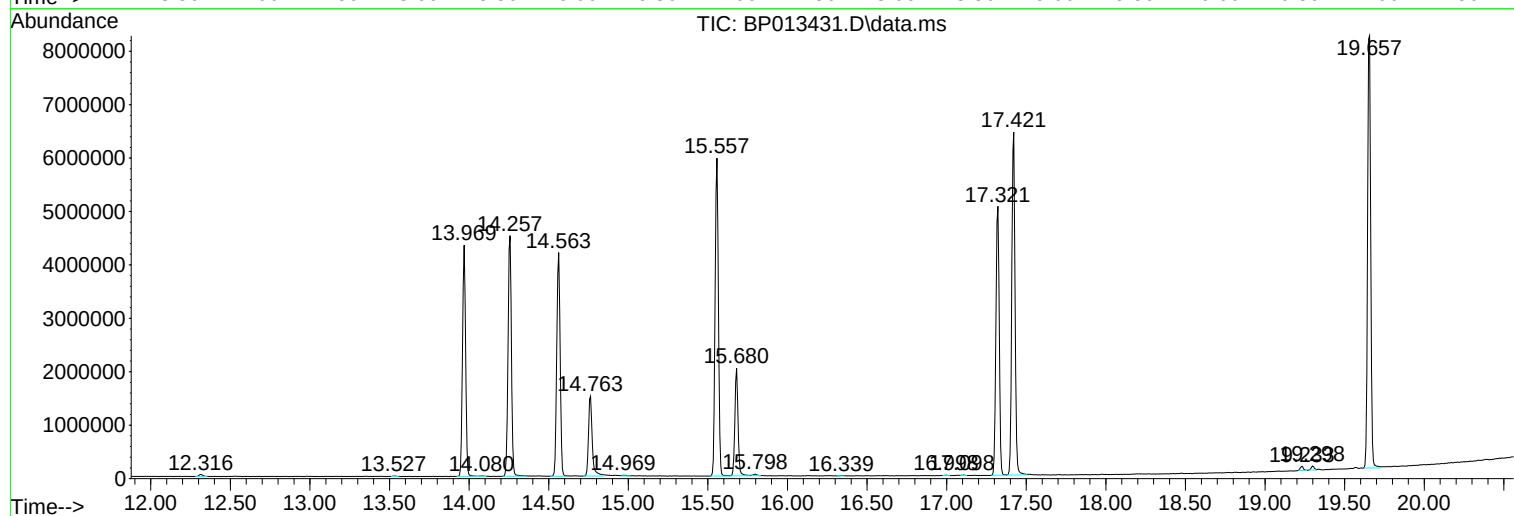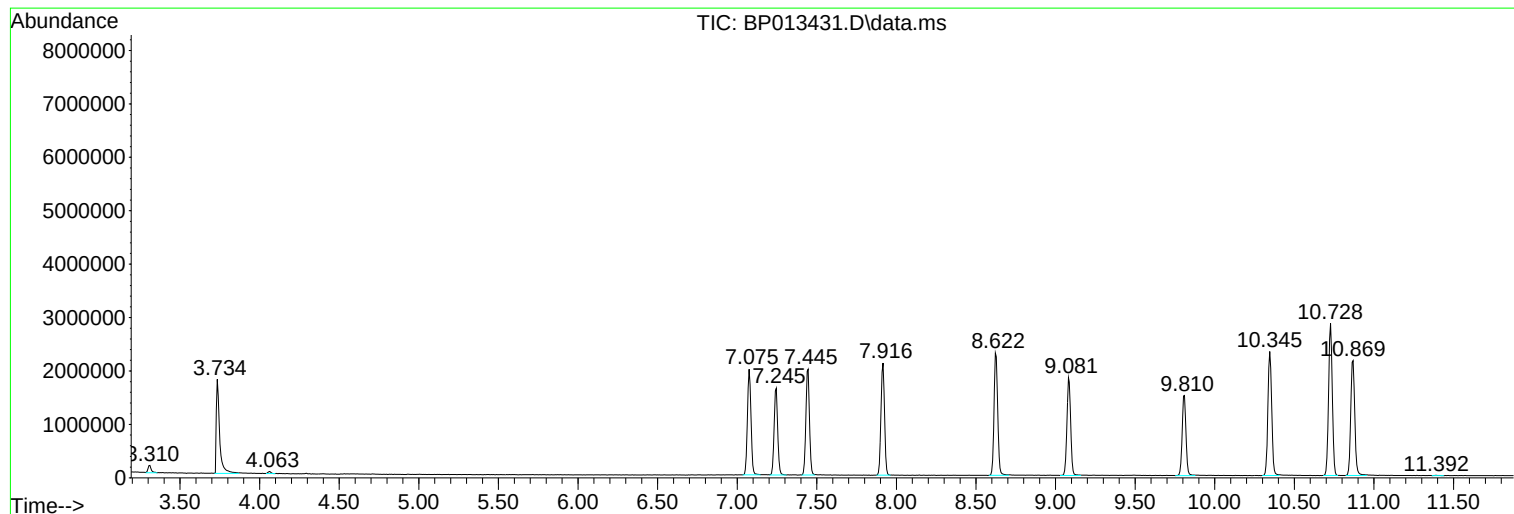

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
Data File : BP013431.D
Acq On : 10 Jan 2023 16:59
Operator : CG/JU
Sample : PB150112BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
Data File : BP013431.D
Acq On : 10 Jan 2023 16:59
Operator : CG/JU
Sample : PB150112BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------