

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
 Data File : BP013433.D
 Acq On : 10 Jan 2023 18:08
 Operator : CG/JU
 Sample : PB150072BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK072

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	3	6	17	rVB	5600937	5555396	30.23%	6.575%
2	3.569	62	65	71	rVB	166160	191259	1.04%	0.226%
3	4.058	144	148	155	rVB	89909	111466	0.61%	0.132%
4	5.005	304	309	318	rVB	111154	171436	0.93%	0.203%
5	7.916	796	804	815	rBV	4611578	7320422	39.83%	8.664%
6	10.728	1273	1282	1299	rBV	6237253	10243151	55.73%	12.124%
7	14.563	1925	1934	1945	rBV	10086717	14501341	78.90%	17.164%
8	17.104	2362	2366	2372	rVB	23233	31298	0.17%	0.037%
9	17.322	2396	2403	2417	rBV	13032498	18378789	100.00%	21.753%
10	19.569	2782	2785	2790	rBV4	40097	43814	0.24%	0.052%
11	21.410	3092	3098	3109	rBV	11886219	15145768	82.41%	17.927%
12	23.868	3509	3516	3532	rVB2	6282737	12793922	69.61%	15.143%




Sum of corrected areas: 84488062

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
Data File : BP013433.D
Acq On : 10 Jan 2023 18:08
Operator : CG/JU
Sample : PB150072BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

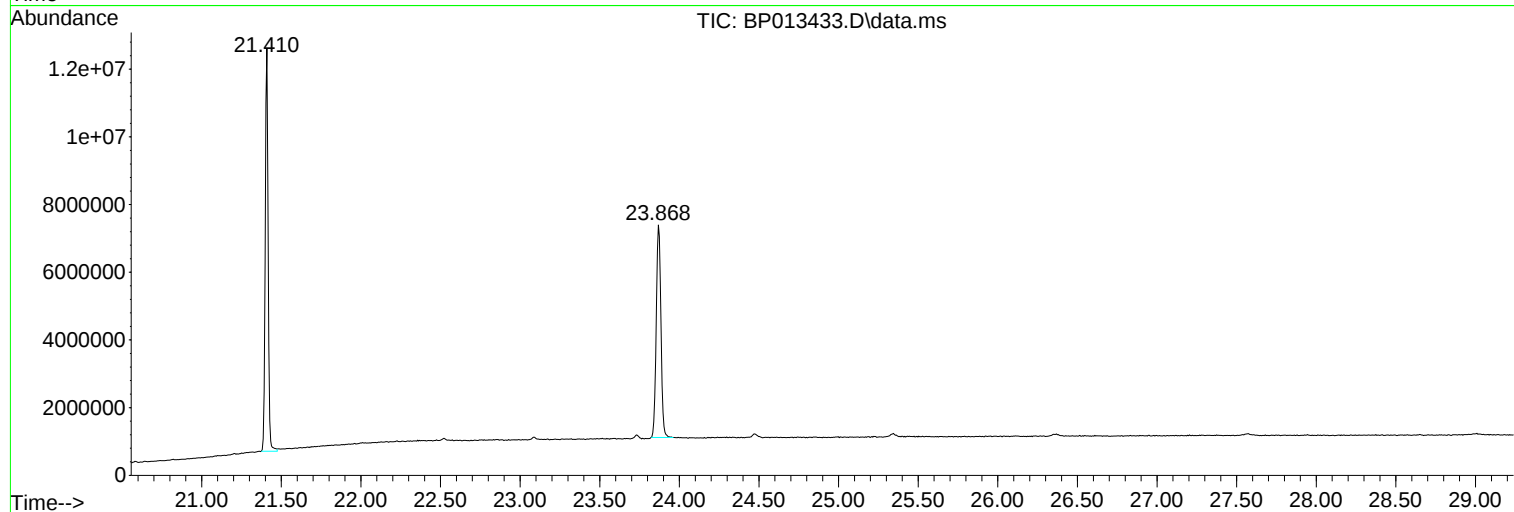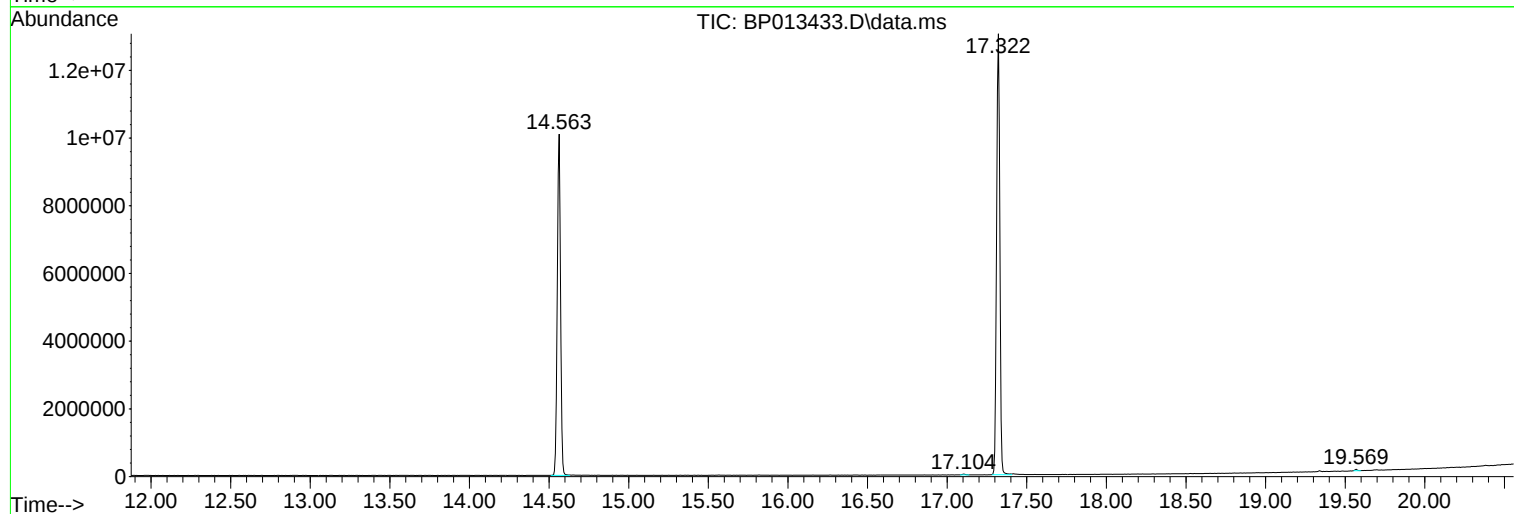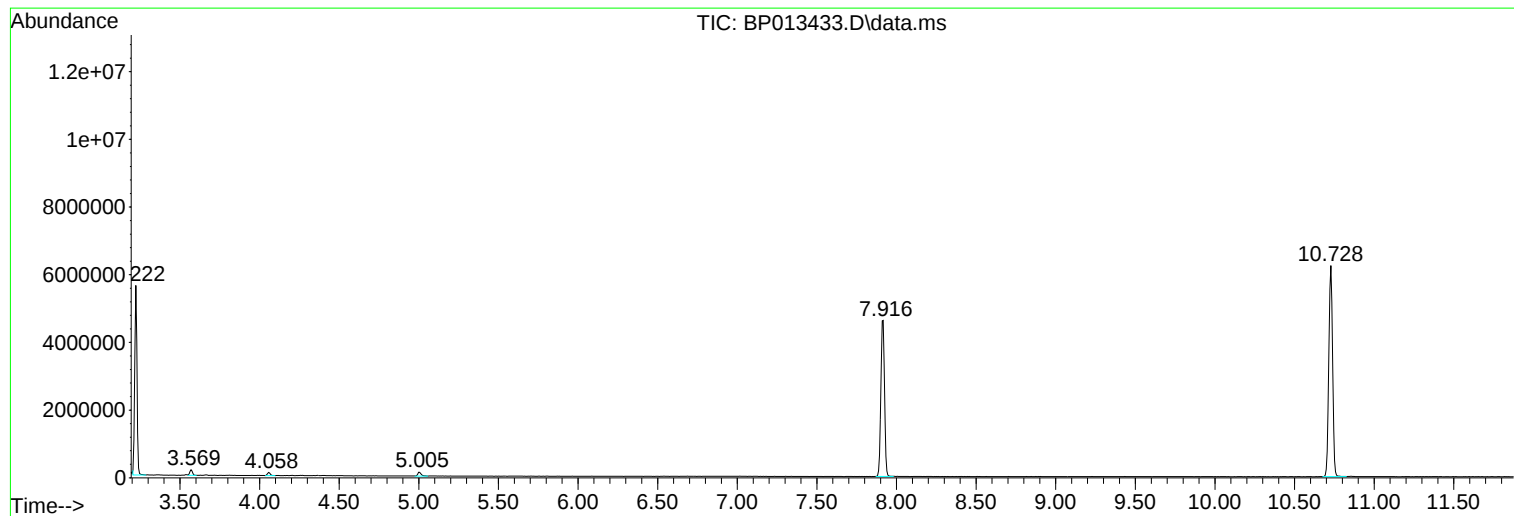

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
Data File : BP013433.D
Acq On : 10 Jan 2023 18:08
Operator : CG/JU
Sample : PB150072BL
Misc :
ALS Vial : 14 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
3.222	15.18 ng/ul	5555400	1,4-Dichlorobenzene-d4		7.916	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Heptane		100	C7H16	000142-82-5	94
2	Heptane		100	C7H16	000142-82-5	94
3	Heptane		100	C7H16	000142-82-5	91
4	Heptane		100	C7H16	000142-82-5	83
5	Oxalic acid, isobutyl pentyl ester		216	C11H20O4	1000309-37-0	64

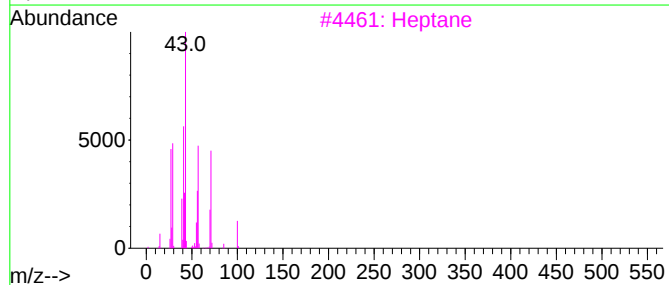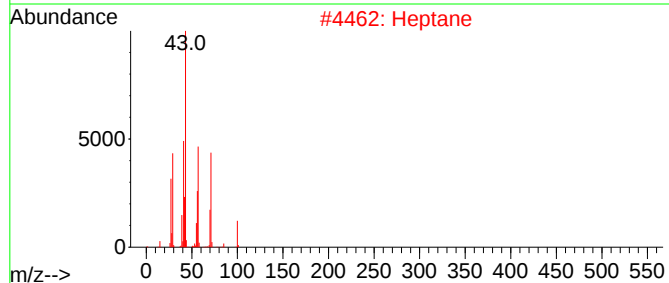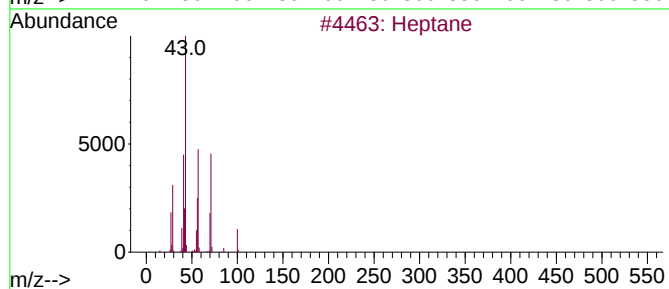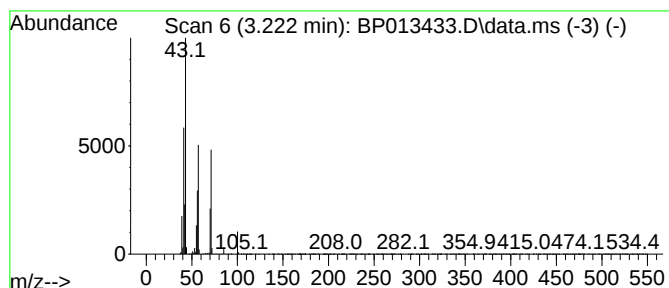

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011023\
Data File : BP013433.D
Acq On : 10 Jan 2023 18:08
Operator : CG/JU
Sample : PB150072BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK072

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.222	15.2	ng/u1	5555400	1	7.916	7320420	20.0