


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011122\
 Data File : BP008762.D
 Acq On : 11 Jan 2022 11:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 12 00:18:56 2022

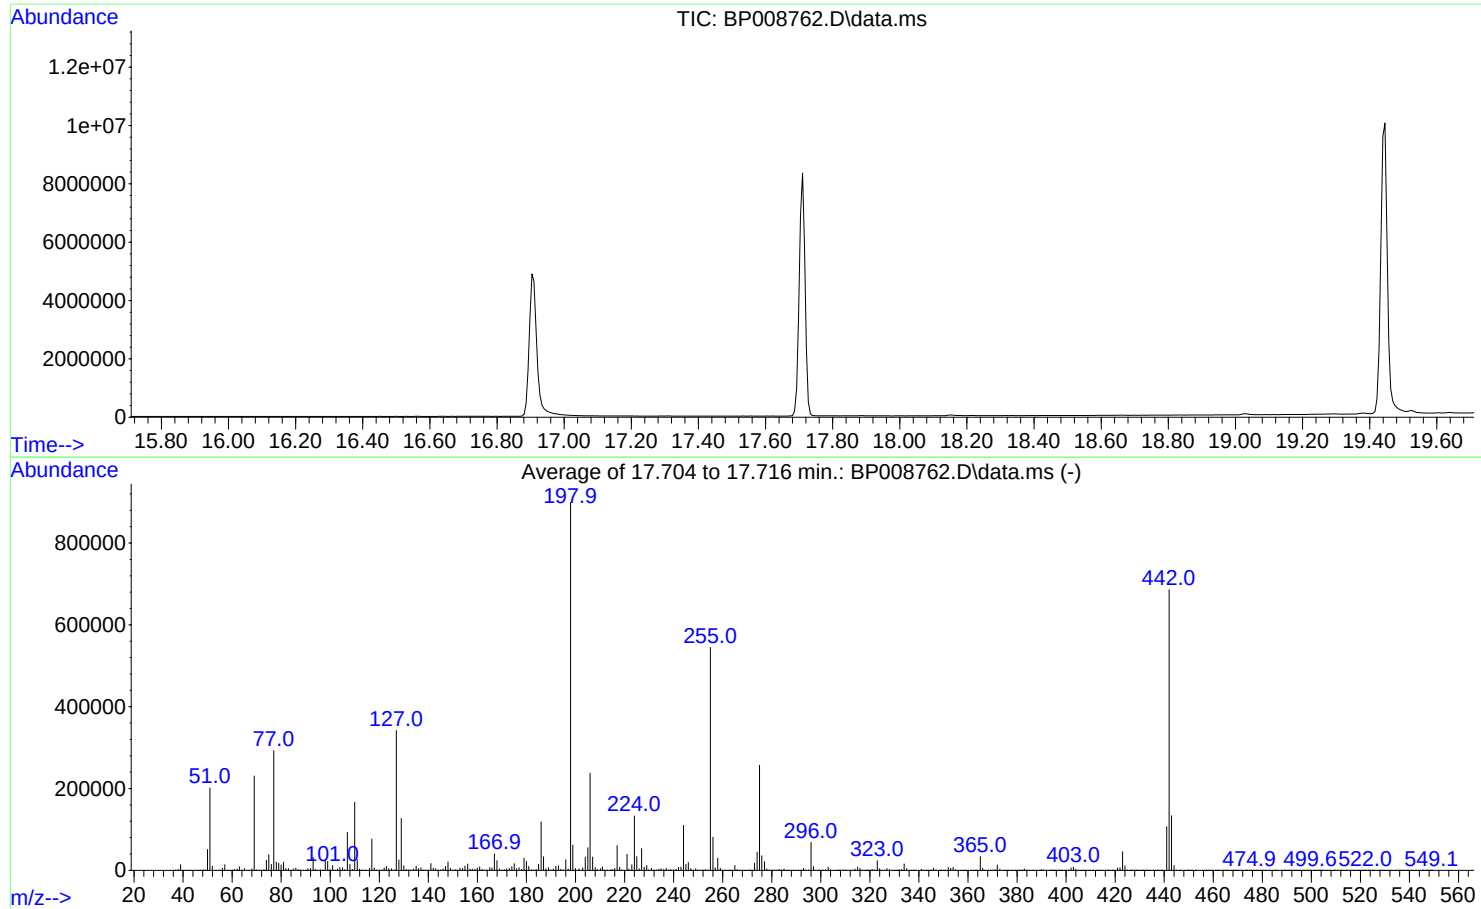




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	201340	PASS
68	69	0.00	2	1.6	3691	PASS
69	198	0.00	100	25.7	230834	PASS
70	69	0.00	2	0.5	1189	PASS
127	198	10	80	38.0	341664	PASS
197	198	0.00	2	0.4	3265	PASS
198	198	100	100	100.0	899094	PASS
199	198	5	9	6.9	61947	PASS
275	198	10	60	28.6	256853	PASS
365	198	1	100	3.7	33486	PASS
441	198	0.01	100	11.9	106728	PASS
442	442	100	100	100.0	685973	PASS
443	442	15	24	19.4	133235	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011122\
 Data File : BP008762.D
 Acq On : 11 Jan 2022 11:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 12 00:33:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 12 00:18:56 2022
 Response via : Initial Calibration

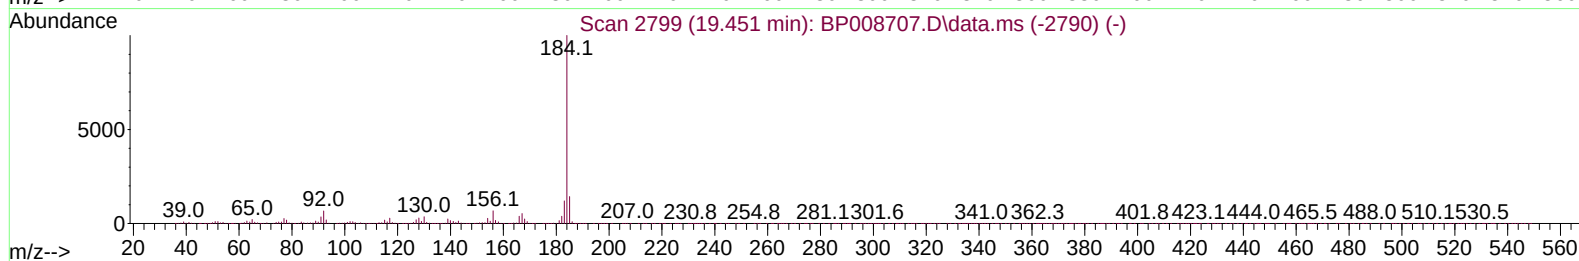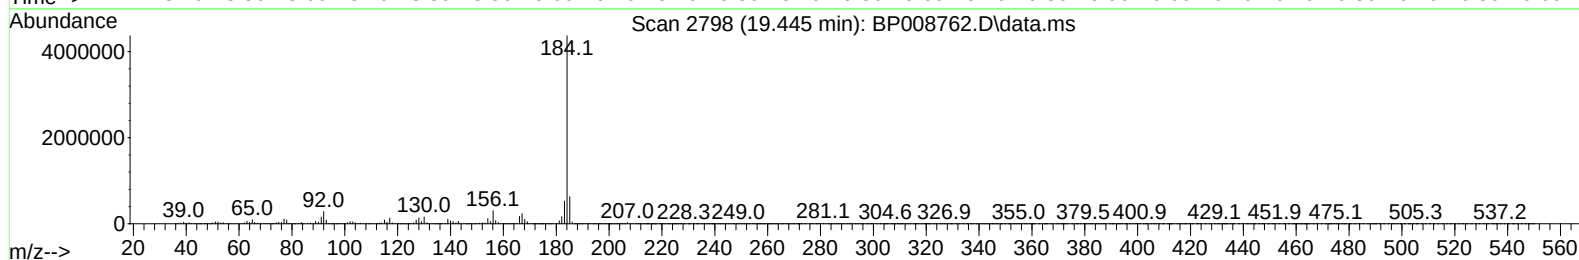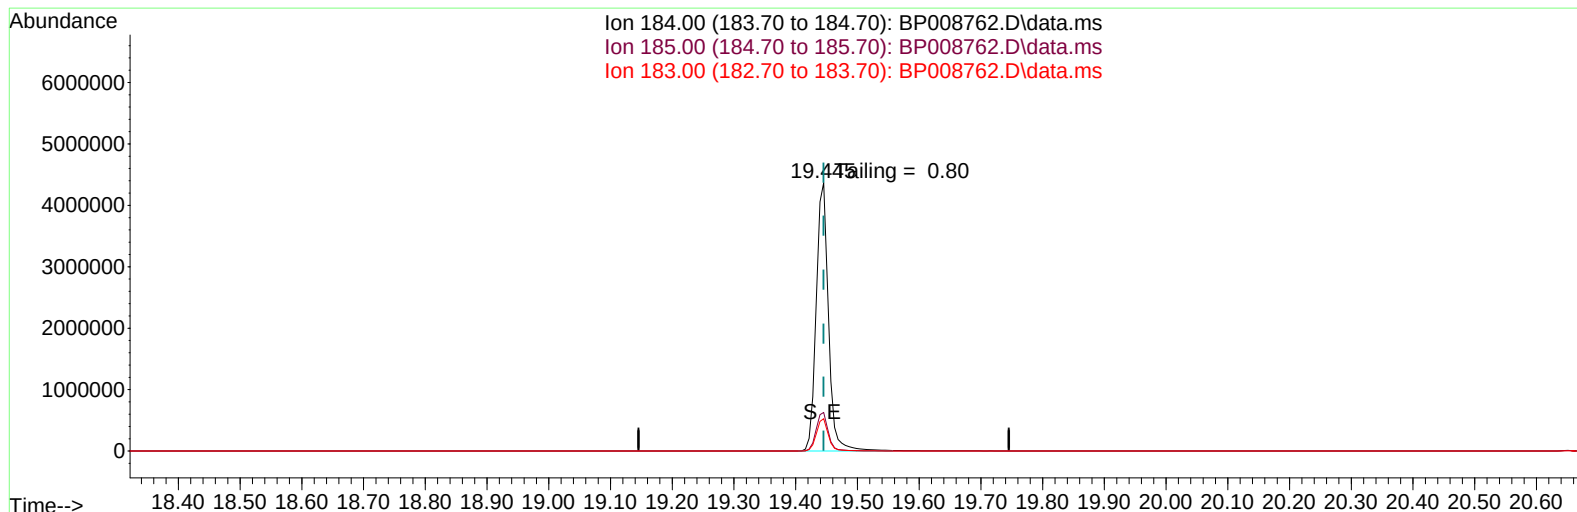

TIC: BP008762.D\data.ms

(77) Benzidine

19.445min (-0.000) 72511.16 ng




response 6065695

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.38
183.00	11.90	12.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011122\
Data File : BP008762.D
Acq On : 11 Jan 2022 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 12 00:33:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 12 00:18:56 2022
Response via : Initial Calibration

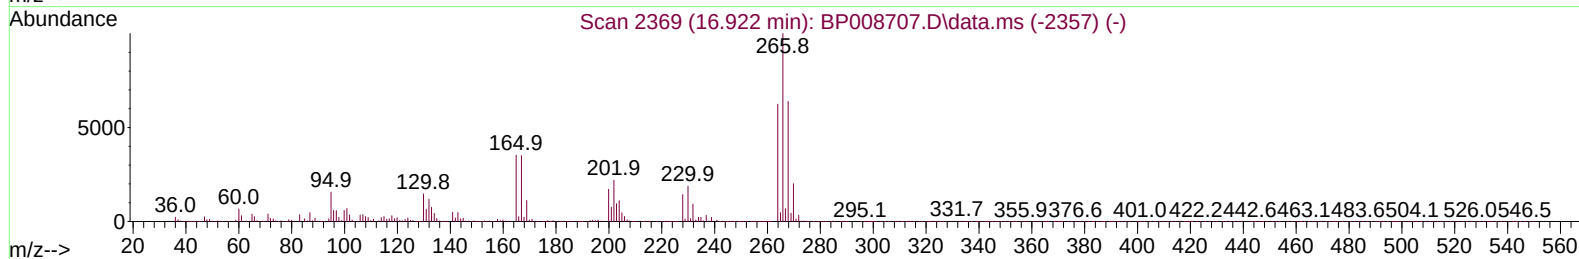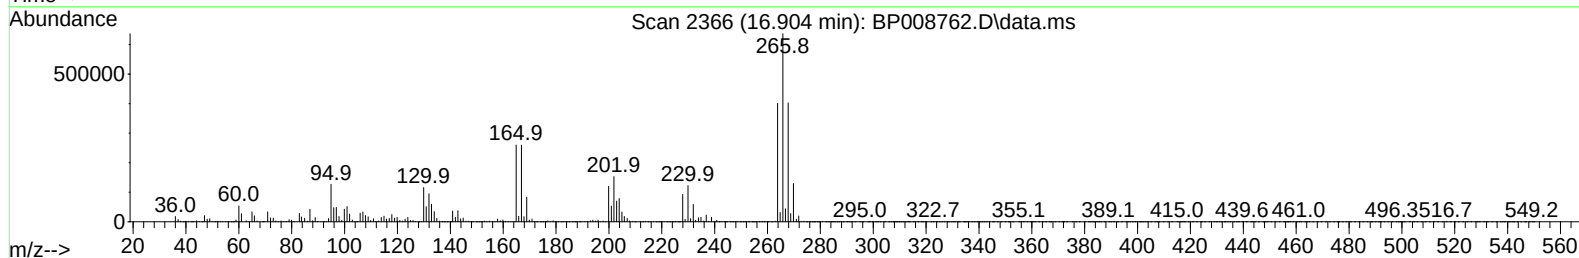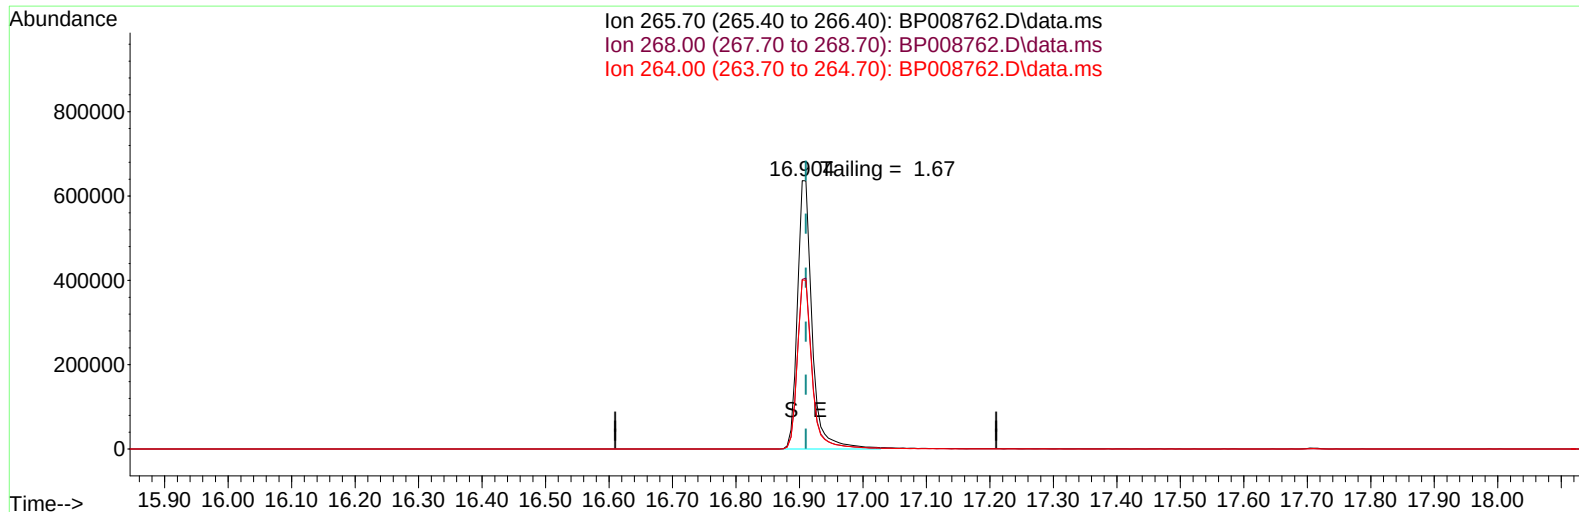

TIC: BP008762.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.006) 565098.53 ng

response 1039253

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.21
264.00	62.90	63.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/11/2022	BNA_P	<u>BP008762.D</u>
Compound Name	Response	Retention Time
DDT	3062712	20.651
DDD	40939	20.216
DDE	5105	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46044	3108756	1.48

Instrument :
BNA_P
ClientSampleId :
DFTPP