

Data File : BP001545.D

Acq On : 08 Jan 2020 09:13

Operator : JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1



Quant Time: Jan 09 05:52:35 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jan 08 15:02:19 2020

Response via : Initial Calibration

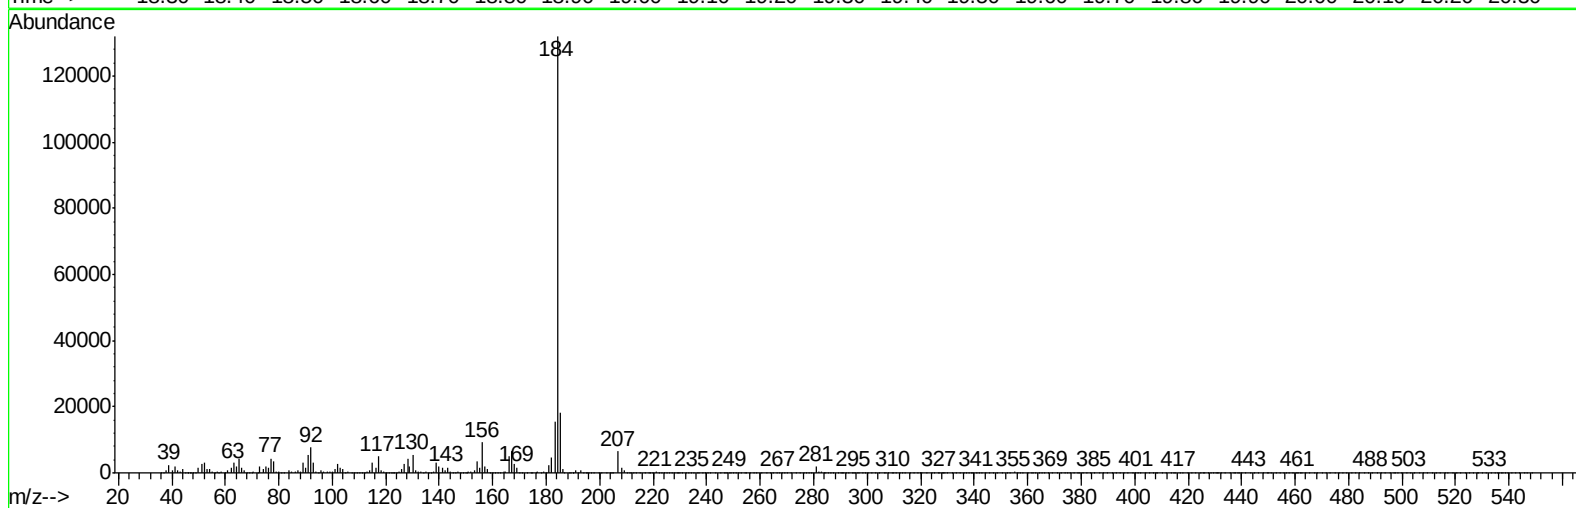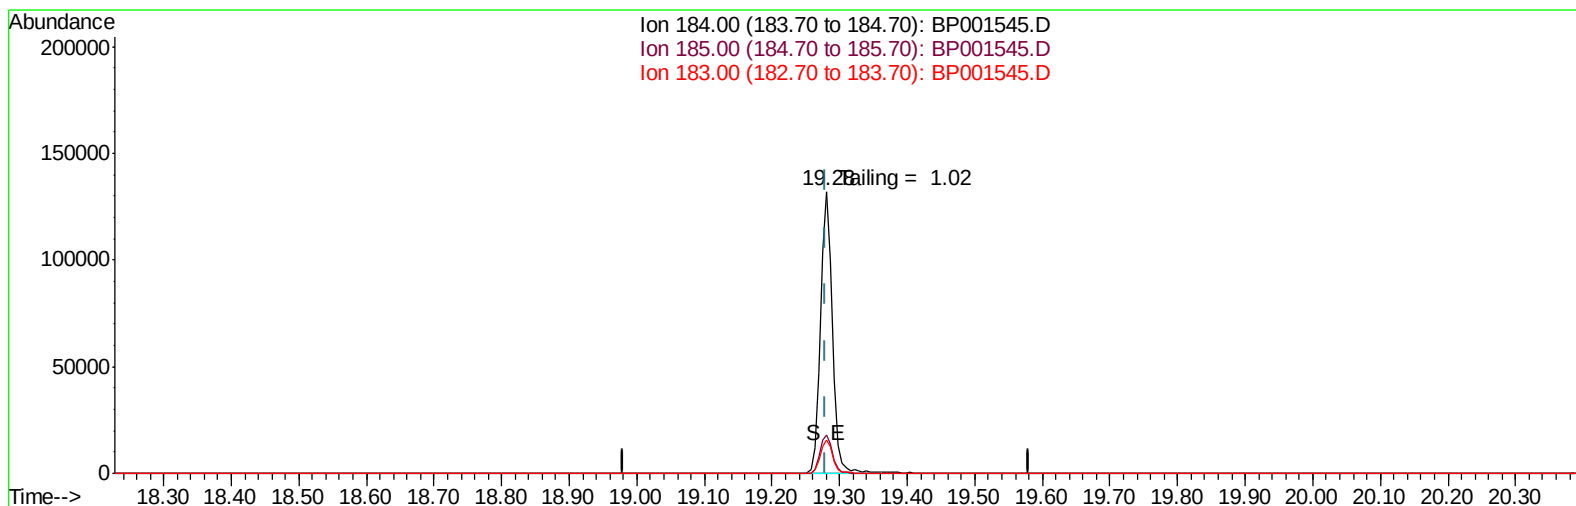

TIC: BP001545.D

(77) Benzidine

19.281min (+0.000) 520853.06ng

response 166501

Ion	Exp%	Act%
184.00	100	100
185.00	13.30	13.69
183.00	11.70	11.75
0.00	0.00	0.00